
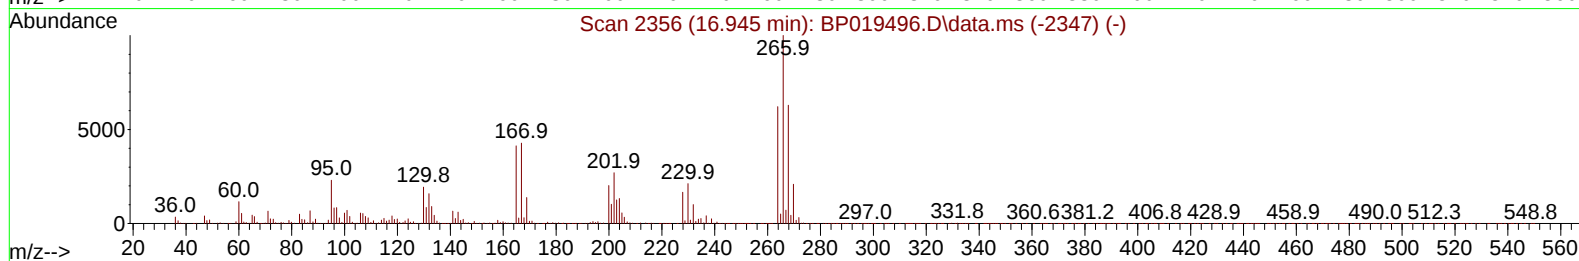
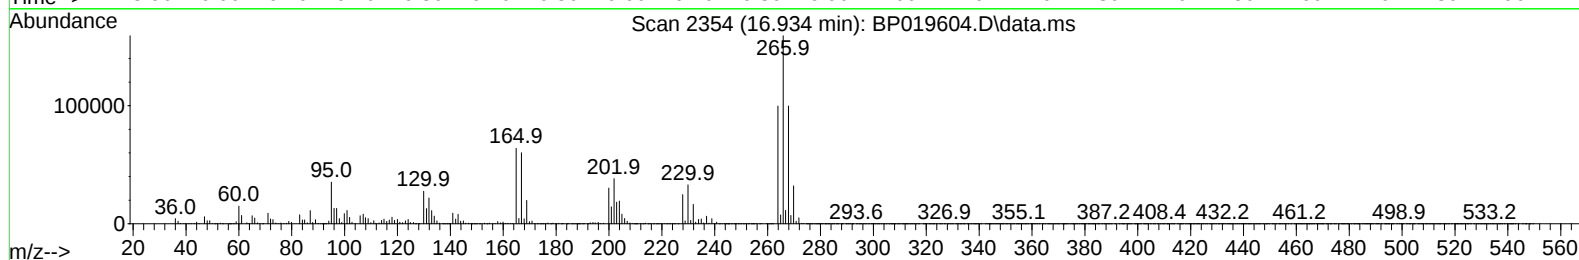


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020824\
Data File : BP019604.D
Acq On : 08 Feb 2024 11:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 13:04:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

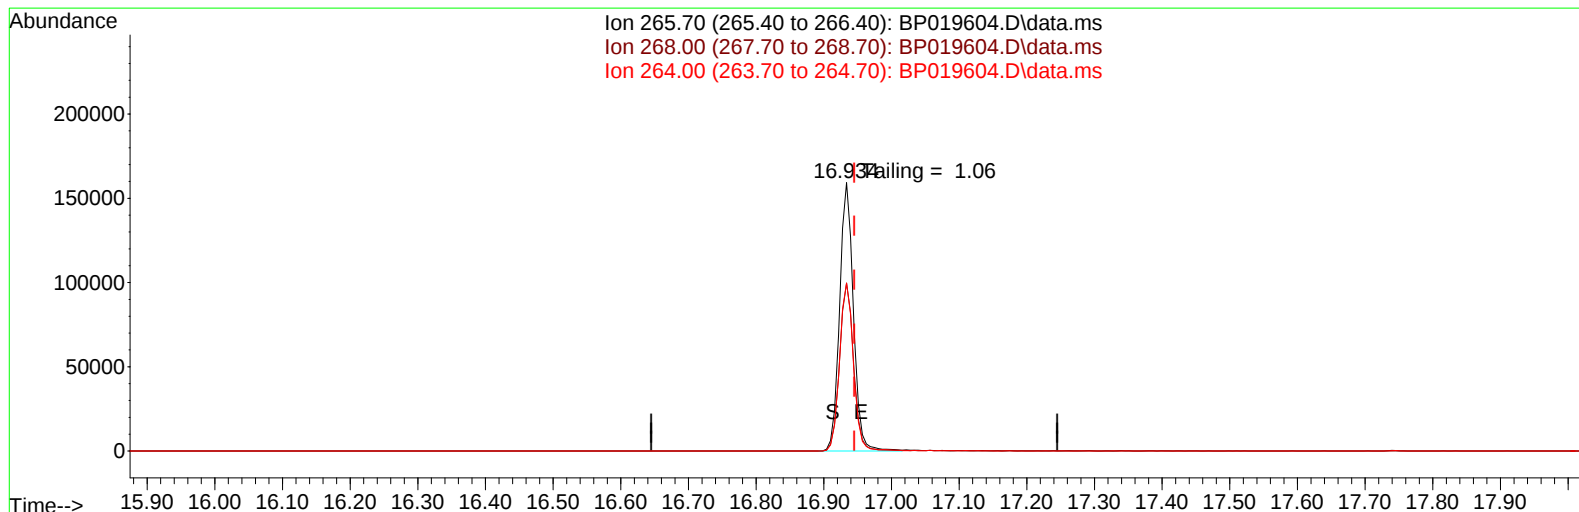

TIC: BP019604.D\data.ms

(70) Pentachlorophenol (C)




16.934min (-0.011) 318481.05 ng

response 225839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.64
264.00	62.10	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020824\
Data File : BP019604.D
Acq On : 08 Feb 2024 11:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 13:04:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

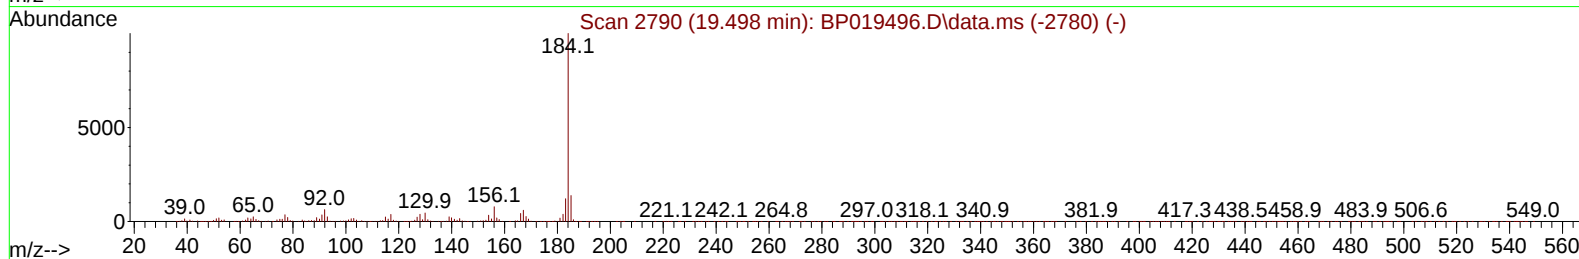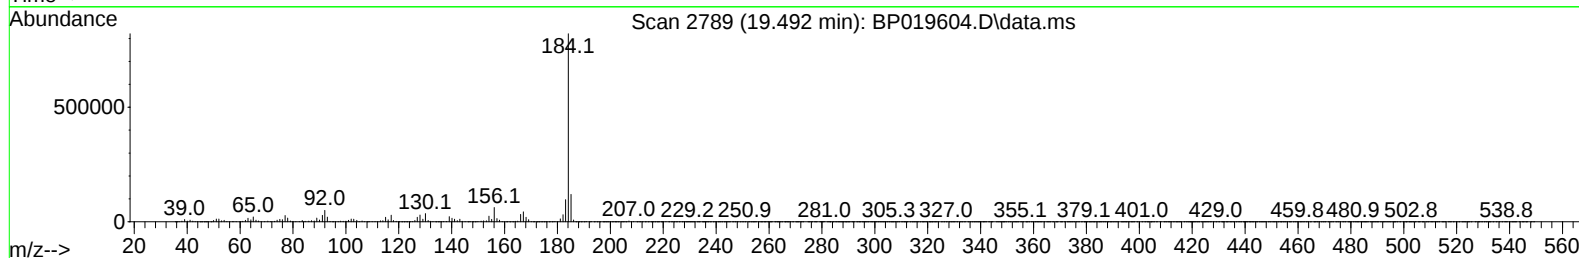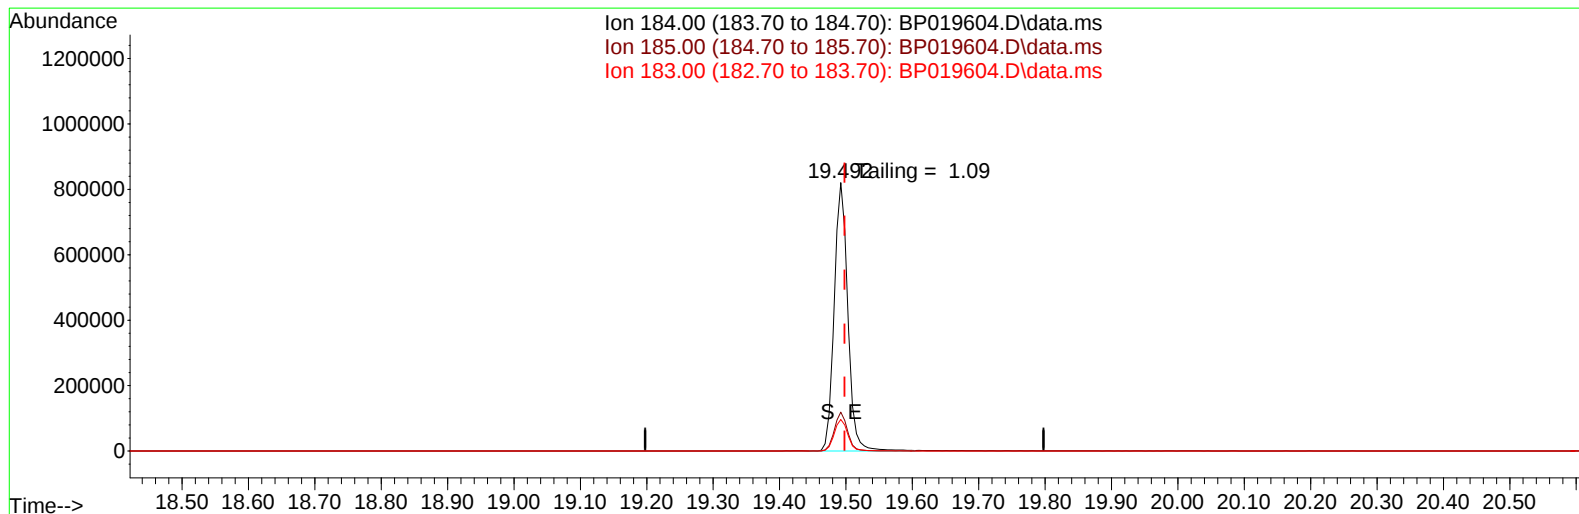

TIC: BP019604.D\data.ms

(77) Benzidine**19.492min (-0.006) 46147.84 ng****response 1169335**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.52
183.00	12.10	11.74
0.00	0.00	0.00