


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020824\
Data File : BP019604.D
Acq On : 08 Feb 2024 11:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

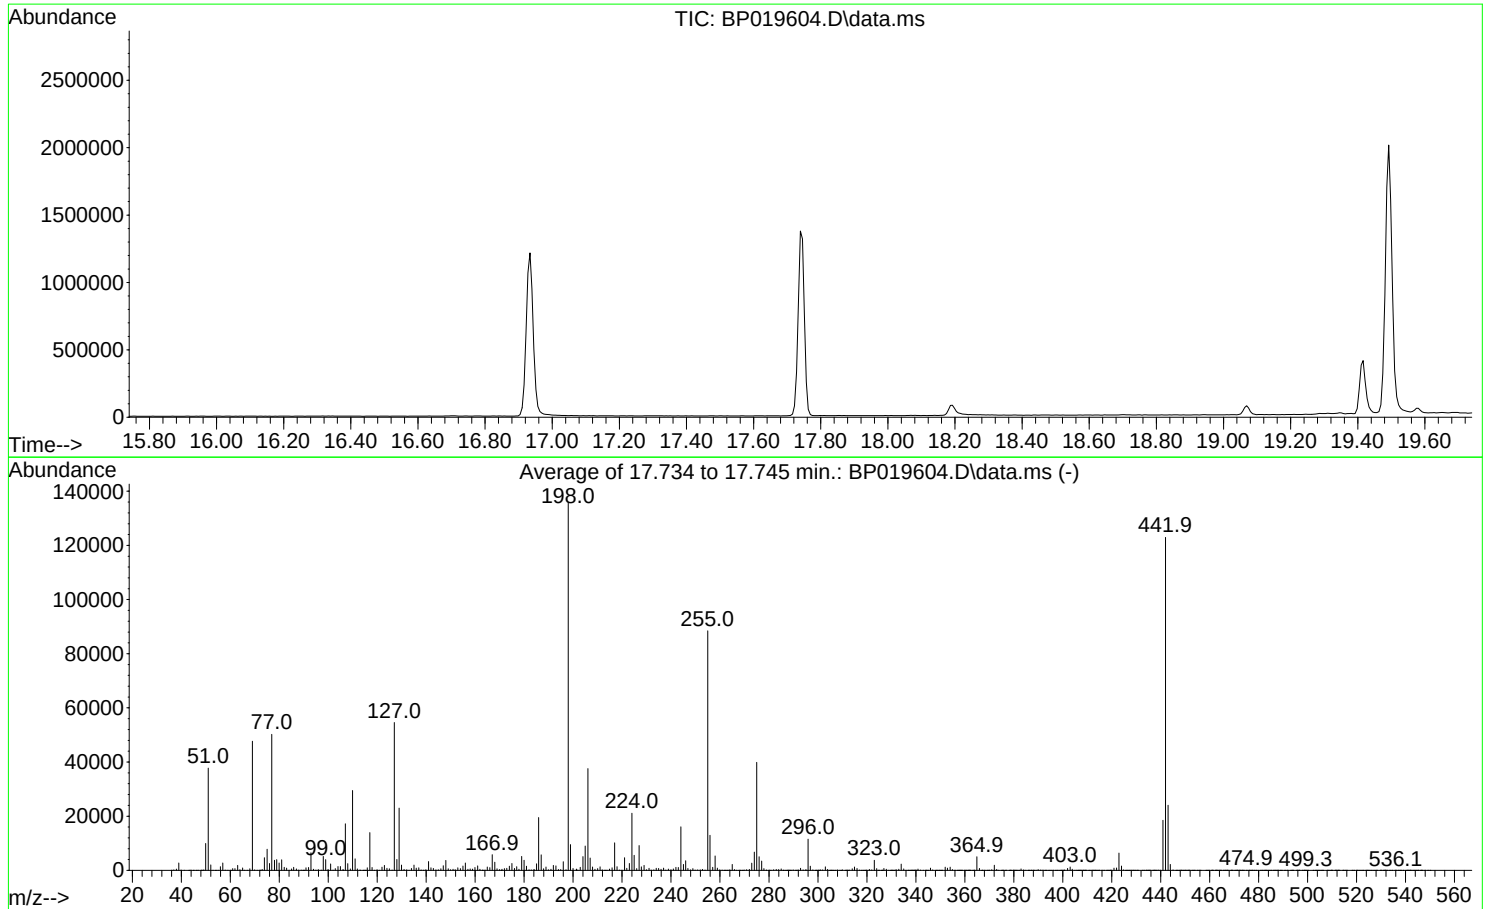




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	37750	PASS
68	69	0.00	2	1.3	606	PASS
69	198	0.00	100	35.1	47693	PASS
70	69	0.00	2	0.4	206	PASS
127	198	10	80	40.2	54590	PASS
197	198	0.00	2	0.2	264	PASS
198	198	100	100	100.0	135836	PASS
199	198	5	9	7.0	9491	PASS
275	198	10	60	29.3	39866	PASS
365	198	1	100	3.7	5054	PASS
441	198	0.01	100	13.6	18516	PASS
442	442	100	100	100.0	122978	PASS
443	442	15	24	19.5	24025	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020824\
Data File : BP019604.D
Acq On : 08 Feb 2024 11:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 08 13:04:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

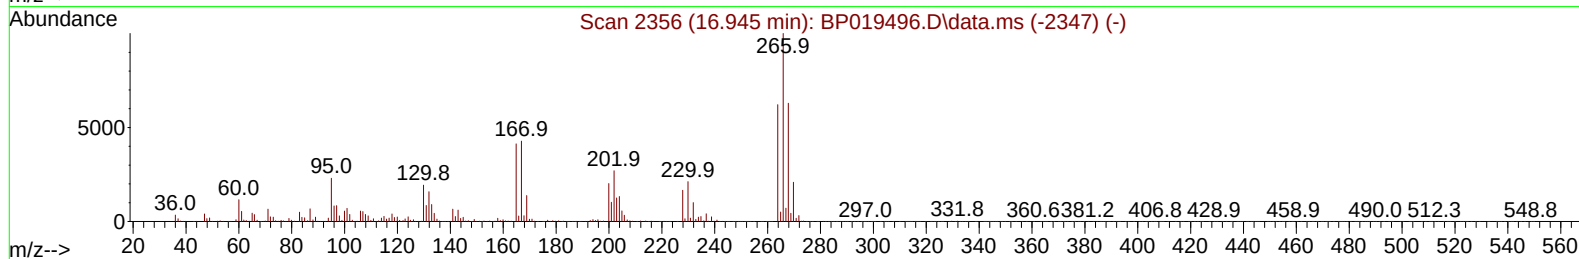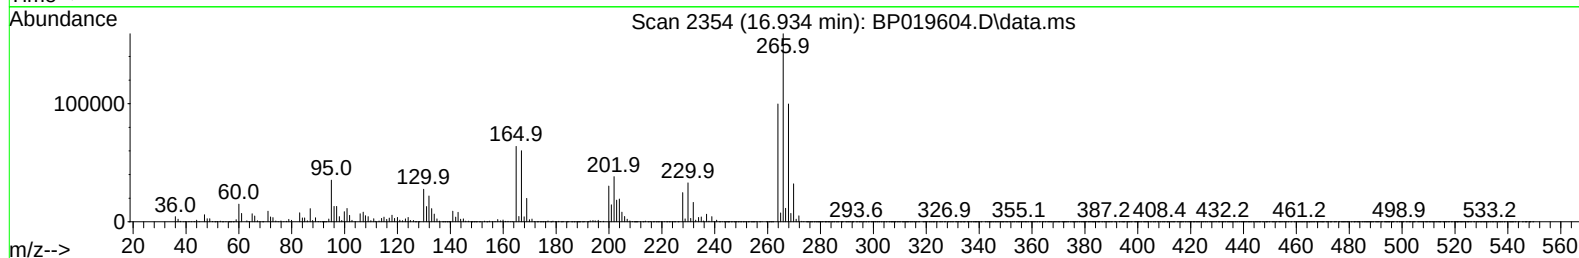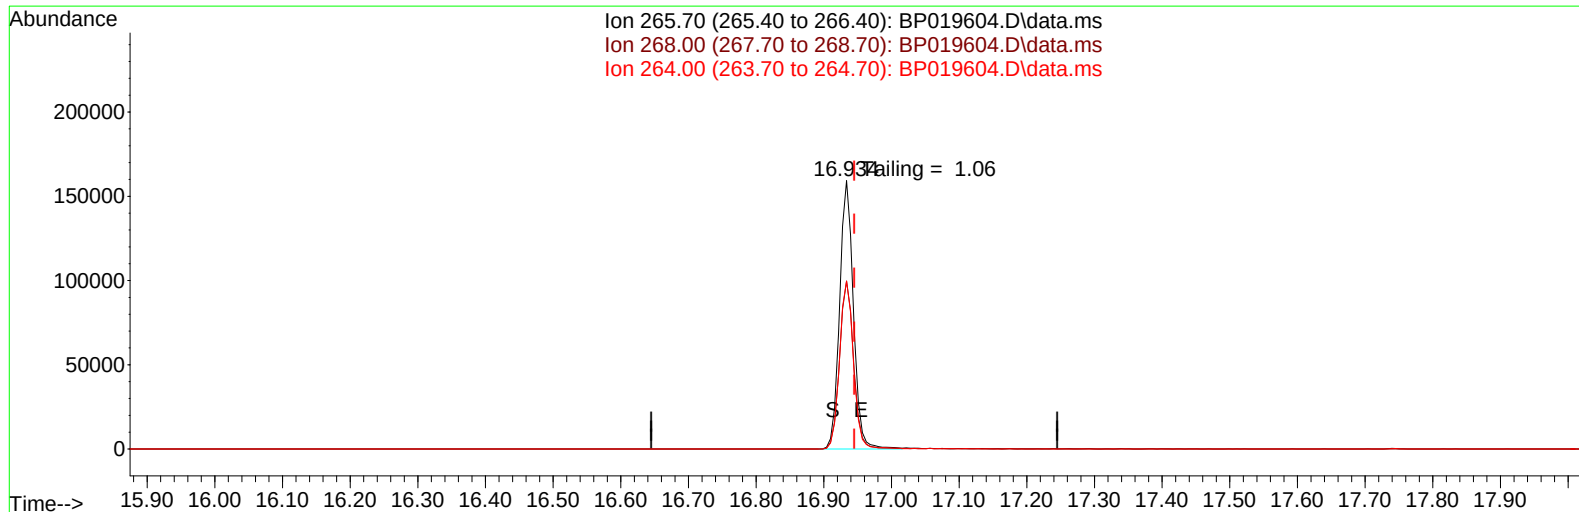

TIC: BP019604.D\data.ms

(70) Pentachlorophenol (C)

16.934min (-0.011) 318481.05 ng




response 225839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.64
264.00	62.10	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020824\
Data File : BP019604.D
Acq On : 08 Feb 2024 11:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 08 13:04:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

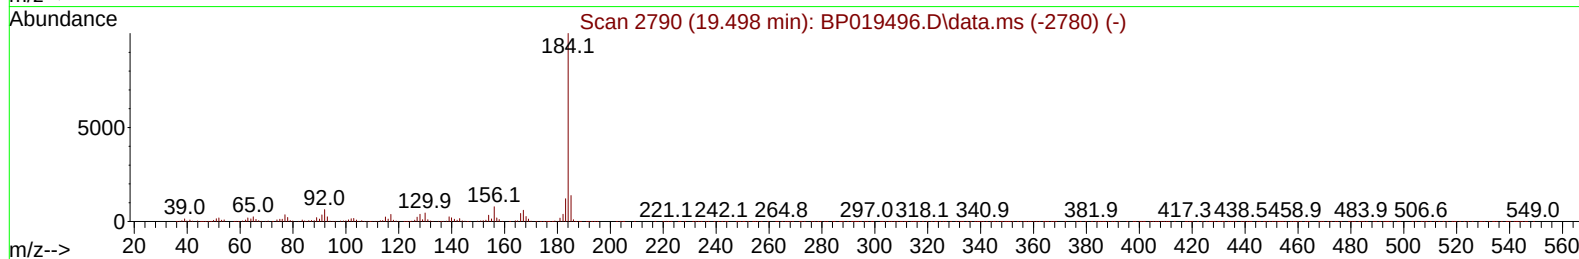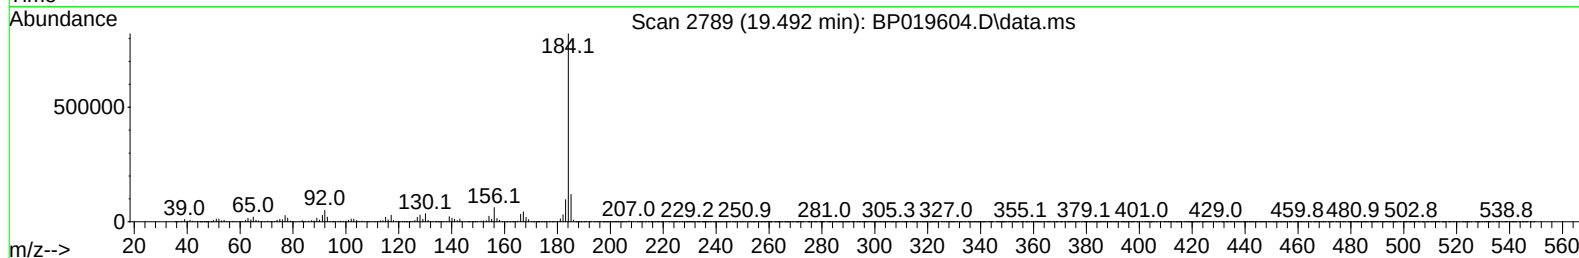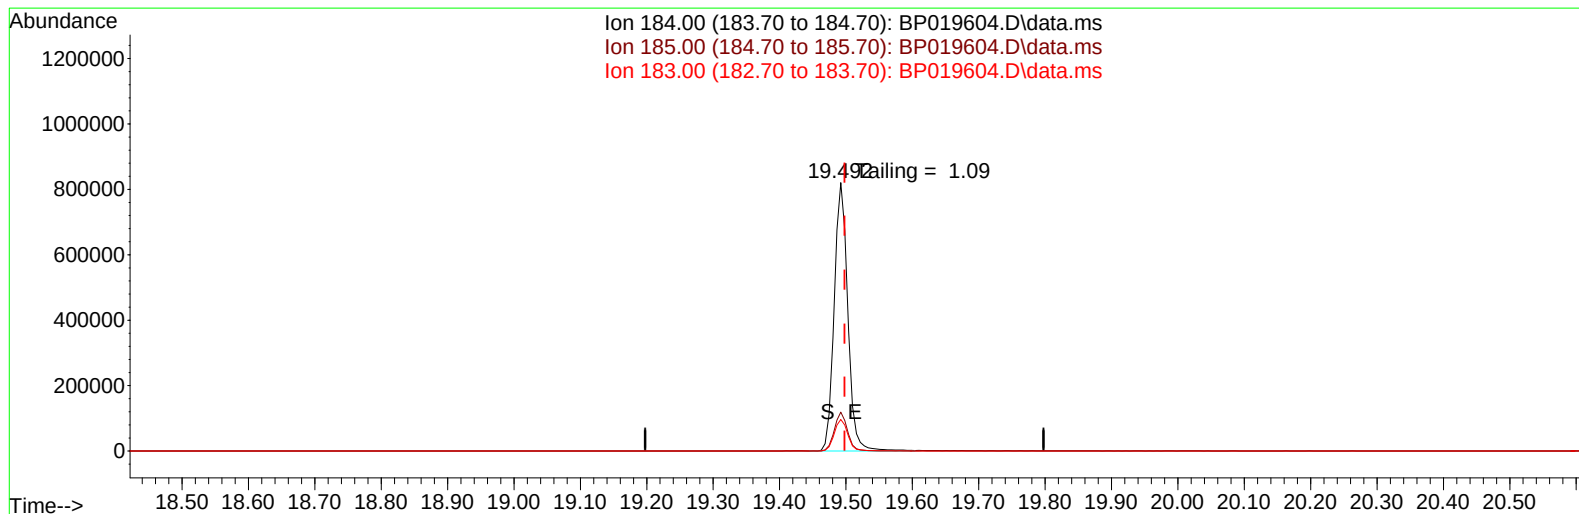

TIC: BP019604.D\data.ms

(77) Benzidine

19.492min (-0.006) 46147.84 ng

response 1169335

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.52
183.00	12.10	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/8/2024	BNA_P	<u>BP019604.D</u>
Compound Name	Response	Retention Time
DDT	679535	20.692
DDD	13194	20.263
DDE	750	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13944	693479	2.01

Instrument :
BNA_P
ClientSampleId :
DFTPP