


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020922\  
 Data File : BP009071.D  
 Acq On : 09 Feb 2022 09:57  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020722.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Feb 07 15:13:17 2022

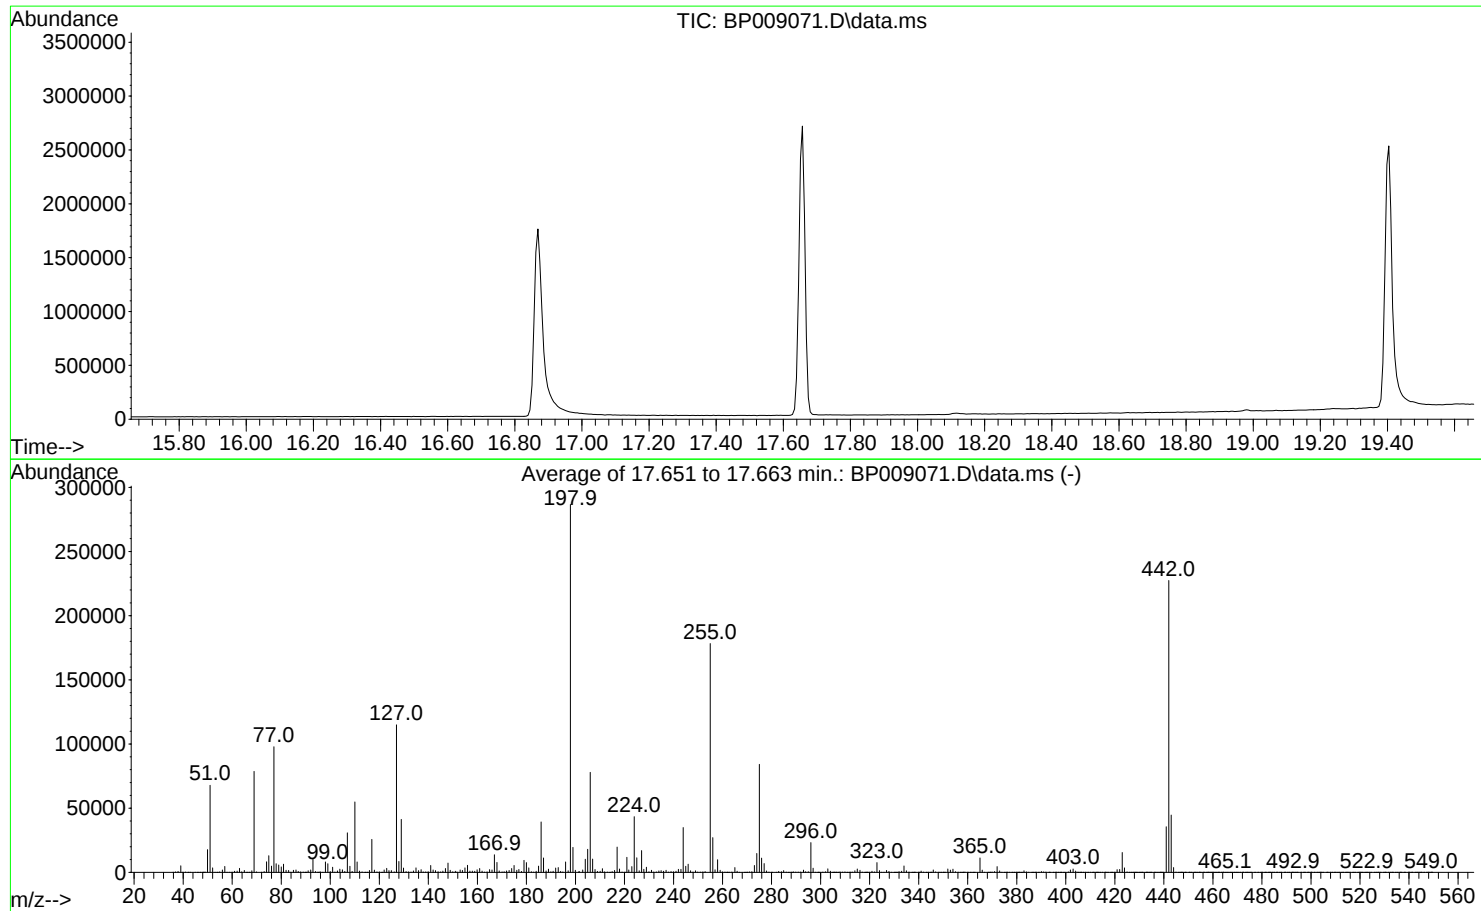




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2485

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 23.7         | 67832      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 1293       | PASS                |
| 69             | 198             | 0.00            | 100             | 27.4         | 78627      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 368        | PASS                |
| 127            | 198             | 10              | 80              | 40.1         | 114941     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 1322       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 286613     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 19475      | PASS                |
| 275            | 198             | 10              | 60              | 29.4         | 84204      | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 11191      | PASS                |
| 441            | 198             | 0.01            | 100             | 12.4         | 35504      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 227349     | PASS                |
| 443            | 442             | 15              | 24              | 19.6         | 44596      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020922\  
Data File : BP009071.D  
Acq On : 09 Feb 2022 09:57  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Feb 09 12:05:57 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 07 15:13:17 2022  
Response via : Initial Calibration

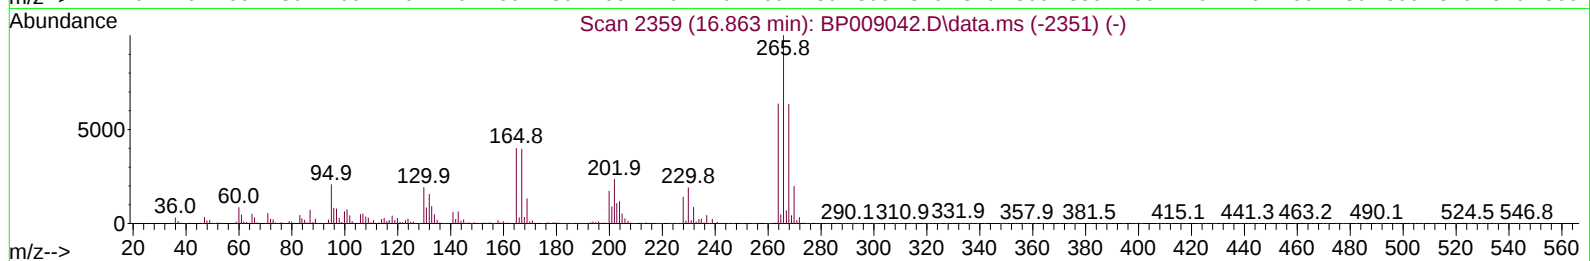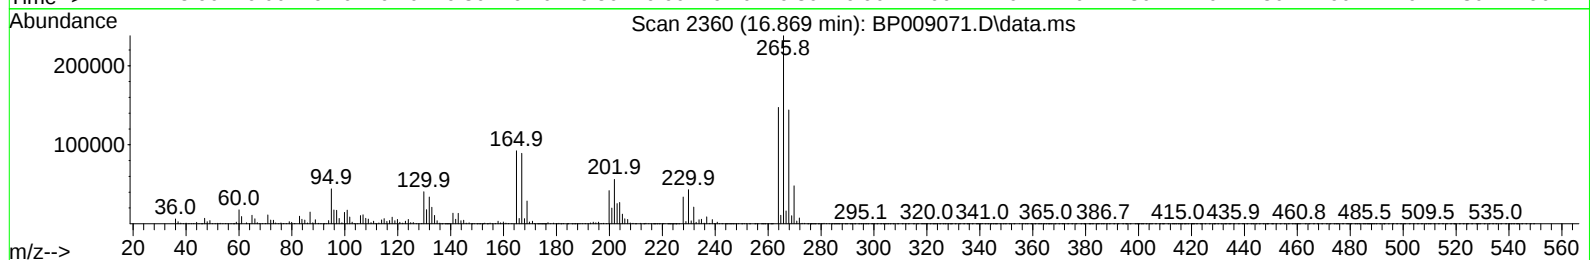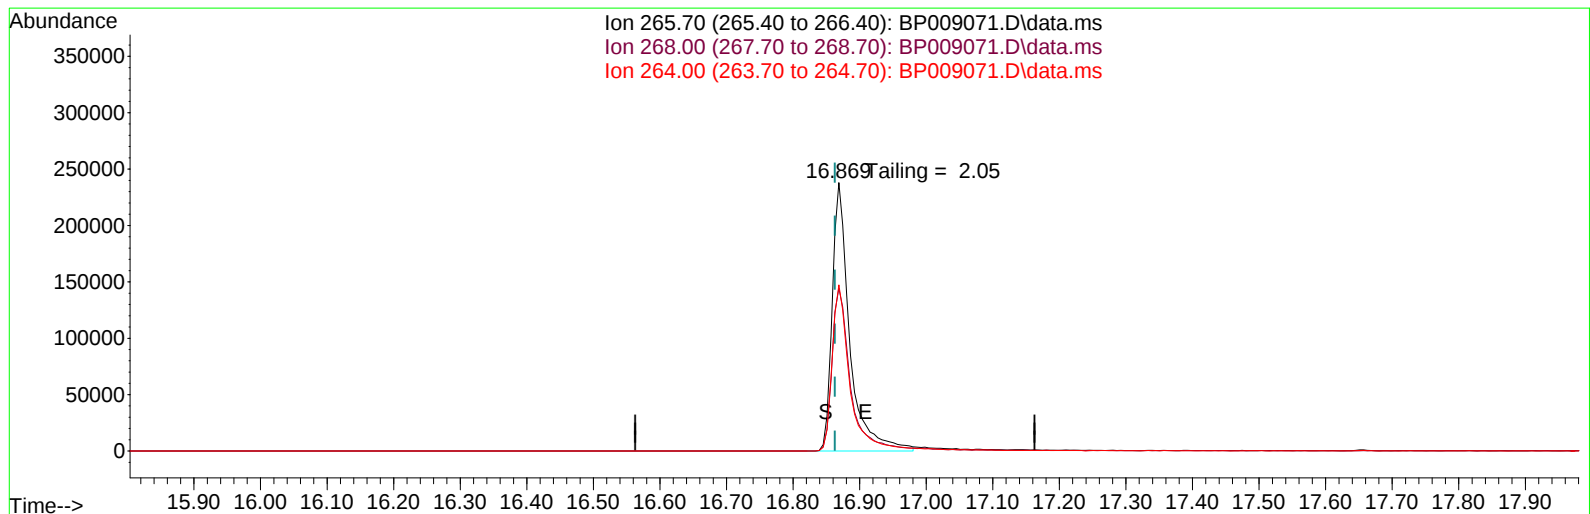

TIC: BP009071.D\data.ms

**(70) Pentachlorophenol (C)**

**16.869min (+ 0.006) 5801337.89 ng**




**response 436167**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.60  | 60.55  |
| 264.00 | 62.90  | 61.90  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020922\  
Data File : BP009071.D  
Acq On : 09 Feb 2022 09:57  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Feb 09 12:05:57 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 07 15:13:17 2022  
Response via : Initial Calibration

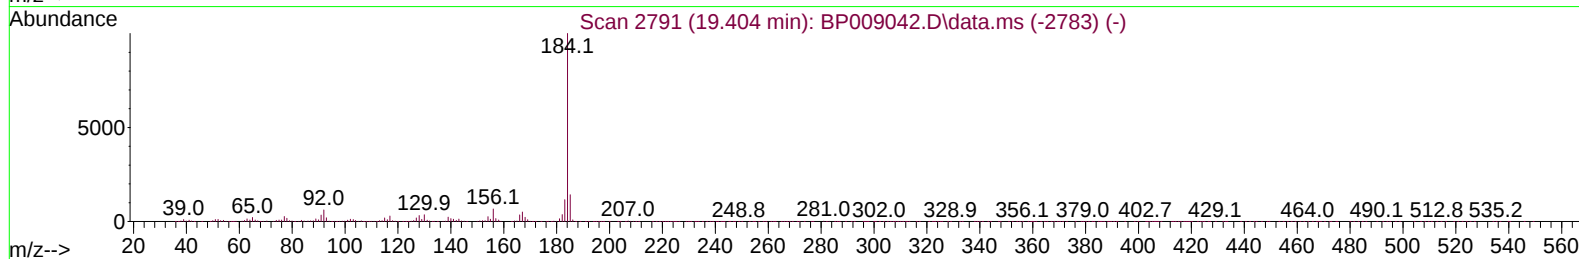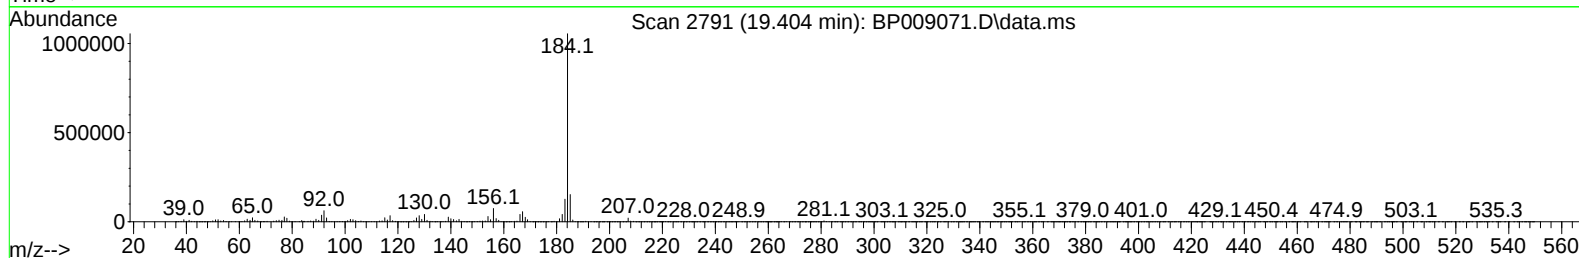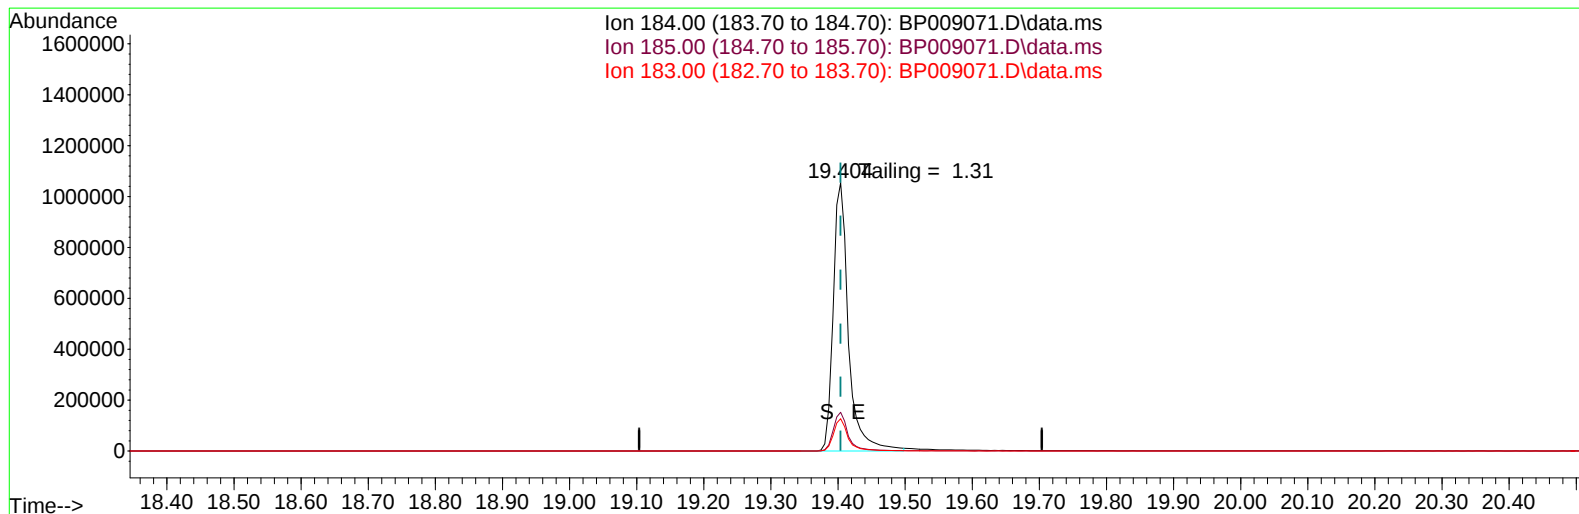

TIC: BP009071.D\data.ms

(77) Benzidine

19.404min (-0.000) 475458.85 ng

response 1669113

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.20  | 14.43  |
| 183.00 | 11.90  | 12.03  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/9/2022      | BNA_P            | <u>BP009071.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 805768           | 20.6               |
| DDD           | 23116            | 20.17              |
| DDE           | 1283             | 19.68              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 24399         | 830167           | 2.94               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP