

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020924\
 Data File : BP019638.D
 Acq On : 09 Feb 2024 18:26
 Operator : MA/JU
 Sample : P1372-06DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CG-MW-17-ch5DL

Quant Time: Feb 10 00:51:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 00:51:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	83735	20.000	ng	-0.01
21) Naphthalene-d8	10.710	136	313065	20.000	ng	0.00
39) Acenaphthene-d10	14.539	164	201018	20.000	ng	-0.01
64) Phenanthrene-d10	17.298	188	432862	20.000	ng	0.00
76) Chrysene-d12	21.386	240	430274	20.000	ng	0.00
86) Perylene-d12	23.810	264	522931	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	73006	14.054	ng	0.00
7) Phenol-d6	7.075	99	57040	8.143	ng	-0.01
23) Nitrobenzene-d5	9.075	82	154404	21.371	ng	-0.01
42) 2,4,6-Tribromophenol	16.034	330	105248	35.860	ng	0.00
45) 2-Fluorobiphenyl	13.169	172	349845	21.515	ng	-0.01
79) Terphenyl-d14	19.863	244	542296	20.727	ng	0.00
Target Compounds						
						Qvalue
4) n-Nitrosodimethylamine	4.011	42	9490	4.017	ng	# 1
10) Phenol	7.105	94	15981	2.289	ng	97
20) 3+4-Methylphenols	8.675	107	322752	50.317	ng	91
31) Naphthalene	10.757	128	904851	52.699	ng	99
33) 4-Chloroaniline	10.757	127	120701	19.009	ng	# 30
37) 2-Methylnaphthalene	12.587	142	136553	11.492	ng	99
38) 1-Methylnaphthalene	12.587	142	136553	11.694	ng	97
49) Acenaphthylene	14.263	152	78530	4.250	ng	98
52) Acenaphthene	14.604	154	47108	4.108	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020924\
Data File : BP019638.D
Acq On : 09 Feb 2024 18:26
Operator : MA/JU
Sample : P1372-06DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CG-MW-17-ch5DL

Quant Time: Feb 10 00:51:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration




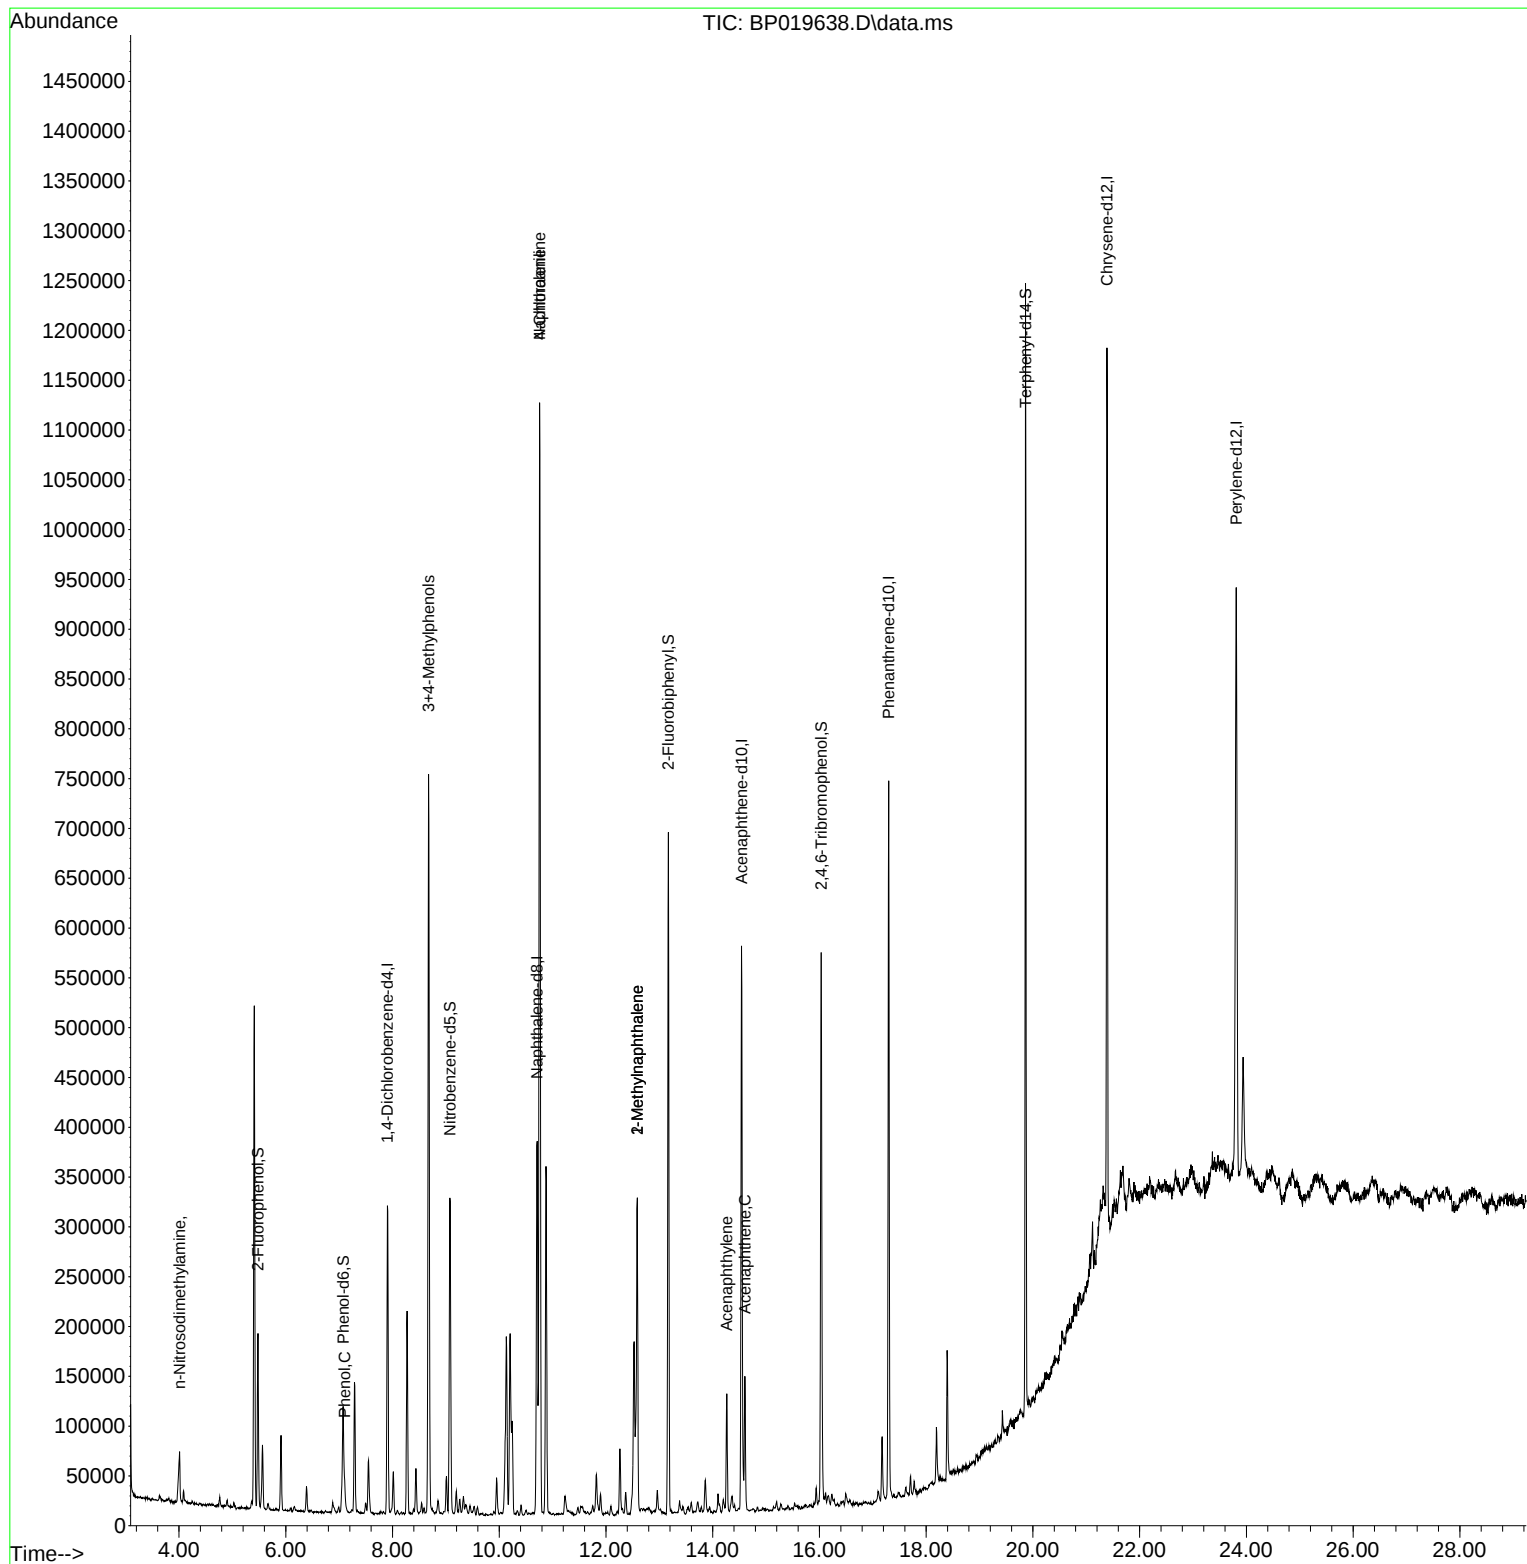




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.905 min Scan# 81
Delta R.T. -0.011 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26




Instrument :
BNA_P
ClientSampleId :
CG-MW-17-ch5DL


Tgt Ion:152 Resp: 83735
Ion Ratio Lower Upper
152 100
150 154.1 121.8 182.8
115 62.3 49.9 74.9

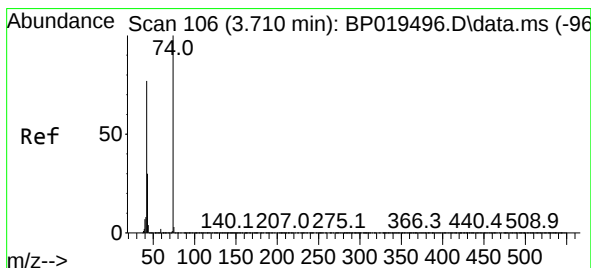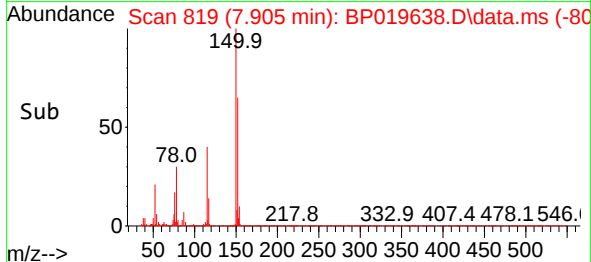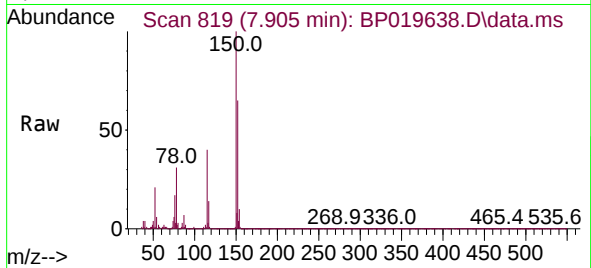

#4
n-Nitrosodimethylamine
Concen: 4.017 ng
RT: 4.011 min Scan# 157
Delta R.T. 0.300 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26

Tgt Ion: 42 Resp: 9490
Ion Ratio Lower Upper
42 100
74 4.6 103.4 155.2#
44 11.5 4.8 7.2#


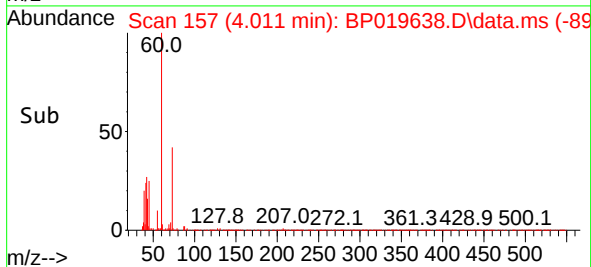

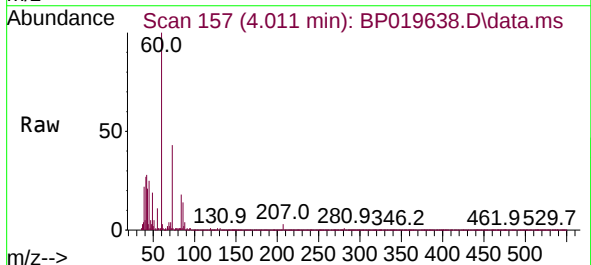




#5
2-Fluorophenol
Concen: 14.054 ng
RT: 5.481 min Scan# 408
Delta R.T. -0.006 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26




Instrument :
BNA_P
ClientSampleId :
CG-MW-17-ch5DL


Tgt Ion:112 Resp: 73006
Ion Ratio Lower Upper
112 100
64 54.7 47.4 71.0
63 33.4 27.0 40.6

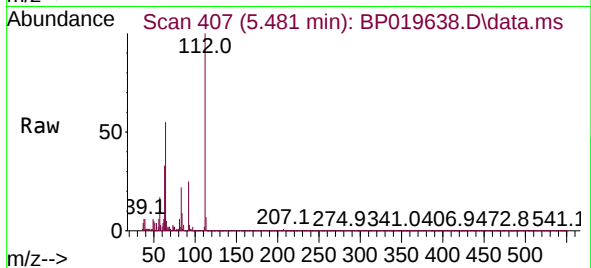

#7
Phenol-d6
Concen: 8.143 ng
RT: 7.075 min Scan# 678
Delta R.T. -0.012 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26

Tgt Ion: 99 Resp: 57040
Ion Ratio Lower Upper
99 100
42 19.0 14.7 22.1
71 44.7 34.8 52.2


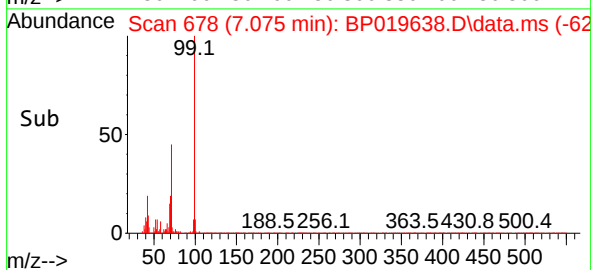






#10
Phenol
Concen: 2.289 ng
RT: 7.105 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26




Instrument :
BNA_P
ClientSampleId :
CG-MW-17-ch5DL


Tgt Ion:	94	Resp:	15981
Ion	Ratio	Lower	Upper
94	100		
65	28.0	11.3	51.3
66	45.5	25.1	65.1



#20
3+4-Methylphenols
Concen: 50.317 ng
RT: 8.675 min Scan# 950
Delta R.T. -0.017 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26

Tgt Ion:	107	Resp:	322752
Ion	Ratio	Lower	Upper
107	100		
108	78.5	65.5	105.5
77	36.9	21.8	61.8
79	25.9	14.1	54.1


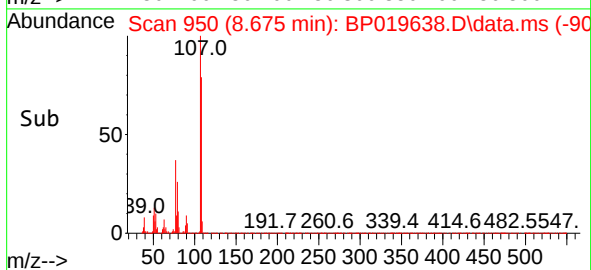






#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.710 min Scan# 1018
Delta R.T. -0.006 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26




Instrument :
BNA_P
ClientSampleId :
CG-MW-17-ch5DL


Tgt Ion:	136	Resp:	313065
Ion Ratio	Lower	Upper	
136	100		
137	10.7	8.8	13.2
54	7.0	5.3	7.9
68	5.2	4.1	6.1



#23
Nitrobenzene-d5
Concen: 21.371 ng
RT: 9.075 min Scan# 1018
Delta R.T. -0.012 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26

Tgt Ion:	82	Resp:	154404
Ion Ratio	Lower	Upper	
82	100		
128	37.7	29.7	44.5
54	45.1	36.8	55.2


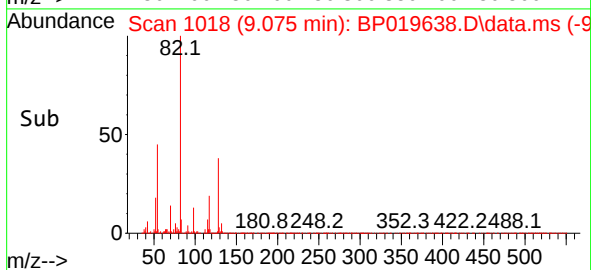






#31
Naphthalene
Concen: 52.699 ng
RT: 10.757 min Scan# 1304
Delta R.T. -0.012 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26




Instrument :
BNA_P
ClientSampleId :
CG-MW-17-ch5DL


Tgt Ion:128 Resp: 904851
Ion Ratio Lower Upper
128 100
129 11.1 8.6 13.0
127 13.3 10.8 16.2



#33
4-Chloroaniline
Concen: 19.009 ng
RT: 10.757 min Scan# 1304
Delta R.T. -0.129 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26

Tgt Ion:127 Resp: 120701
Ion Ratio Lower Upper
127 100
129 83.8 24.6 36.8#
65 0.0 28.2 42.4#
92 0.1 18.9 28.3#


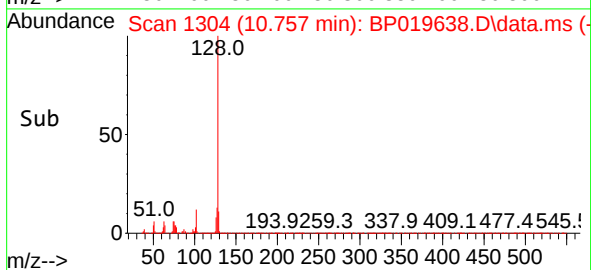
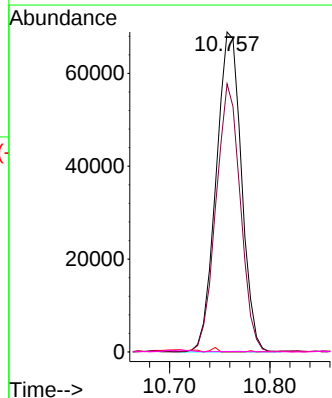



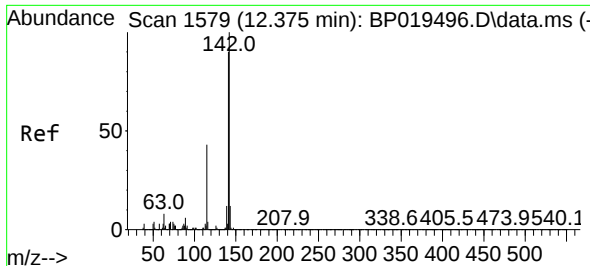

#37
2-Methylnaphthalene
Concen: 11.492 ng
RT: 12.587 min Scan# 1615
Delta R.T. 0.212 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26




Instrument :
BNA_P
ClientSampleId :
CG-MW-17-ch5DL


Tgt Ion:142 Resp: 136553
Ion Ratio Lower Upper
142 100
141 89.7 72.2 108.4
115 42.2 34.2 51.2

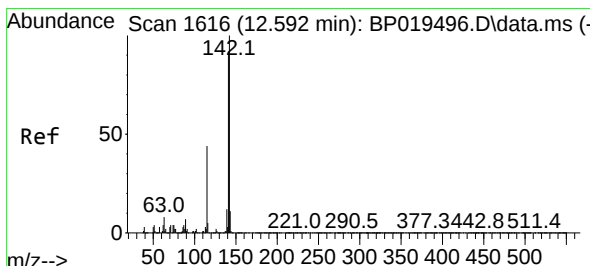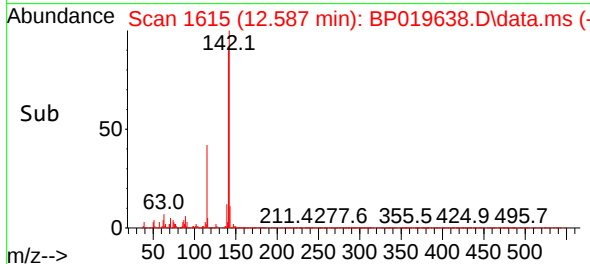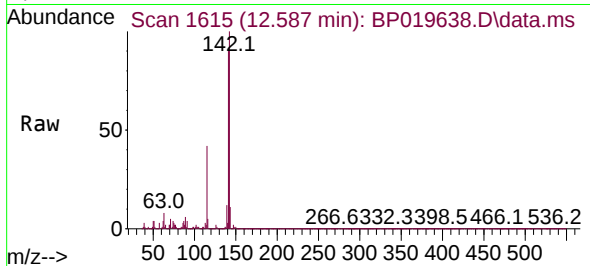

#38
1-Methylnaphthalene
Concen: 11.694 ng
RT: 12.587 min Scan# 1615
Delta R.T. -0.006 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26

Tgt Ion:142 Resp: 136553
Ion Ratio Lower Upper
142 100
141 89.7 74.0 111.0
116 4.7 3.7 5.5


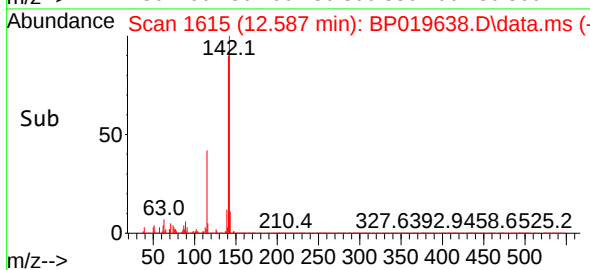

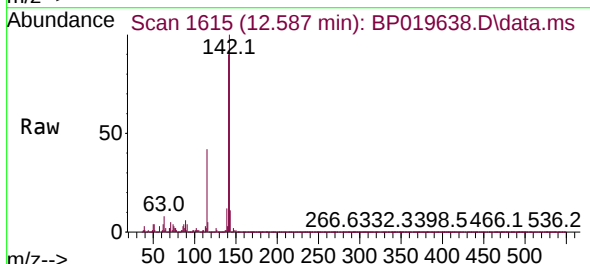




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.539 min Scan# 1947
Delta R.T. -0.012 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26




Instrument :
BNA_P
ClientSampleId :
CG-MW-17-ch5DL


Tgt Ion:164 Resp: 201018
Ion Ratio Lower Upper
164 100
162 101.3 81.2 121.8
160 44.7 35.1 52.7



#42
2,4,6-Tribromophenol
Concen: 35.860 ng
RT: 16.034 min Scan# 2201
Delta R.T. -0.006 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26

Tgt Ion:330 Resp: 105248
Ion Ratio Lower Upper
330 100
332 97.7 77.2 115.8
141 31.4 27.0 40.4


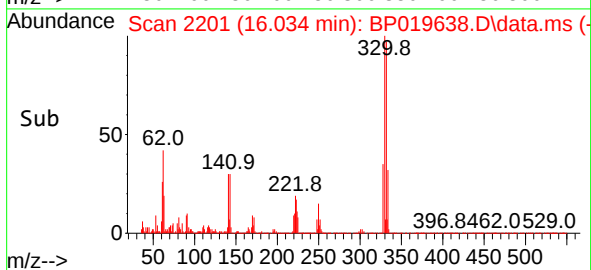




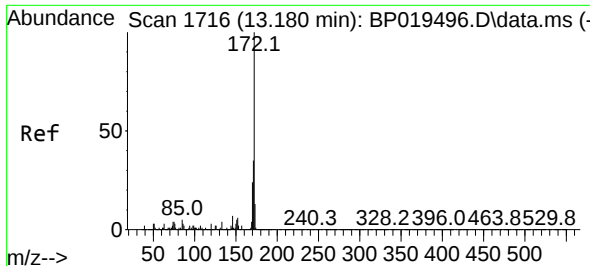

#45
2-Fluorobiphenyl
Concen: 21.515 ng
RT: 13.169 min Scan# 1716
Delta R.T. -0.012 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26




Instrument :
BNA_P
ClientSampleId :
CG-MW-17-ch5DL


Tgt Ion:172 Resp: 349845
Ion Ratio Lower Upper
172 100
171 35.0 28.2 42.4
170 23.3 18.9 28.3

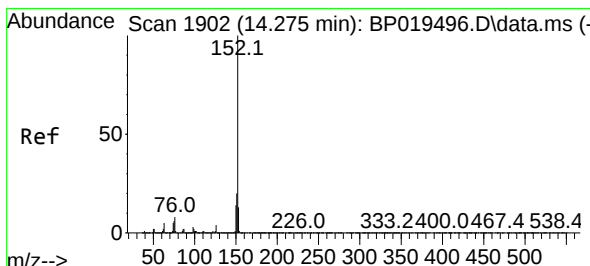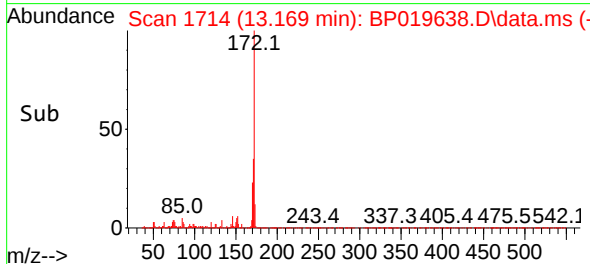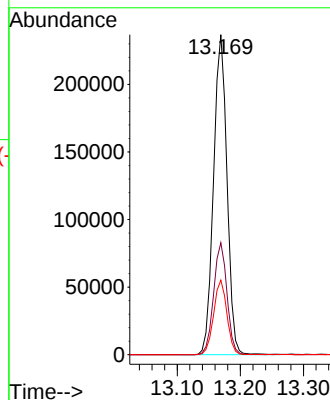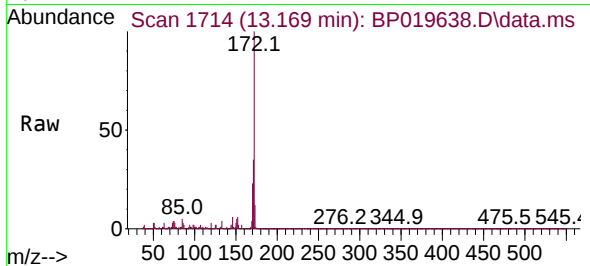

#49
Acenaphthylene
Concen: 4.250 ng
RT: 14.263 min Scan# 1900
Delta R.T. -0.012 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26

Tgt Ion:152 Resp: 78530
Ion Ratio Lower Upper
152 100
151 19.3 15.8 23.6
153 14.3 10.6 15.8


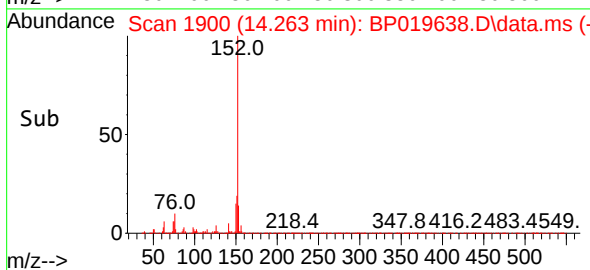
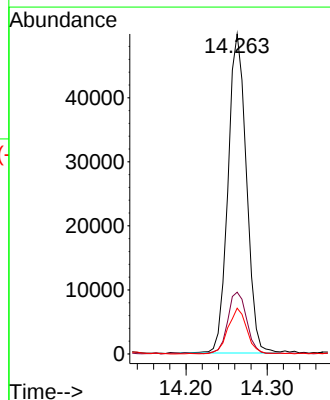
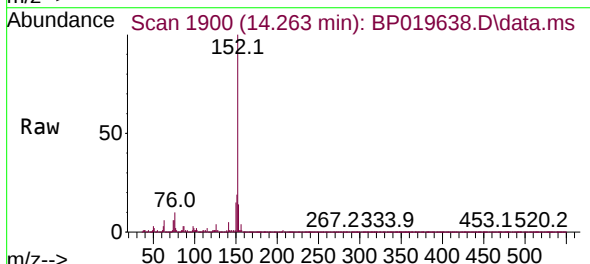




#52
Acenaphthene
Concen: 4.108 ng
RT: 14.604 min Scan# 1958
Delta R.T. -0.012 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26




Instrument :
BNA_P
ClientSampleId :
CG-MW-17-ch5DL


Tgt Ion:154 Resp: 47108
Ion Ratio Lower Upper
154 100
153 111.6 90.5 135.7
152 50.3 42.1 63.1



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.298 min Scan# 2416
Delta R.T. -0.006 min
Lab File: BP019638.D
Acq: 09 Feb 2024 18:26

Tgt Ion:188 Resp: 432862
Ion Ratio Lower Upper
188 100
94 6.7 5.4 8.2
80 7.9 6.3 9.5

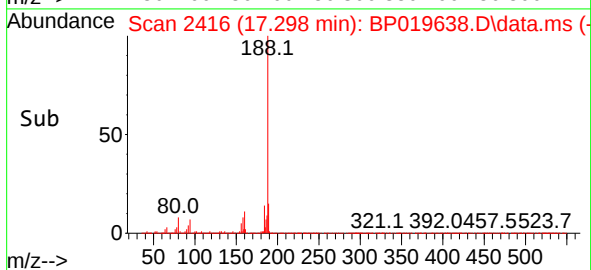

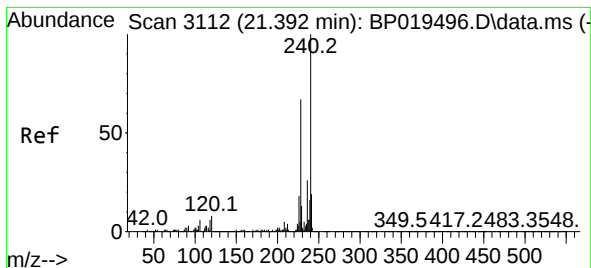

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.386 min Scan# 3111

Delta R.T. -0.006 min

Lab File: BP019638.D

Acq: 09 Feb 2024 18:26

Instrument :

BNA_P

ClientSampleId :

CG-MW-17-ch5DL





Tgt Ion:240 Resp: 430274

Ion Ratio Lower Upper

240 100

120 6.8 6.1 9.1

236 25.8 20.7 31.1

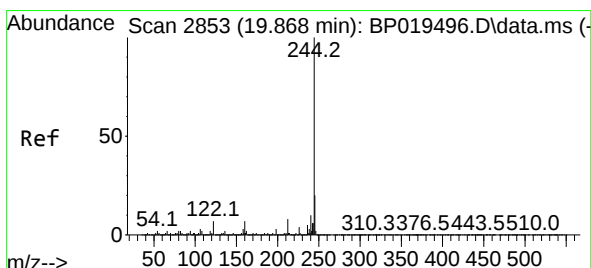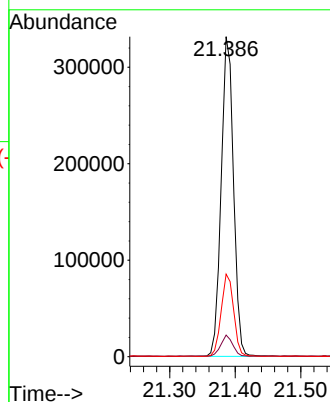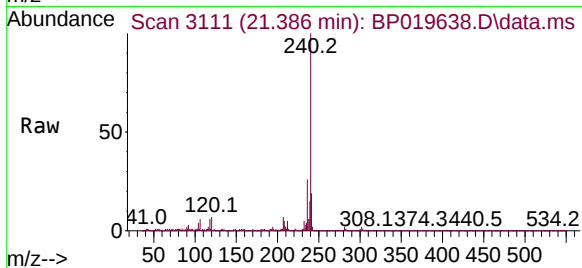

#79

Terphenyl-d14

Concen: 20.727 ng

RT: 19.863 min Scan# 2852

Delta R.T. -0.006 min

Lab File: BP019638.D

Acq: 09 Feb 2024 18:26




Tgt Ion:244 Resp: 542296


Ion Ratio Lower Upper

244 100

212 7.7 6.1 9.1

122 7.3 5.9 8.9

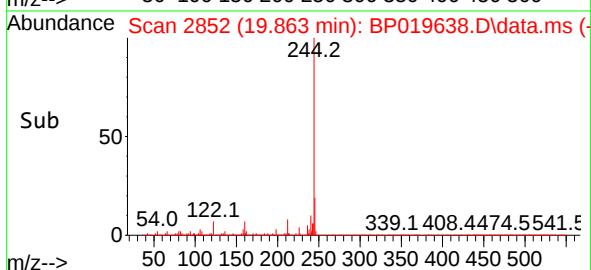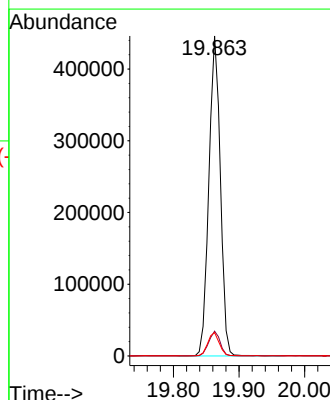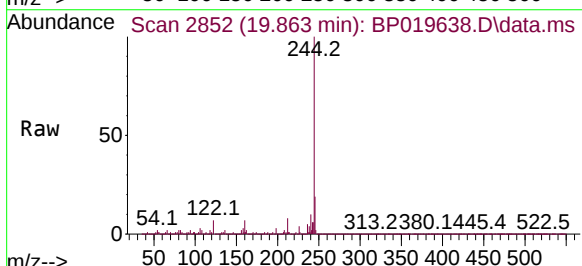



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.810 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BP019638.D
 Acq: 09 Feb 2024 18:26

Instrument :
 BNA_P
 ClientSampleId :
 CG-MW-17-ch5DL

Tgt Ion:264 Resp: 522931
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.2 28.8
 265 21.9 17.0 25.4

