
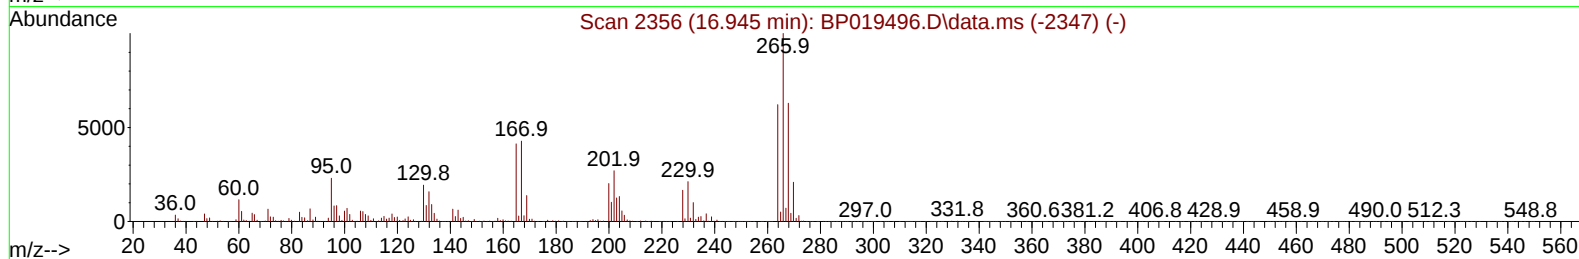
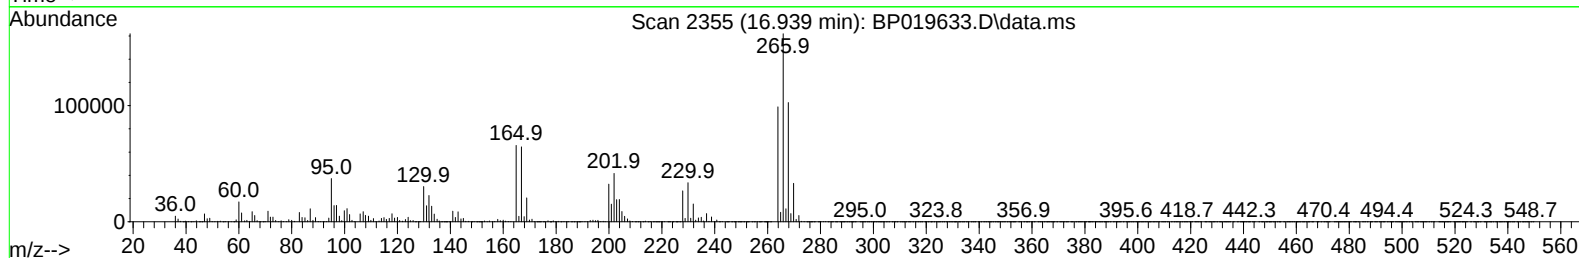


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020924\
Data File : BP019633.D
Acq On : 09 Feb 2024 15:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 16:03:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

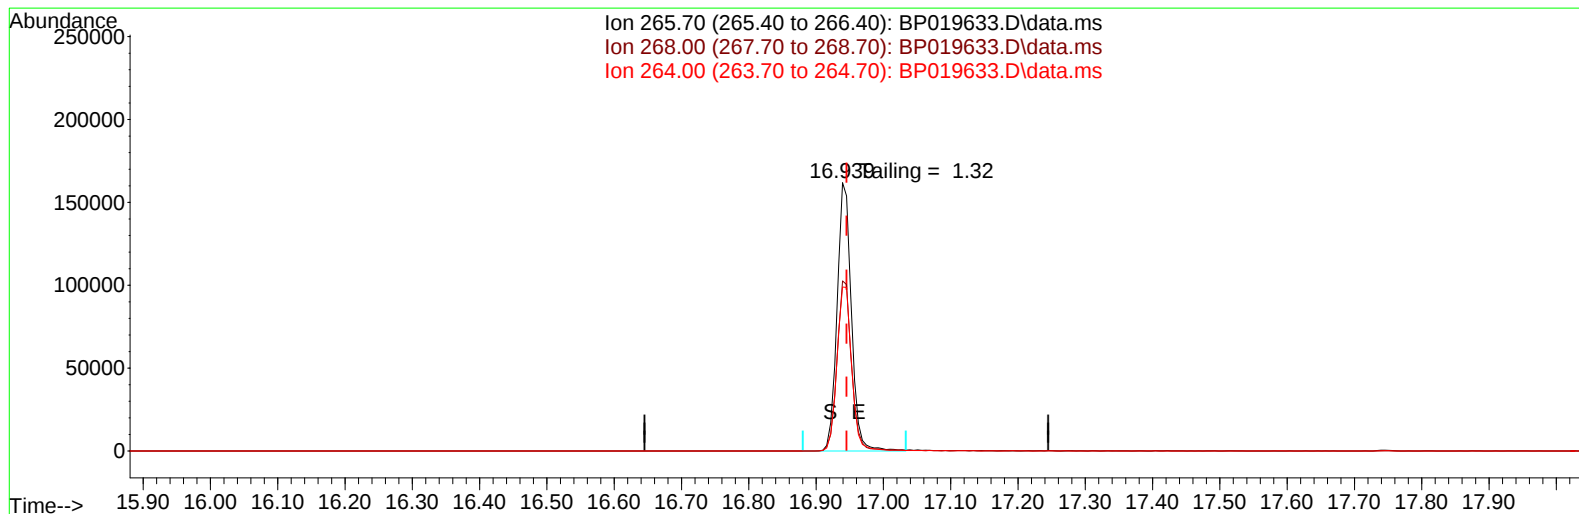

TIC: BP019633.D\data.ms

(70) Pentachlorophenol (C)




16.939min (-0.006) 1197577.97 ng m

response 239523

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.39
264.00	62.10	61.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020924\
Data File : BP019633.D
Acq On : 09 Feb 2024 15:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 16:03:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

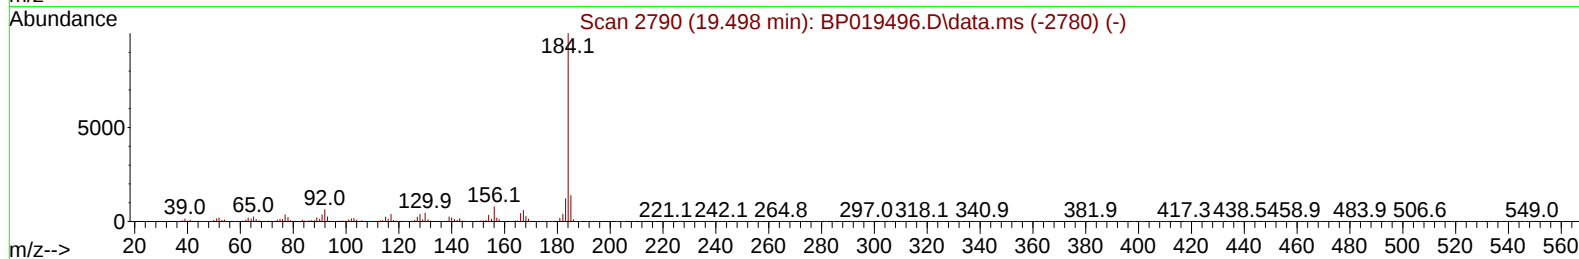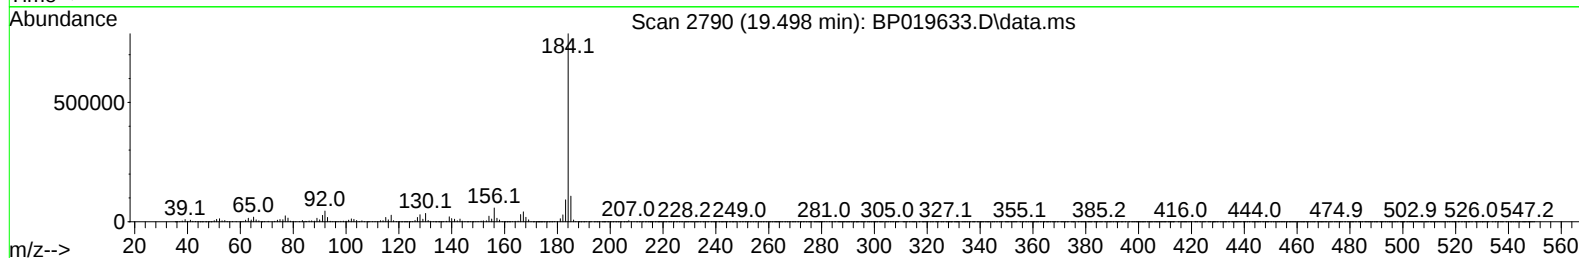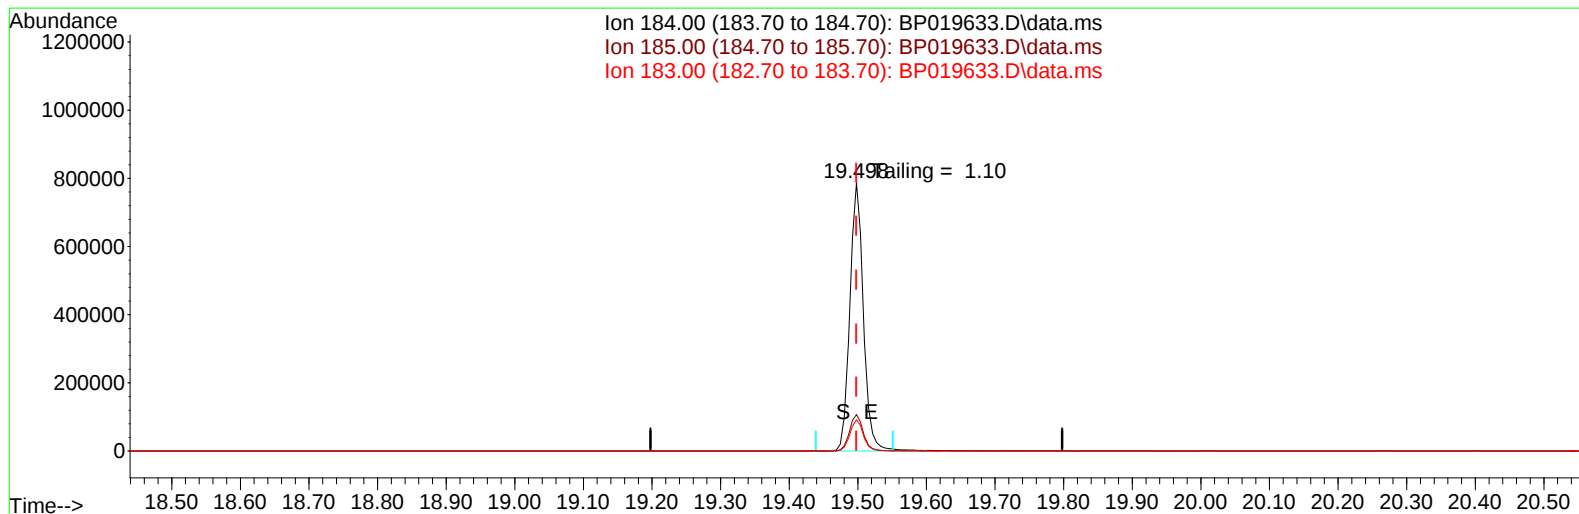

TIC: BP019633.D\data.ms

(77) Benzidine**19.498min (+ 0.000) 953881.04 ng****response 1076894**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.59
183.00	12.10	11.66
0.00	0.00	0.00