


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020924\
Data File : BP019623.D
Acq On : 09 Feb 2024 09:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

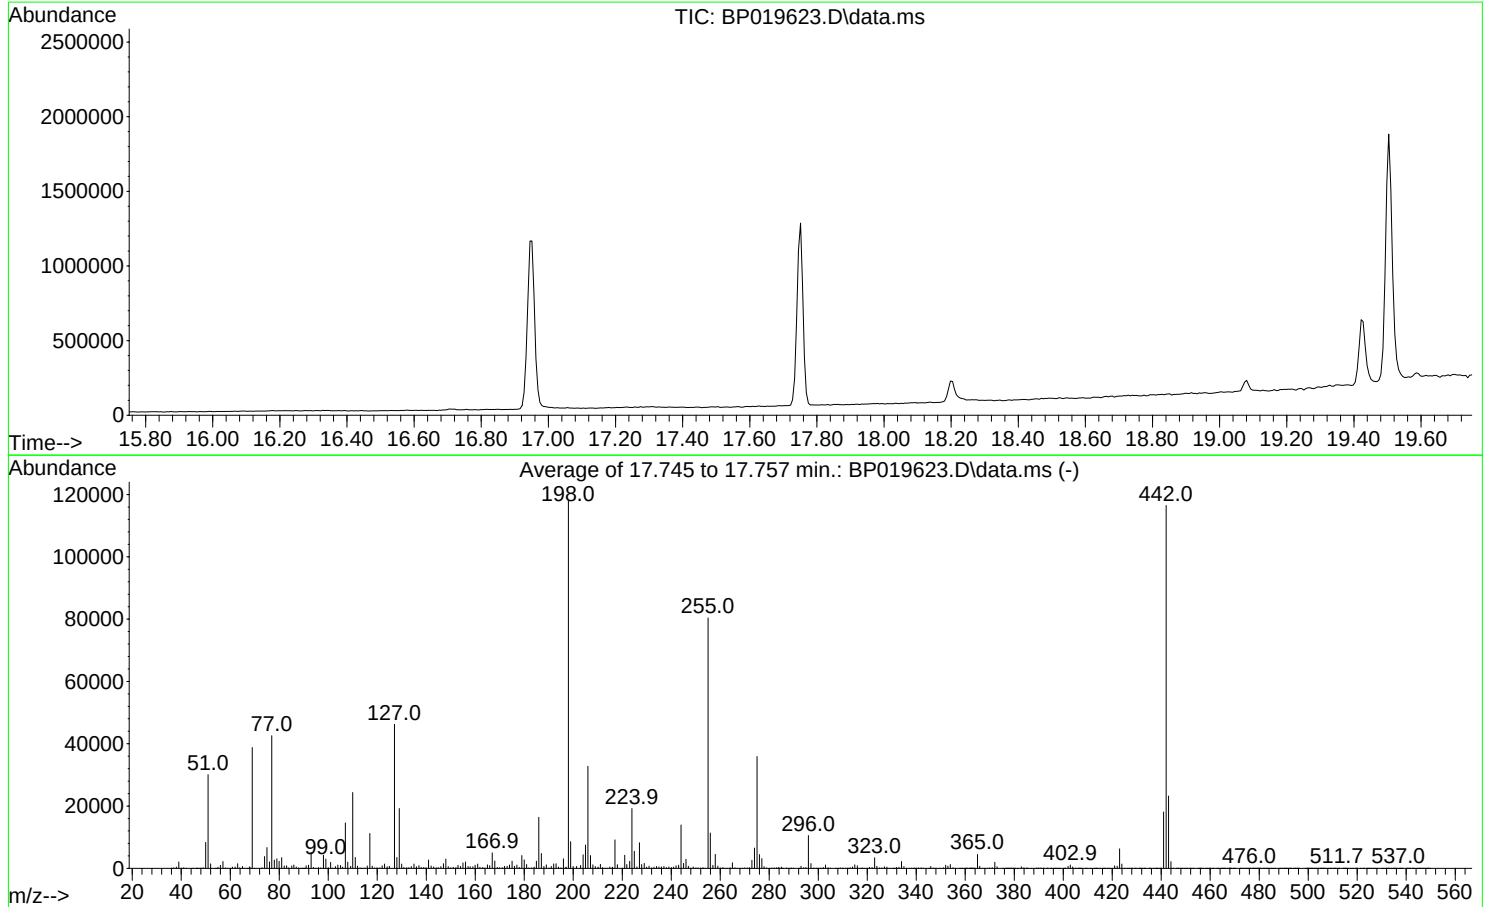




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	30104	PASS
68	69	0.00	2	1.4	533	PASS
69	198	0.00	100	32.8	38761	PASS
70	69	0.00	2	0.2	76	PASS
127	198	10	80	39.1	46224	PASS
197	198	0.00	2	0.4	439	PASS
198	198	100	100	100.0	118084	PASS
199	198	5	9	7.3	8596	PASS
275	198	10	60	30.4	35883	PASS
365	198	1	100	3.8	4493	PASS
441	198	0.01	100	15.3	18107	PASS
442	442	100	100	100.0	116480	PASS
443	442	15	24	19.9	23193	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020924\
Data File : BP019623.D
Acq On : 09 Feb 2024 09:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 09 18:34:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

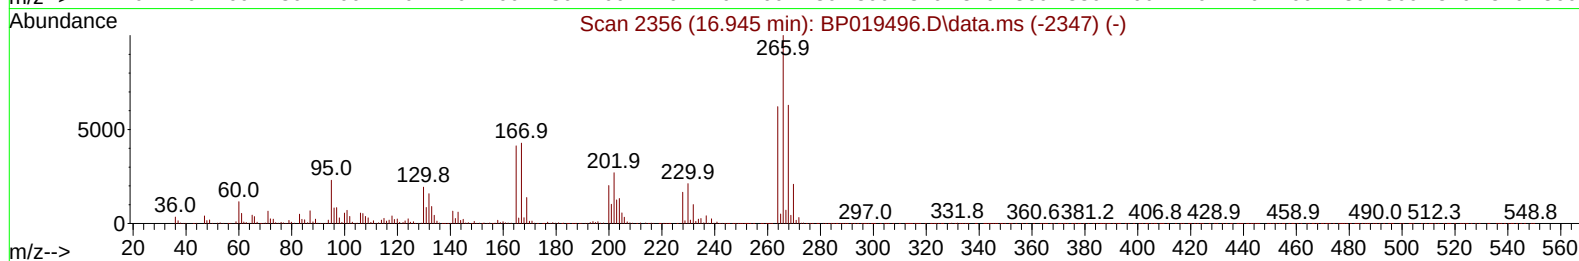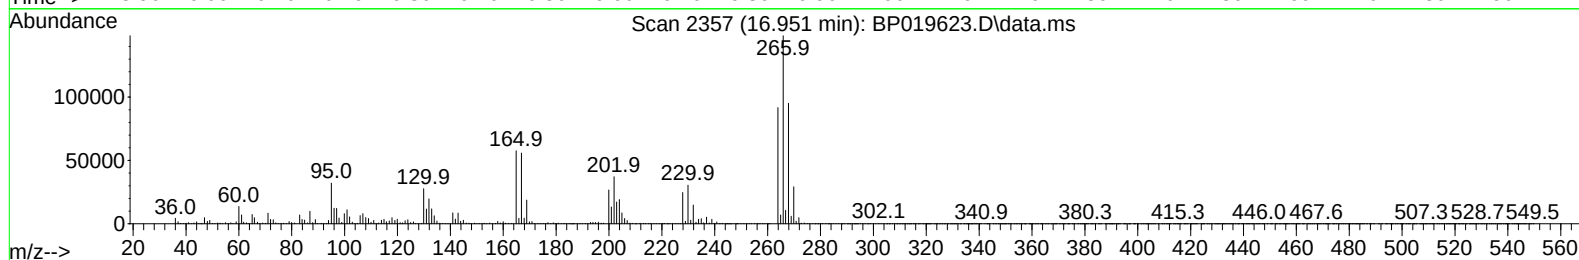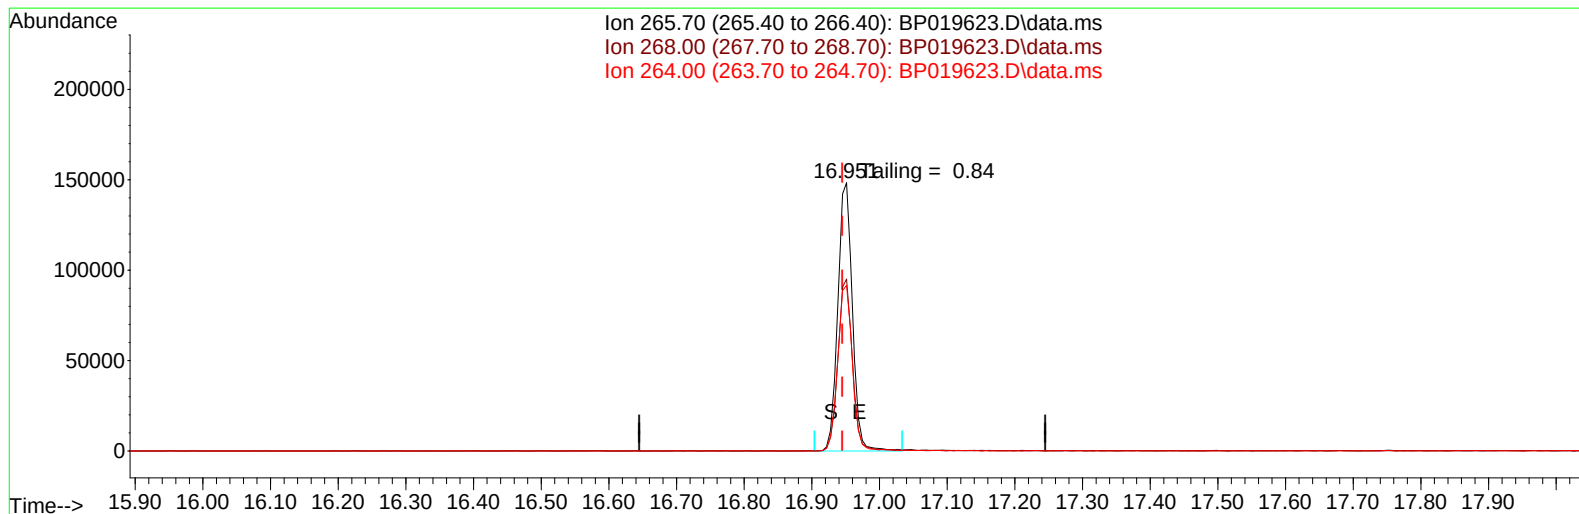

TIC: BP019623.D\data.ms

(70) Pentachlorophenol (C)

16.951min (+ 0.006) 84534.30 ng




response 221333

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.07
264.00	62.10	61.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020924\
Data File : BP019623.D
Acq On : 09 Feb 2024 09:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 09 18:34:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

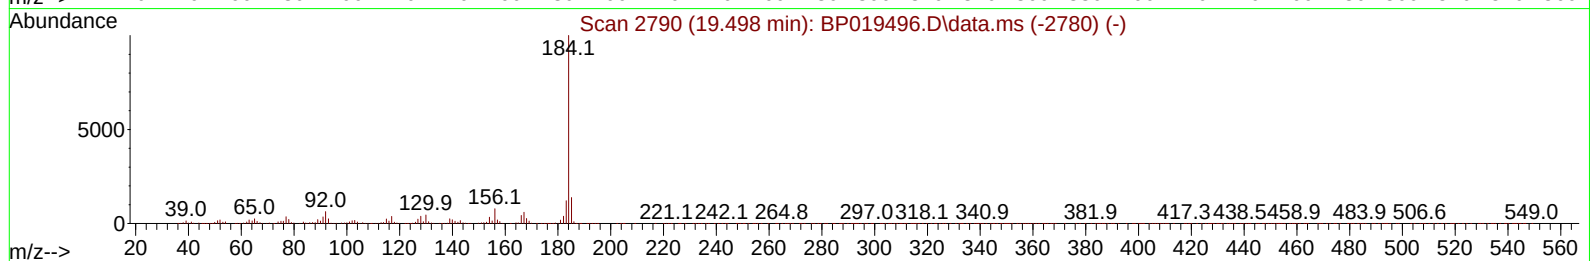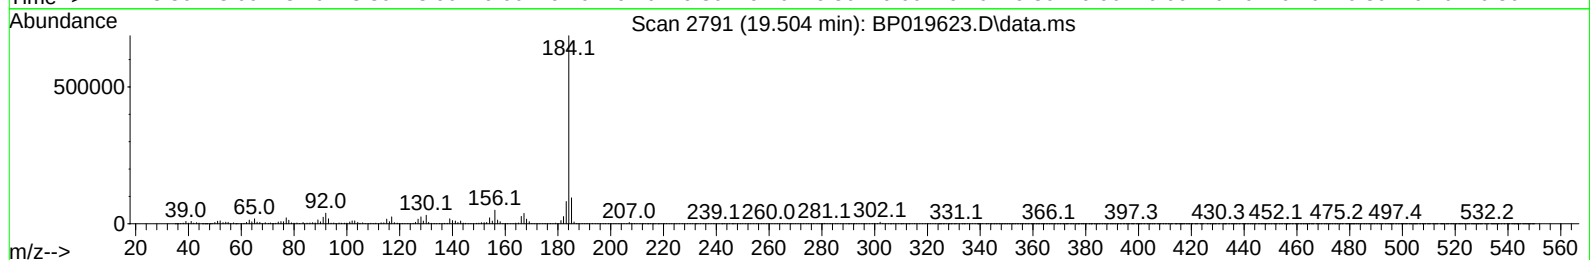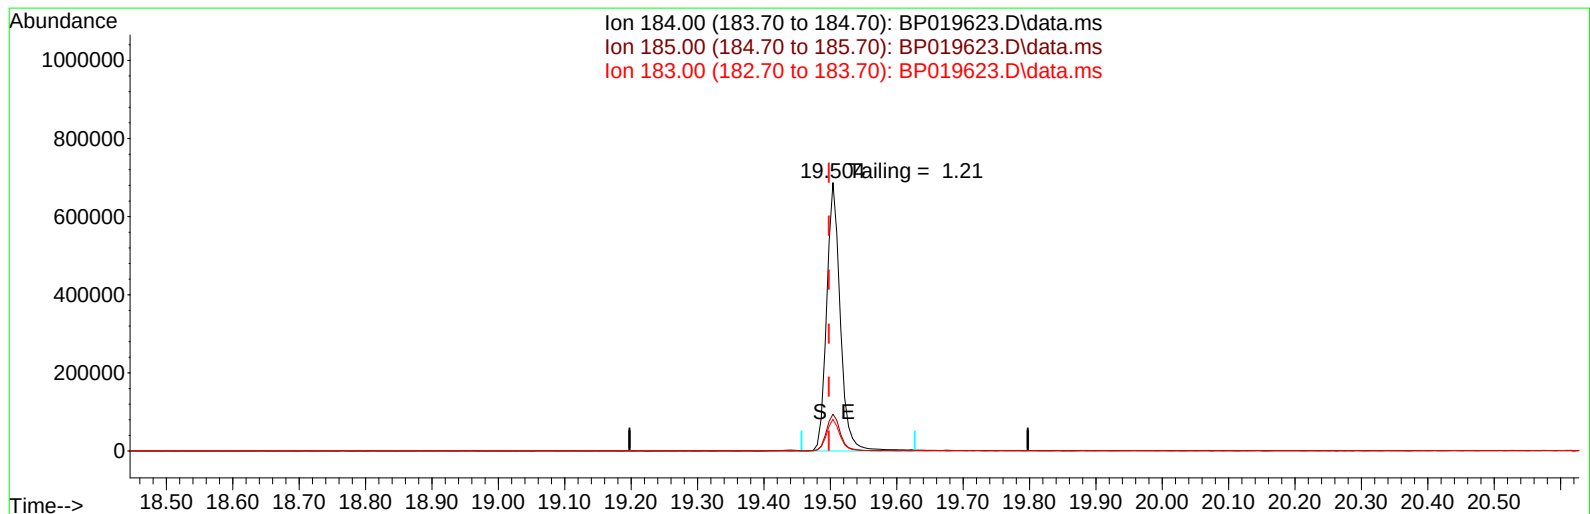

TIC: BP019623.D\data.ms

(77) Benzidine

19.504min (+ 0.006) 88599.52 ng

response 979878

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.76
183.00	12.10	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/9/2024	BNA_P	<u>BP019623.D</u>
Compound Name	Response	Retention Time
DDT	533359	20.704
DDD	11977	20.274
DDE	1386	19.427
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13363	546722	2.44

Instrument :
BNA_P
ClientSampleId :
DFTPP