


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020924\
Data File : BP019633.D
Acq On : 09 Feb 2024 15:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

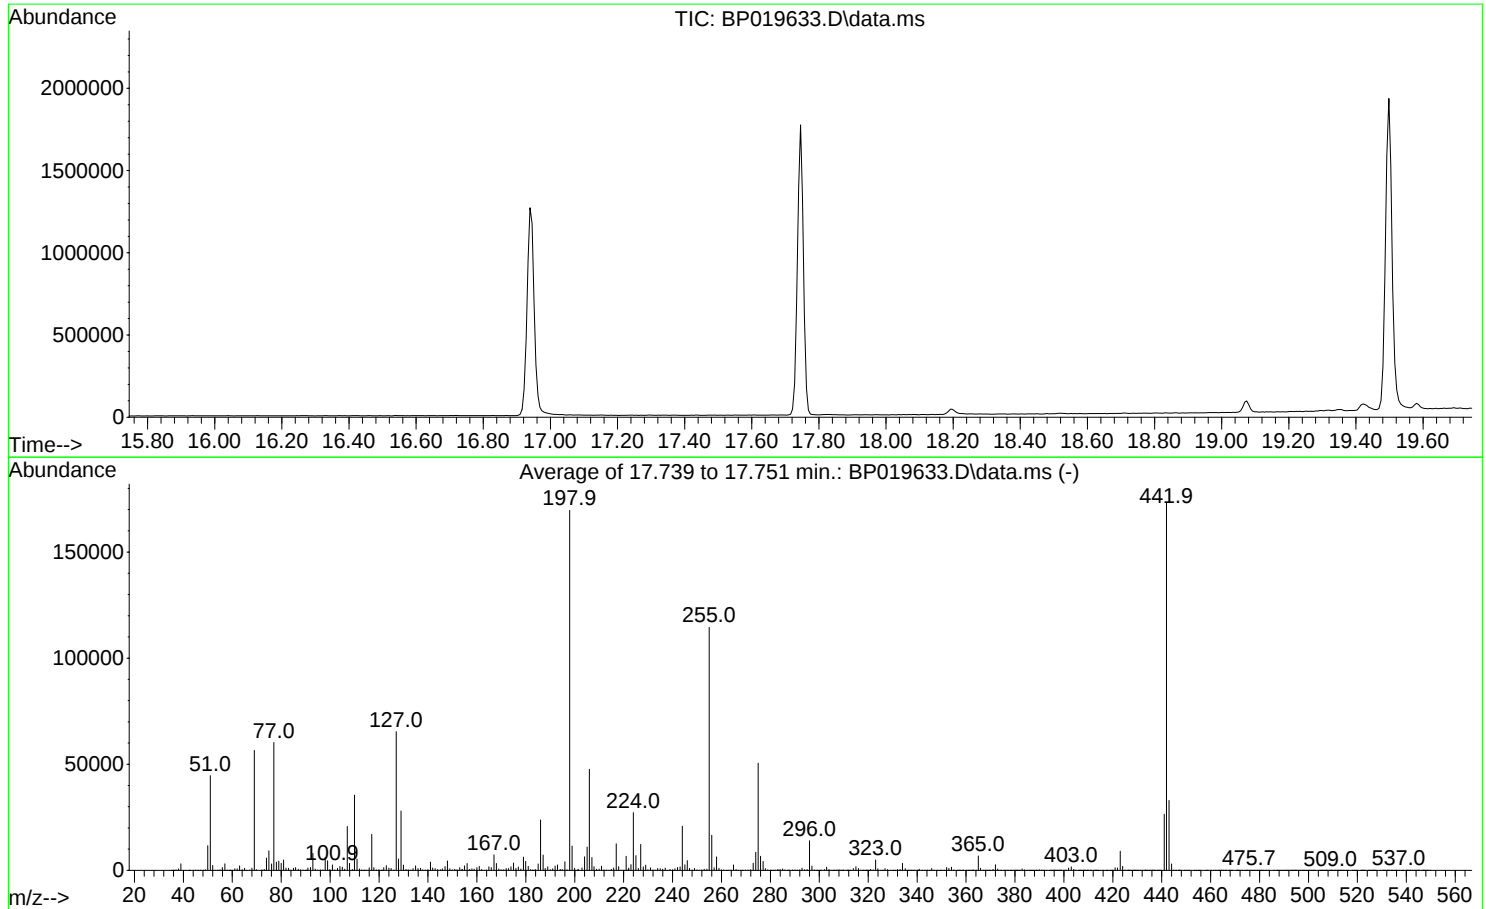




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.3	44664	PASS
68	69	0.00	2	1.9	1072	PASS
69	198	0.00	100	33.3	56571	PASS
70	69	0.00	2	0.6	325	PASS
127	198	10	80	38.5	65363	PASS
197	198	0.00	2	0.2	291	PASS
198	198	100	100	100.0	169678	PASS
199	198	5	9	6.7	11439	PASS
275	198	10	60	29.8	50536	PASS
365	198	1	100	4.0	6821	PASS
441	198	0.01	100	15.6	26439	PASS
442	442	100	100	100.0	173362	PASS
443	442	15	24	19.0	32990	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020924\
Data File : BP019633.D
Acq On : 09 Feb 2024 15:37
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 09 16:03:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

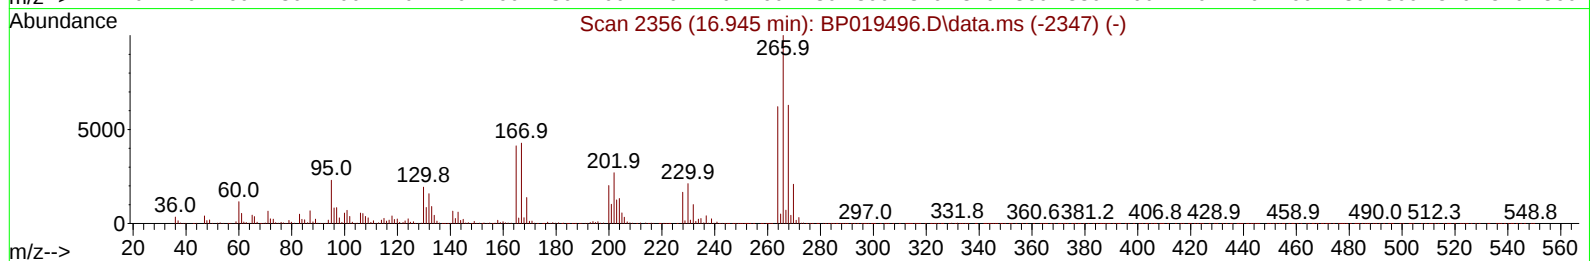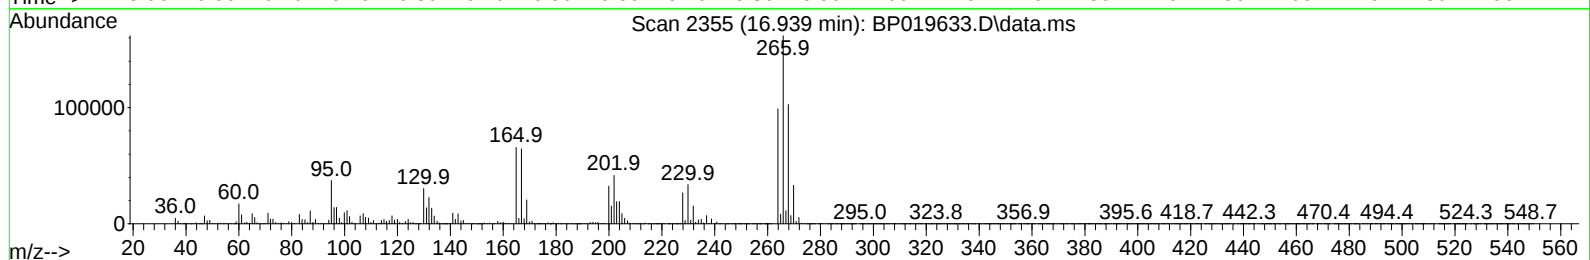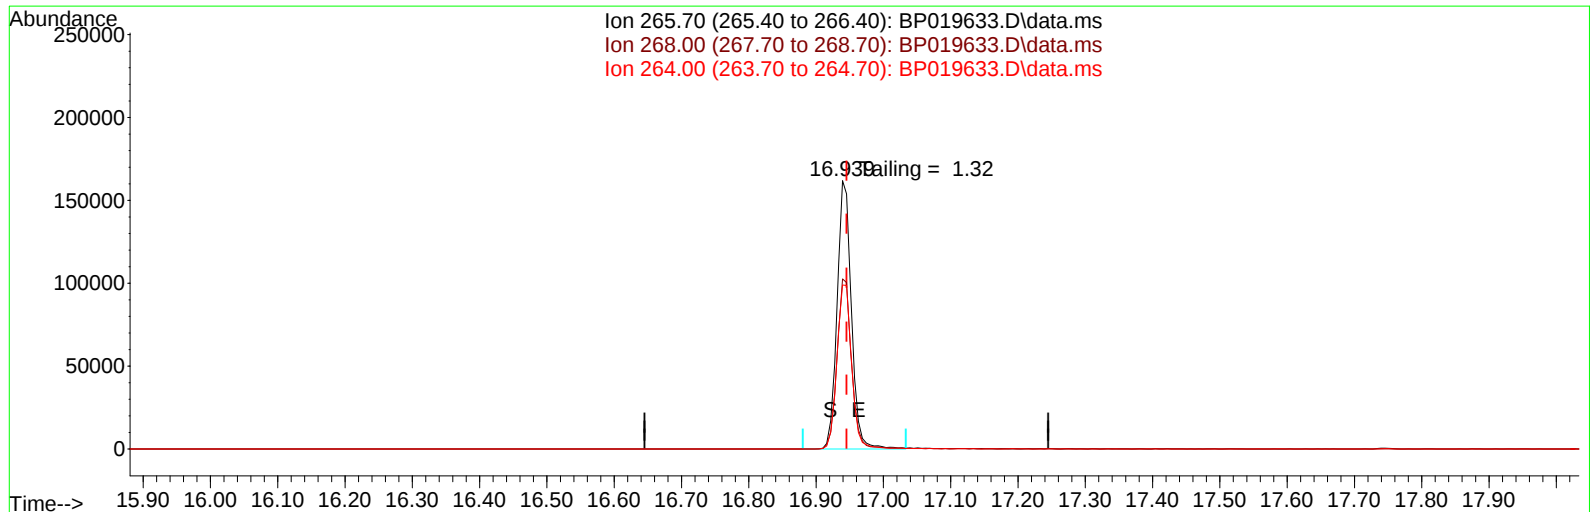

TIC: BP019633.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.006) 1197577.97 ng m

response 239523

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.39
264.00	62.10	61.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/9/2024	BNA_P	<u>BP019633.D</u>
Compound Name	Response	Retention Time
DDT	531735	20.698
DDD	44634	20.269
DDE	757	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45391	577126	7.87

Instrument :
BNA_P
ClientSampleId :
DFTPP