

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021021\
 Data File : BP004705.D
 Acq On : 10 Feb 2021 13:35
 Operator : CG/JU
 Sample : M1329-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.458	44	46	48	rBV2	1270	1189	0.15%	0.034%
2	3.475	48	49	52	rVB3	1591	1151	0.15%	0.033%
3	3.511	52	55	58	rBV6	1258	1359	0.17%	0.038%
4	3.687	82	85	86	rVB3	1287	1262	0.16%	0.036%
5	3.869	114	116	118	rVB3	935	931	0.12%	0.026%
6	3.928	124	126	130	rVB5	1234	1524	0.20%	0.043%
7	3.987	130	136	141	rBV4	2591	5089	0.65%	0.144%
8	4.122	156	159	160	rBV3	970	919	0.12%	0.026%
9	4.317	190	192	196	rBV4	914	1269	0.16%	0.036%
10	4.405	205	207	212	rVB5	1818	2611	0.33%	0.074%
11	4.446	212	214	216	rBV2	1896	2107	0.27%	0.060%
12	4.705	254	258	261	rBV5	1320	1853	0.24%	0.052%
13	5.016	310	311	314	rBV3	752	795	0.10%	0.022%
14	5.481	388	390	394	rVV5	1131	906	0.12%	0.026%
15	5.534	398	399	403	rVB3	926	1026	0.13%	0.029%
16	5.711	428	429	432	rBV3	798	880	0.11%	0.025%
17	5.993	476	477	481	rBV4	811	876	0.11%	0.025%
18	6.346	534	537	540	rVB3	774	1032	0.13%	0.029%
19	6.569	574	575	578	rVB2	1050	857	0.11%	0.024%
20	6.658	589	590	593	rBV3	956	983	0.13%	0.028%
21	6.828	618	619	624	rVB4	915	1310	0.17%	0.037%
22	6.875	624	627	628	rBV3	752	964	0.12%	0.027%
23	7.381	711	713	715	rBV3	786	816	0.10%	0.023%
24	7.669	760	762	764	rBV2	967	944	0.12%	0.027%
25	7.775	773	780	791	rBV	192054	302822	38.78%	8.570%
26	8.075	828	831	834	rBV5	767	1161	0.15%	0.033%
27	8.163	843	846	848	rBV4	727	1029	0.13%	0.029%
28	8.252	859	861	863	rBV3	1020	898	0.12%	0.025%
29	8.528	907	908	912	rBV3	710	805	0.10%	0.023%
30	8.787	948	952	953	rBV2	1050	1270	0.16%	0.036%
31	9.234	1025	1028	1032	rVB6	782	823	0.11%	0.023%
32	9.387	1050	1054	1059	rVB7	855	1546	0.20%	0.044%
33	9.769	1116	1119	1123	rVB4	975	1255	0.16%	0.036%
34	9.804	1123	1125	1127	rBV3	1004	993	0.13%	0.028%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021021\
 Data File : BP004705.D
 Acq On : 10 Feb 2021 13:35
 Operator : CG/JU
 Sample : M1329-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

35	10.569	1247	1255	1266	rBV	234934	399954	51.22%	11.319%
36	10.704	1276	1278	1283	rVB5	948	1404	0.18%	0.040%
37	10.846	1299	1302	1305	rBV3	772	1090	0.14%	0.031%
38	11.257	1370	1372	1376	rVB4	1001	1054	0.13%	0.030%
39	11.410	1396	1398	1402	rBV2	757	842	0.11%	0.024%
40	11.687	1442	1445	1448	rBV4	1002	1461	0.19%	0.041%
41	12.569	1593	1595	1599	rVB4	708	929	0.12%	0.026%
42	12.622	1599	1604	1606	rBV3	902	1533	0.20%	0.043%
43	12.957	1658	1661	1662	rBV3	880	833	0.11%	0.024%
44	13.422	1735	1740	1742	rBV6	611	1096	0.14%	0.031%
45	13.616	1770	1773	1777	rVB4	980	1313	0.17%	0.037%
46	13.669	1779	1782	1785	rVV5	621	1038	0.13%	0.029%
47	13.722	1785	1791	1794	rVB7	867	1921	0.25%	0.054%
48	13.845	1809	1812	1815	rBV4	653	794	0.10%	0.022%
49	14.140	1860	1862	1866	rBV2	1041	1153	0.15%	0.033%
50	14.263	1880	1883	1886	rBV4	602	965	0.12%	0.027%
51	14.422	1903	1910	1918	rBV	373451	544217	69.70%	15.402%
52	14.504	1922	1924	1929	rVB5	1010	1518	0.19%	0.043%
53	15.422	2077	2080	2081	rBV3	952	844	0.11%	0.024%
54	15.445	2081	2084	2089	rVB4	760	1125	0.14%	0.032%
55	15.639	2114	2117	2118	rBV3	933	1050	0.13%	0.030%
56	15.698	2124	2127	2129	rBV3	983	877	0.11%	0.025%
57	15.928	2164	2166	2168	rBV2	774	787	0.10%	0.022%
58	16.134	2198	2201	2203	rBV4	1044	979	0.13%	0.028%
59	16.251	2218	2221	2225	rBV5	665	1000	0.13%	0.028%
60	16.663	2289	2291	2296	rVB5	609	1006	0.13%	0.028%
61	16.798	2310	2314	2316	rVB3	769	895	0.11%	0.025%
62	16.963	2337	2342	2347	rVB5	1804	2733	0.35%	0.077%
63	17.092	2361	2364	2366	rBV4	597	822	0.11%	0.023%
64	17.175	2371	2378	2391	rVV	468535	666378	85.35%	18.860%
65	17.275	2391	2395	2397	rVB5	2182	3095	0.40%	0.088%
66	17.481	2428	2430	2433	rBV4	965	943	0.12%	0.027%
67	17.551	2438	2442	2444	rBV4	911	1471	0.19%	0.042%
68	17.639	2454	2457	2463	rVB7	926	1744	0.22%	0.049%
69	17.704	2466	2468	2470	rVB3	927	892	0.11%	0.025%
70	17.781	2477	2481	2483	rVB3	1323	1770	0.23%	0.050%
71	17.810	2483	2486	2487	rBV3	1475	1621	0.21%	0.046%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021021\
 Data File : BP004705.D
 Acq On : 10 Feb 2021 13:35
 Operator : CG/JU
 Sample : M1329-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

72	17.975	2510	2514	2517	rBV5	873	1647	0.21%	0.047%
73	18.057	2525	2528	2531	rBV5	1375	2351	0.30%	0.067%
74	18.198	2550	2552	2554	rBV2	1069	791	0.10%	0.022%
75	18.286	2565	2567	2570	rVB4	1063	979	0.13%	0.028%
76	18.322	2572	2573	2576	rBV3	1424	1425	0.18%	0.040%
77	18.422	2589	2590	2594	rVB4	1465	1623	0.21%	0.046%
78	18.539	2608	2610	2612	rVB3	1270	796	0.10%	0.023%
79	18.575	2614	2616	2617	rBV2	943	792	0.10%	0.022%
80	18.628	2623	2625	2626	rBV2	1089	844	0.11%	0.024%
81	18.769	2644	2649	2650	rBV4	1830	2435	0.31%	0.069%
82	18.833	2658	2660	2663	rBV4	1371	1344	0.17%	0.038%
83	19.357	2747	2749	2751	rBV3	1770	1785	0.23%	0.051%
84	21.251	3066	3071	3078	rBV	649467	780780	100.00%	22.098%
85	23.557	3457	3463	3473	rVB	376263	737342	94.44%	20.868%




Sum of corrected areas: 3533336

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021021\
Data File : BP004705.D
Acq On : 10 Feb 2021 13:35
Operator : CG/JU
Sample : M1329-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

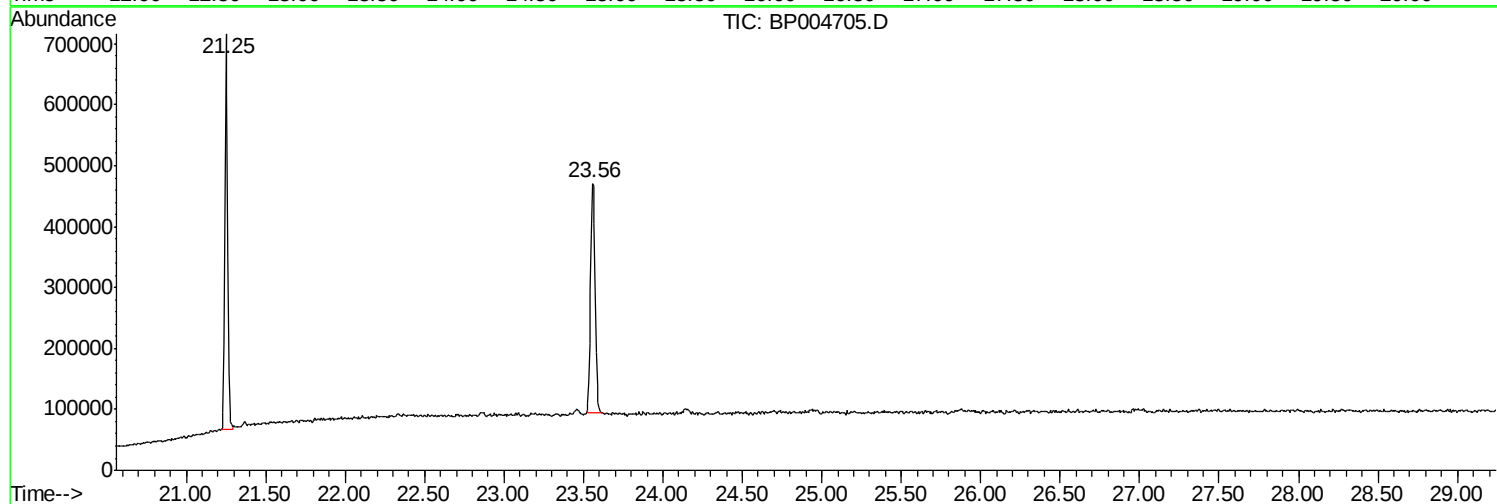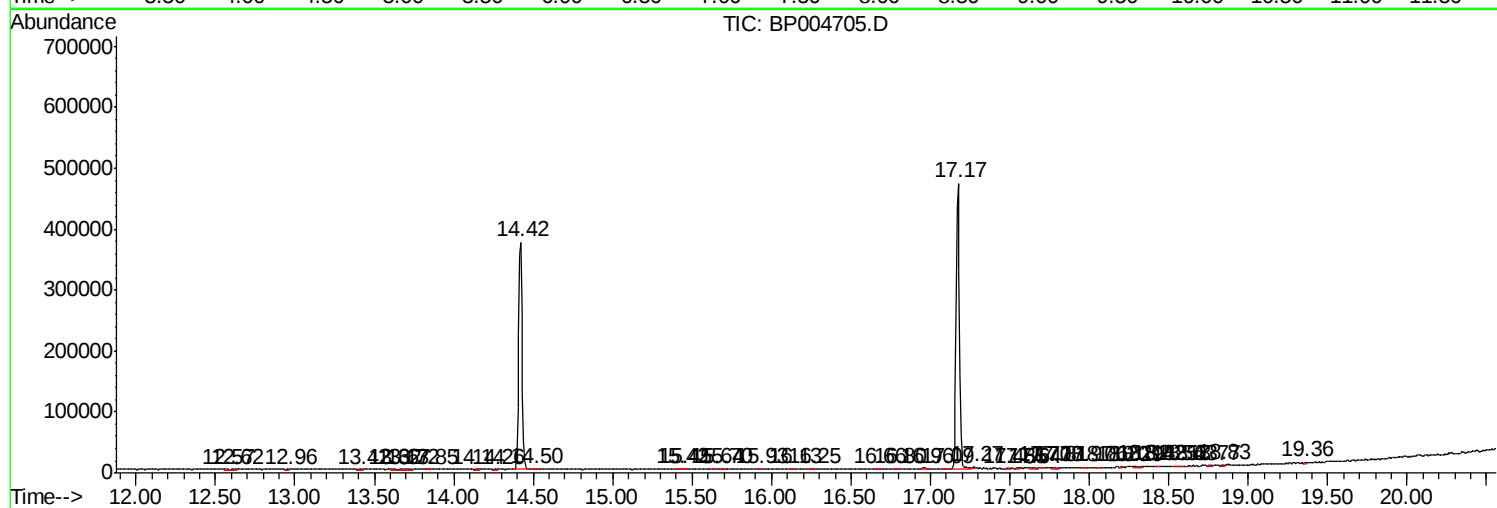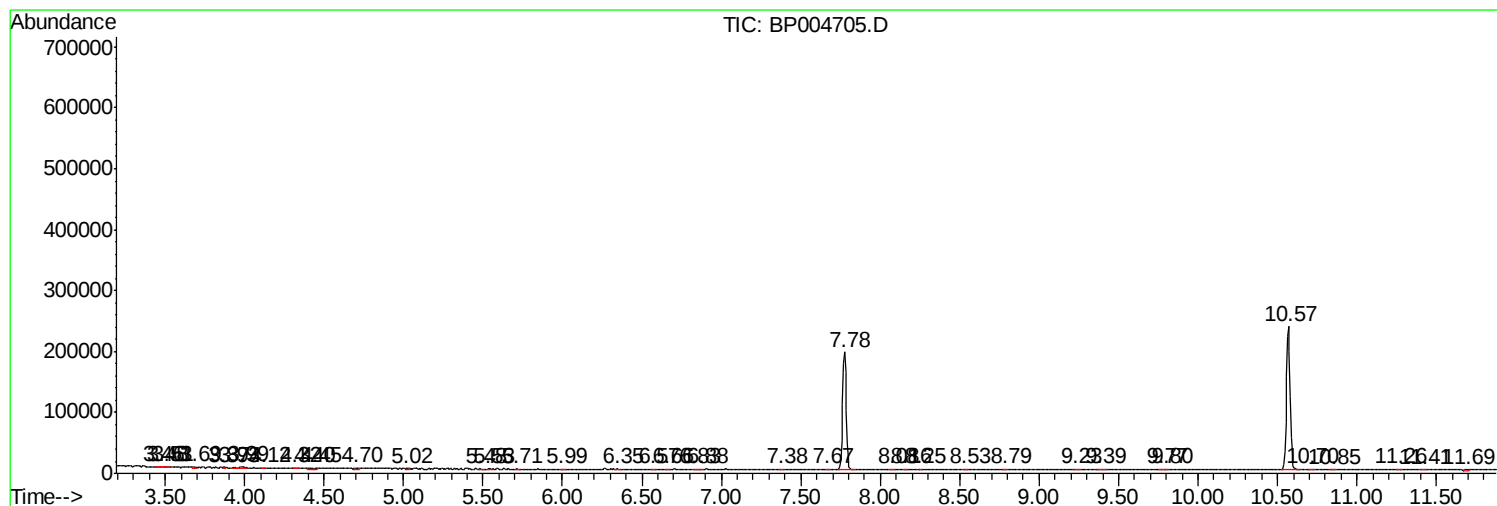

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021021\
Data File : BP004705.D
Acq On : 10 Feb 2021 13:35
Operator : CG/JU
Sample : M1329-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021021\
Data File : BP004705.D
Acq On : 10 Feb 2021 13:35
Operator : CG/JU
Sample : M1329-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
