

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021021\
 Data File : BP004706.D
 Acq On : 10 Feb 2021 14:09
 Operator : CG/JU
 Sample : M1329-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	17	19	22	rVB3	1389	1067	0.16%	0.036%
2	3.328	22	24	26	rVB3	1758	1368	0.21%	0.046%
3	3.358	26	29	31	rBV4	1266	1668	0.25%	0.056%
4	3.464	45	47	49	rVB3	1076	927	0.14%	0.031%
5	3.675	81	83	85	rBV3	1313	855	0.13%	0.029%
6	3.946	127	129	132	rBV4	1169	887	0.14%	0.030%
7	3.987	132	136	141	rVV6	2682	3412	0.52%	0.115%
8	4.123	157	159	160	rBV	1703	979	0.15%	0.033%
9	4.152	162	164	167	rVB3	1257	1168	0.18%	0.039%
10	4.275	181	185	187	rBV3	1052	1186	0.18%	0.040%
11	4.346	194	197	200	rVB5	1056	1603	0.24%	0.054%
12	4.405	206	207	212	rVB5	1584	1605	0.25%	0.054%
13	4.464	215	217	220	rVB4	1318	1008	0.15%	0.034%
14	4.746	263	265	269	rBV5	886	715	0.11%	0.024%
15	4.822	276	278	281	rBV4	664	738	0.11%	0.025%
16	5.017	309	311	314	rVB4	1042	1055	0.16%	0.036%
17	5.370	367	371	375	rBV5	1459	2004	0.31%	0.068%
18	5.569	403	405	409	rBV4	908	1198	0.18%	0.040%
19	5.652	415	419	421	rBV5	684	976	0.15%	0.033%
20	5.728	430	432	435	rBV3	931	1286	0.20%	0.043%
21	6.275	523	525	527	rBV3	746	737	0.11%	0.025%
22	6.311	527	531	532	rVB3	851	1106	0.17%	0.037%
23	6.464	555	557	560	rBV4	636	861	0.13%	0.029%
24	6.628	583	585	586	rBV2	939	715	0.11%	0.024%
25	6.693	593	596	598	rBV4	499	772	0.12%	0.026%
26	6.858	622	624	626	rVB3	1324	889	0.14%	0.030%
27	6.875	626	627	630	rBV3	932	976	0.15%	0.033%
28	6.911	632	633	637	rBV4	916	845	0.13%	0.029%
29	6.952	638	640	642	rVB3	893	773	0.12%	0.026%
30	7.164	675	676	679	rBV3	781	911	0.14%	0.031%
31	7.769	773	779	788	rVB	158958	249803	38.18%	8.441%
32	8.163	841	846	852	rBV7	1090	2865	0.44%	0.097%
33	8.522	902	907	908	rBV3	810	1131	0.17%	0.038%
34	8.652	926	929	930	rBV3	901	794	0.12%	0.027%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021021\
 Data File : BP004706.D
 Acq On : 10 Feb 2021 14:09
 Operator : CG/JU
 Sample : M1329-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

35	8.675	930	933	935	rVV4	930	931	0.14%	0.031%
36	8.693	935	936	940	rVV3	874	732	0.11%	0.025%
37	9.016	987	991	992	rVB4	811	908	0.14%	0.031%
38	9.040	992	995	997	rBV4	673	818	0.13%	0.028%
39	9.269	1032	1034	1037	rBV4	602	853	0.13%	0.029%
40	9.305	1037	1040	1042	rVB3	643	714	0.11%	0.024%
41	9.405	1054	1057	1060	rBV4	895	1142	0.17%	0.039%
42	9.540	1076	1080	1082	rBV3	925	1063	0.16%	0.036%
43	9.605	1088	1091	1096	rBV7	776	1392	0.21%	0.047%
44	9.663	1099	1101	1105	rVB2	970	910	0.14%	0.031%
45	9.699	1105	1107	1108	rBV	985	752	0.11%	0.025%
46	9.934	1145	1147	1150	rBV4	842	1070	0.16%	0.036%
47	9.963	1150	1152	1154	rBV4	890	866	0.13%	0.029%
48	10.034	1161	1164	1166	rBV3	712	869	0.13%	0.029%
49	10.246	1195	1200	1203	rVB6	564	972	0.15%	0.033%
50	10.563	1247	1254	1263	rBV	199200	324345	49.57%	10.960%
51	11.116	1345	1348	1349	rBV2	1056	766	0.12%	0.026%
52	11.199	1359	1362	1365	rBV3	763	706	0.11%	0.024%
53	11.446	1400	1404	1405	rBV4	772	907	0.14%	0.031%
54	11.628	1432	1435	1436	rBV3	780	799	0.12%	0.027%
55	11.704	1443	1448	1449	rBV4	557	871	0.13%	0.029%
56	11.752	1454	1456	1460	rVV4	681	763	0.12%	0.026%
57	11.799	1460	1464	1467	rVB6	473	778	0.12%	0.026%
58	11.828	1467	1469	1472	rBV4	734	766	0.12%	0.026%
59	12.281	1542	1546	1548	rVB5	651	919	0.14%	0.031%
60	12.334	1548	1555	1557	rBV8	605	1138	0.17%	0.038%
61	12.940	1653	1658	1662	rVB6	566	908	0.14%	0.031%
62	13.128	1687	1690	1692	rBV3	654	804	0.12%	0.027%
63	13.716	1787	1790	1793	rBV3	738	805	0.12%	0.027%
64	13.863	1813	1815	1817	rBV4	710	704	0.11%	0.024%
65	13.946	1823	1829	1830	rBV6	487	836	0.13%	0.028%
66	14.240	1876	1879	1880	rBV3	847	879	0.13%	0.030%
67	14.251	1880	1881	1887	rVB4	969	1051	0.16%	0.036%
68	14.416	1901	1909	1921	rBV	306820	446771	68.28%	15.097%
69	14.645	1947	1948	1953	rBV4	848	772	0.12%	0.026%
70	14.893	1987	1990	1992	rVV3	747	925	0.14%	0.031%
71	15.181	2035	2039	2041	rBV4	708	933	0.14%	0.032%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021021\
 Data File : BP004706.D
 Acq On : 10 Feb 2021 14:09
 Operator : CG/JU
 Sample : M1329-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

72	15.234	2046	2048	2051	rBV4	609	785	0.12%	0.027%
73	15.298	2057	2059	2060	rBV2	916	772	0.12%	0.026%
74	15.587	2103	2108	2110	rBV3	647	766	0.12%	0.026%
75	15.622	2110	2114	2115	rVB4	740	867	0.13%	0.029%
76	15.657	2117	2120	2123	rVB5	741	868	0.13%	0.029%
77	15.775	2138	2140	2143	rBV4	680	841	0.13%	0.028%
78	15.928	2162	2166	2168	rBV4	680	814	0.12%	0.028%
79	16.192	2207	2211	2212	rBV4	713	843	0.13%	0.028%
80	16.545	2270	2271	2274	rBV2	853	855	0.13%	0.029%
81	16.957	2336	2341	2344	rBV6	1878	2731	0.42%	0.092%
82	17.110	2366	2367	2371	rVB4	909	946	0.14%	0.032%
83	17.169	2371	2377	2387	rBV	393172	552587	84.45%	18.673%
84	17.263	2392	2393	2400	rVB3	1466	1908	0.29%	0.064%
85	17.604	2449	2451	2455	rBV5	770	1395	0.21%	0.047%
86	17.810	2484	2486	2490	rVB5	733	949	0.15%	0.032%
87	17.839	2490	2491	2494	rBV3	1171	939	0.14%	0.032%
88	17.863	2494	2495	2498	rBV2	633	747	0.11%	0.025%
89	17.922	2502	2505	2507	rBV4	1041	1146	0.18%	0.039%
90	17.963	2510	2512	2513	rBV2	1205	889	0.14%	0.030%
91	18.016	2520	2521	2523	rBV2	1074	822	0.13%	0.028%
92	18.098	2532	2535	2538	rBV5	1320	1537	0.23%	0.052%
93	18.181	2547	2549	2552	rBV3	963	1083	0.17%	0.037%
94	18.310	2569	2571	2573	rBV3	1118	810	0.12%	0.027%
95	18.457	2591	2596	2600	rBV7	1786	3245	0.50%	0.110%
96	18.657	2629	2630	2632	rBV2	1319	1143	0.17%	0.039%
97	18.810	2653	2656	2659	rBV5	1533	1900	0.29%	0.064%
98	18.869	2665	2666	2668	rBV2	1138	1086	0.17%	0.037%
99	21.251	3066	3071	3079	rBV	534020	654298	100.00%	22.109%
100	23.557	3456	3463	3473	rVB	327037	630767	96.40%	21.314%


Sum of corrected areas: 2959360

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021021\
Data File : BP004706.D
Acq On : 10 Feb 2021 14:09
Operator : CG/JU
Sample : M1329-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

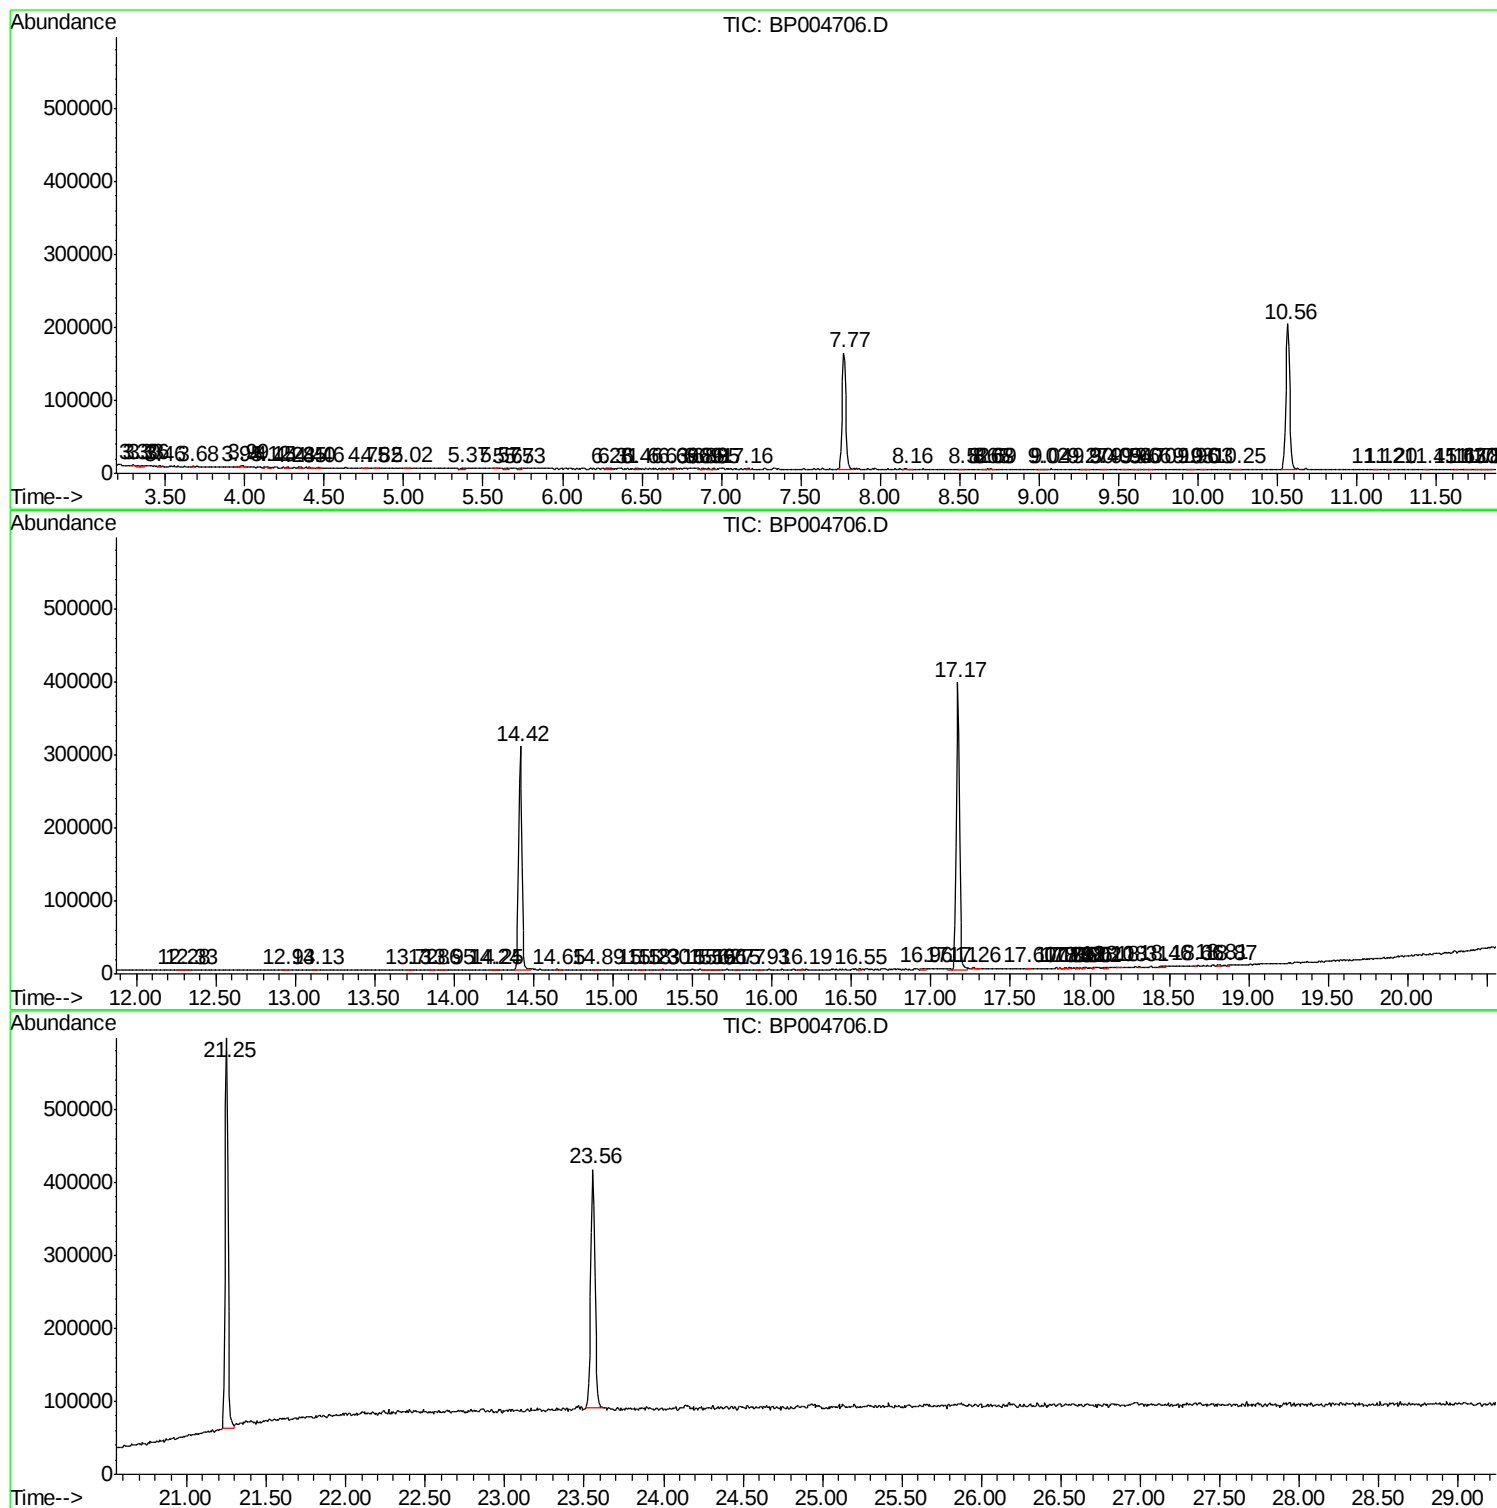

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021021\
Data File : BP004706.D
Acq On : 10 Feb 2021 14:09
Operator : CG/JU
Sample : M1329-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021021\
Data File : BP004706.D
Acq On : 10 Feb 2021 14:09
Operator : CG/JU
Sample : M1329-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc