
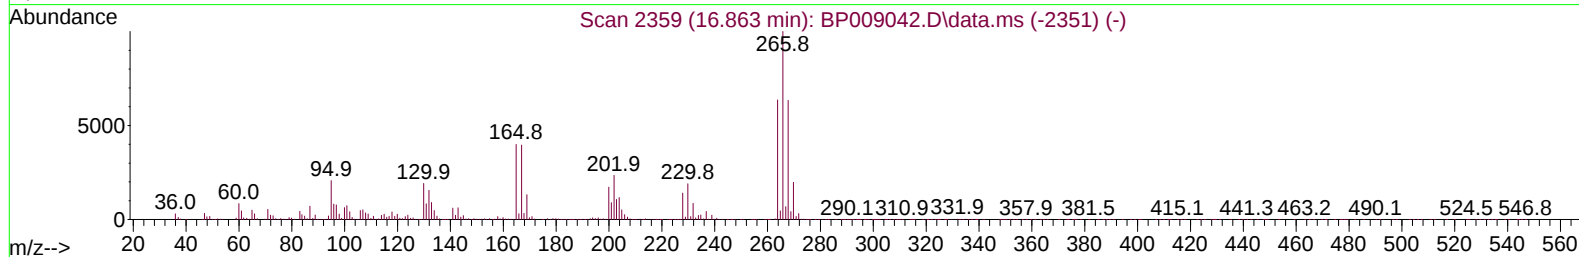
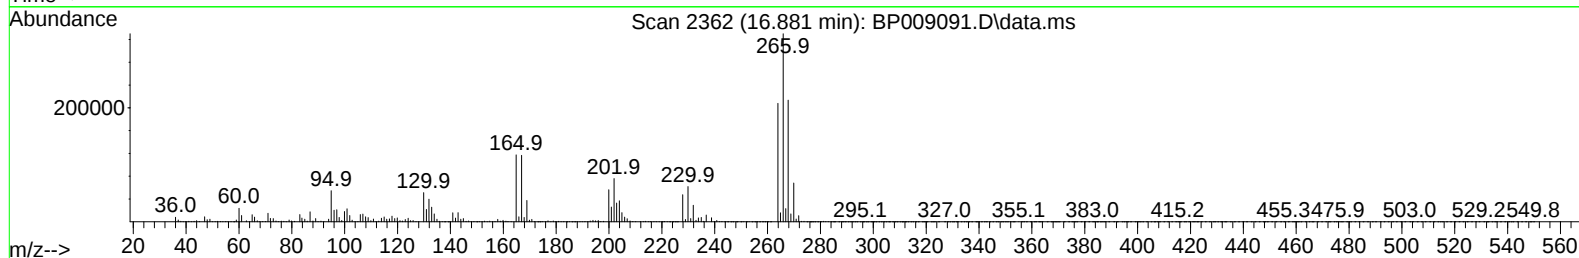


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021022\
Data File : BP009091.D
Acq On : 10 Feb 2022 09:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 13:58:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 15:13:17 2022
Response via : Initial Calibration

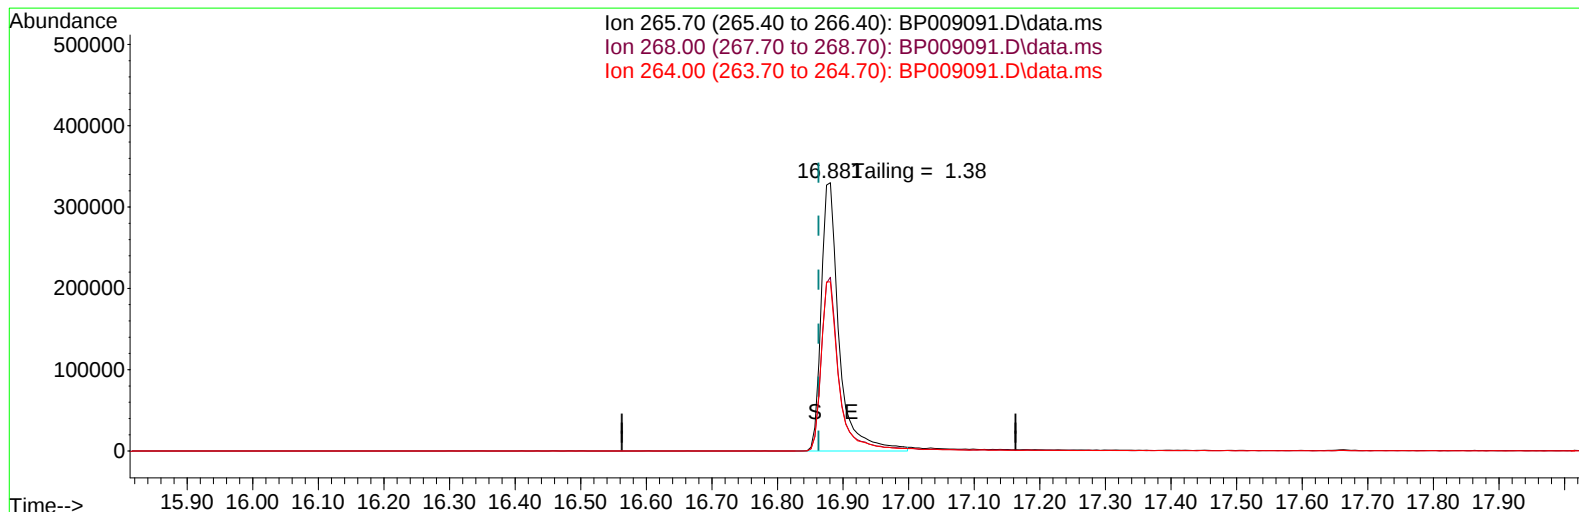

TIC: BP009091.D\data.ms

(70) Pentachlorophenol (C)




16.881min (+ 0.018) 1751262.46 ng

response 634394

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.73
264.00	62.90	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021022\
Data File : BP009091.D
Acq On : 10 Feb 2022 09:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 13:58:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 15:13:17 2022
Response via : Initial Calibration

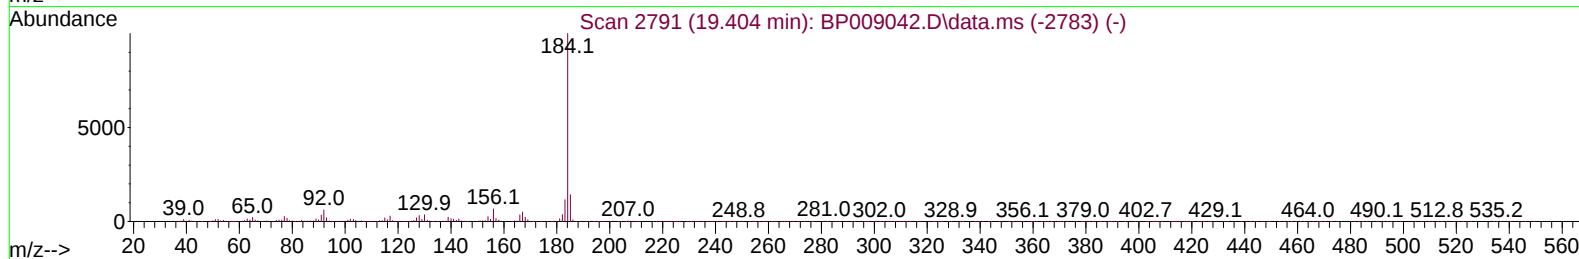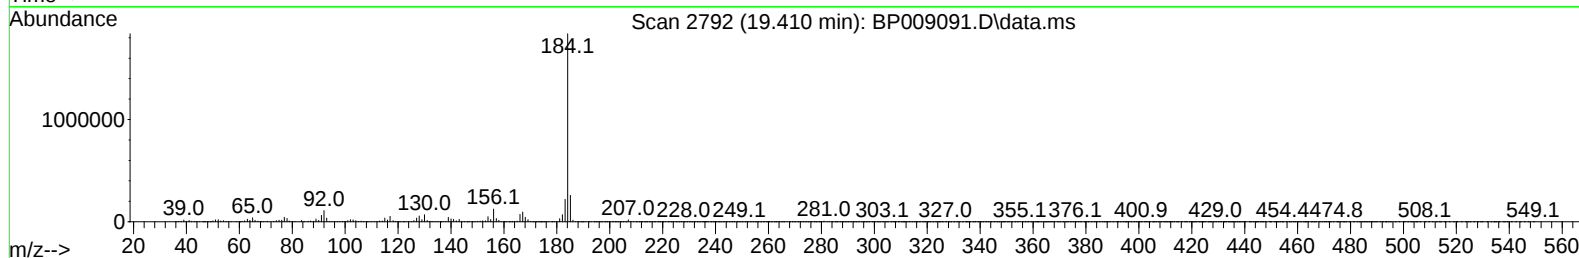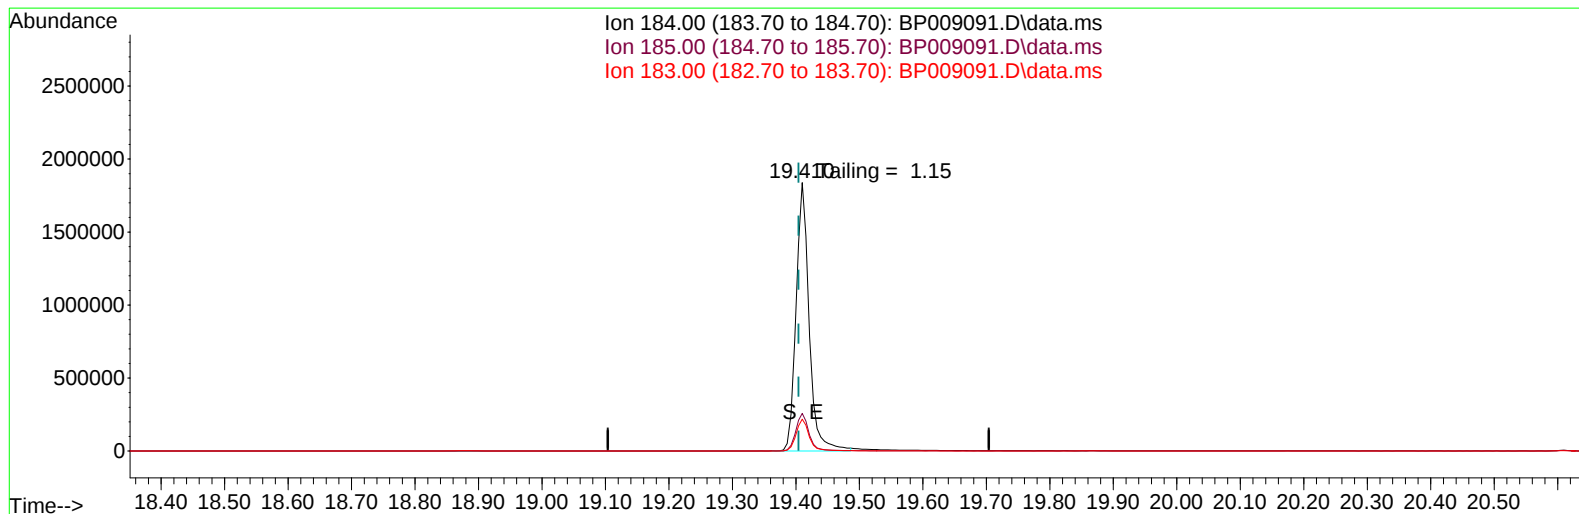

TIC: BP009091.D\data.ms

(77) Benzidine**19.410min (+ 0.006) 771026.22 ng****response 2690600**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.01
183.00	11.90	11.89
0.00	0.00	0.00