

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021022\
 Data File : BP009093.D
 Acq On : 10 Feb 2022 11:29
 Operator : CG/JU
 Sample : PB142564BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142564BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	12	rVB	136042	143012	1.57%	0.301%
2	5.405	405	411	432	rBV	3274574	5114885	56.30%	10.774%
3	7.005	675	683	710	rBV	2783032	4992068	54.95%	10.515%
4	7.810	812	820	829	rBV	678502	1136844	12.51%	2.395%
5	8.969	1009	1017	1037	rBV	1848665	3311318	36.45%	6.975%
6	10.604	1285	1295	1313	rBV	781247	1507863	16.60%	3.176%
7	13.075	1707	1715	1748	rBV	5415686	8489668	93.44%	17.883%
8	14.451	1942	1949	1973	rBV	1264222	2099925	23.11%	4.423%
9	15.951	2197	2204	2228	rBV	3060023	5689301	62.62%	11.984%
10	17.210	2411	2418	2433	rBV	1345439	2192406	24.13%	4.618%
11	19.774	2848	2854	2864	rBV	7120780	9085482	100.00%	19.138%
12	21.310	3110	3115	3125	rBV	1277475	1916409	21.09%	4.037%
13	23.715	3518	3524	3535	rVB2	818494	1794246	19.75%	3.779%




Sum of corrected areas: 47473427

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021022\
Data File : BP009093.D
Acq On : 10 Feb 2022 11:29
Operator : CG/JU
Sample : PB142564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142564BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

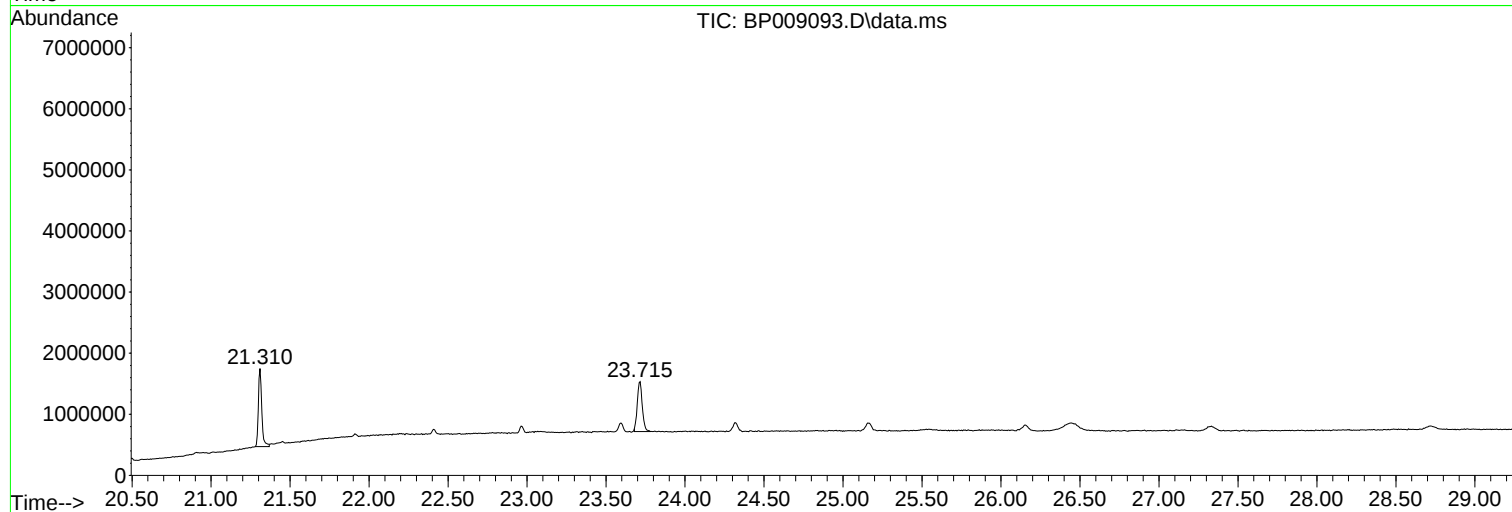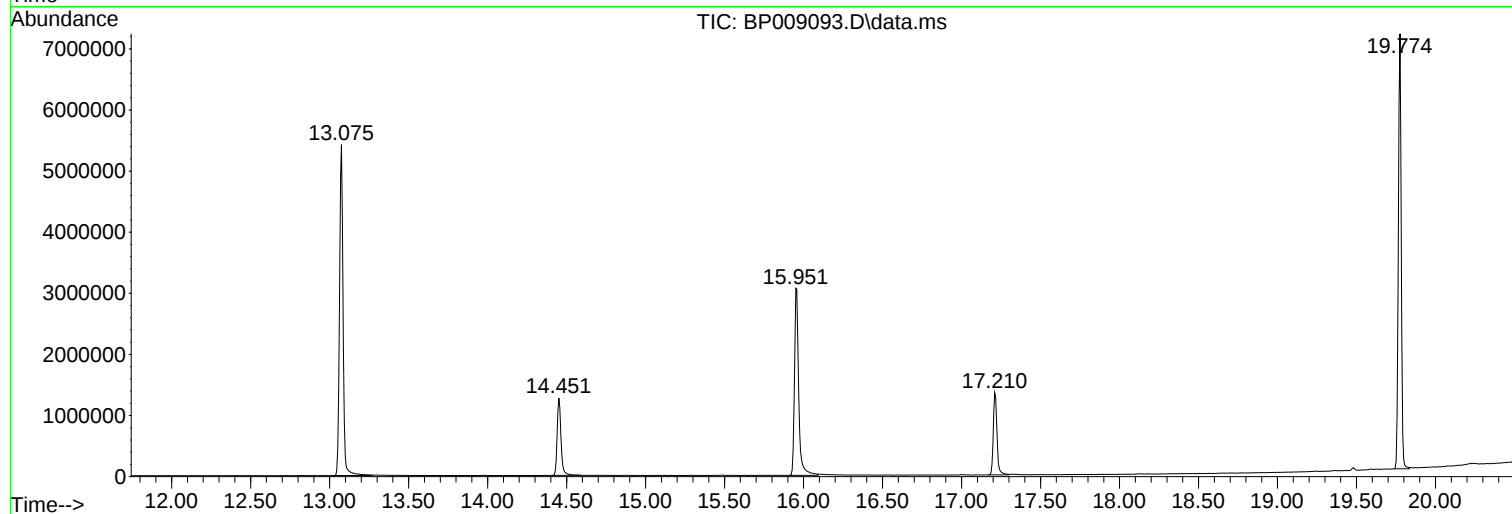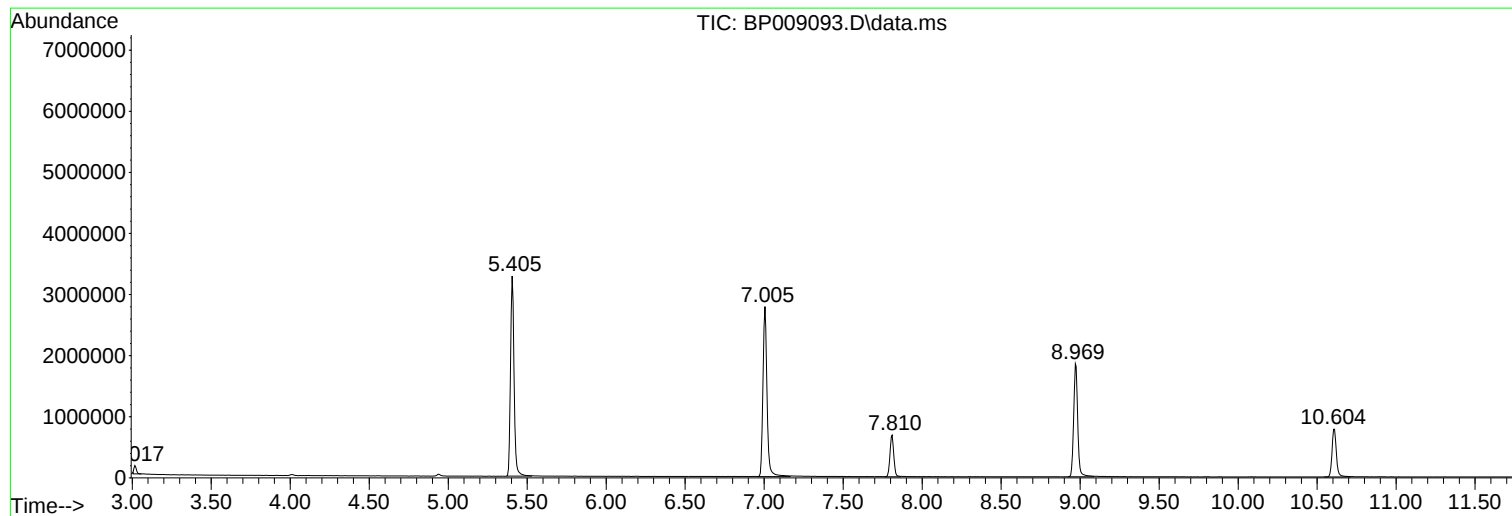

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021022\
Data File : BP009093.D
Acq On : 10 Feb 2022 11:29
Operator : CG/JU
Sample : PB142564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142564BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.017	2.52 ng	143012	1,4-Dichlorobenzene-d4	7.810

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	33
3			1-(2-Methoxyethoxy)-2-methyl-2-p...	162	C8H18O3	1000364-24-4	17
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	12

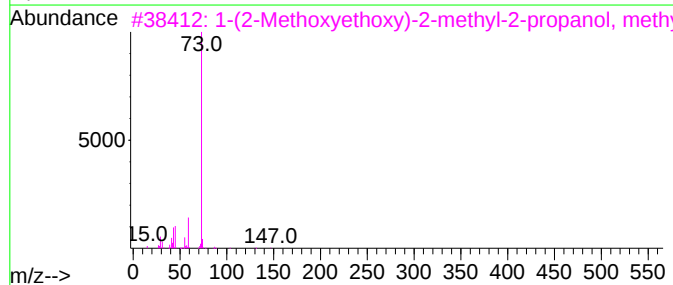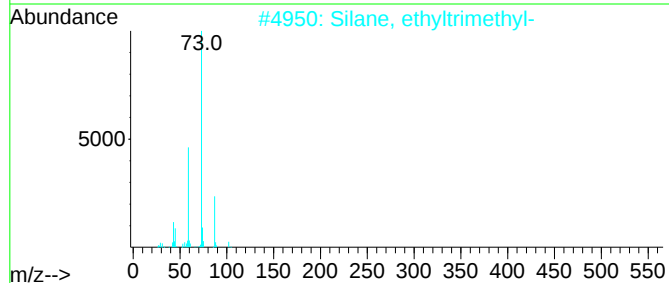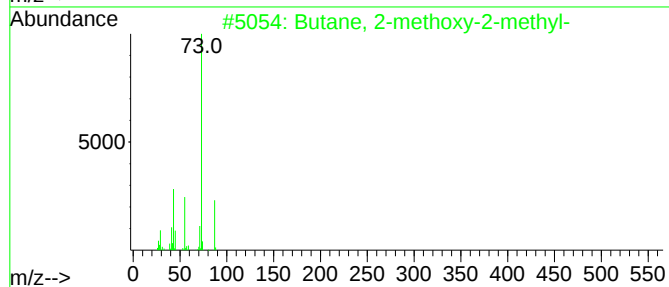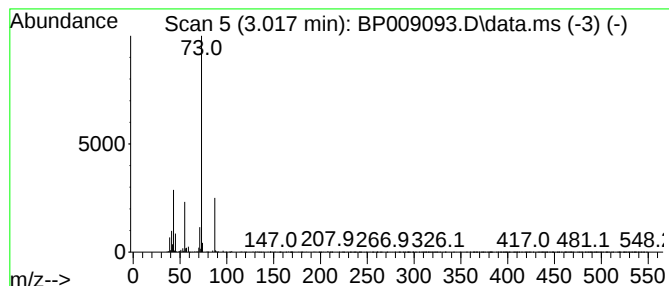

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021022\
Data File : BP009093.D
Acq On : 10 Feb 2022 11:29
Operator : CG/JU
Sample : PB142564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142564BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.017	2.5	ng	143012	1	7.810	1136840	20.0