
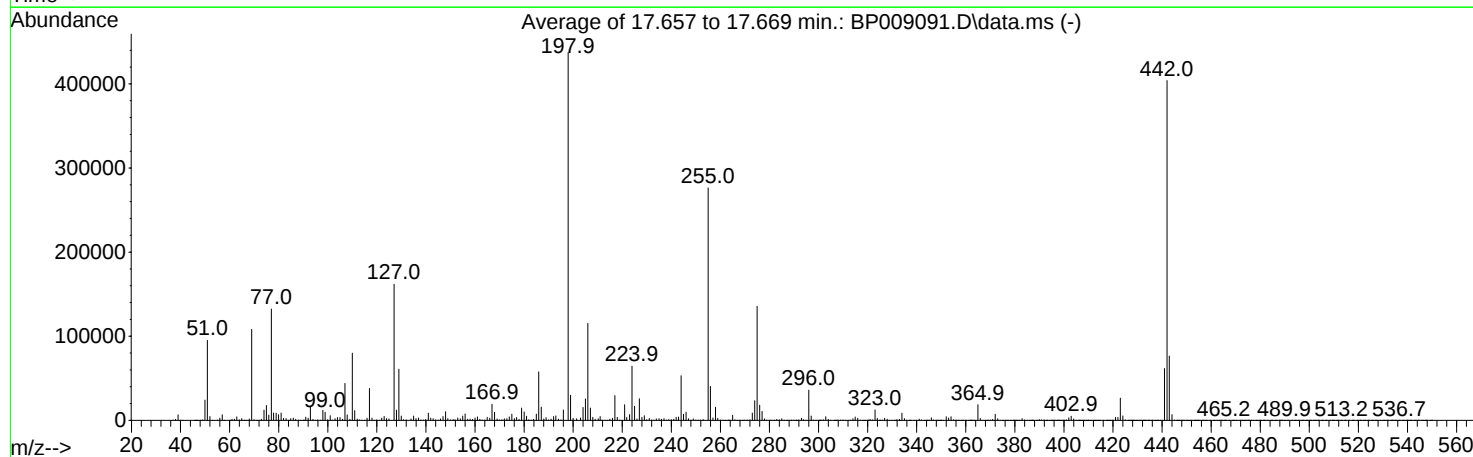


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021022\
 Data File : BP009091.D
 Acq On : 10 Feb 2022 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 07 15:13:17 2022

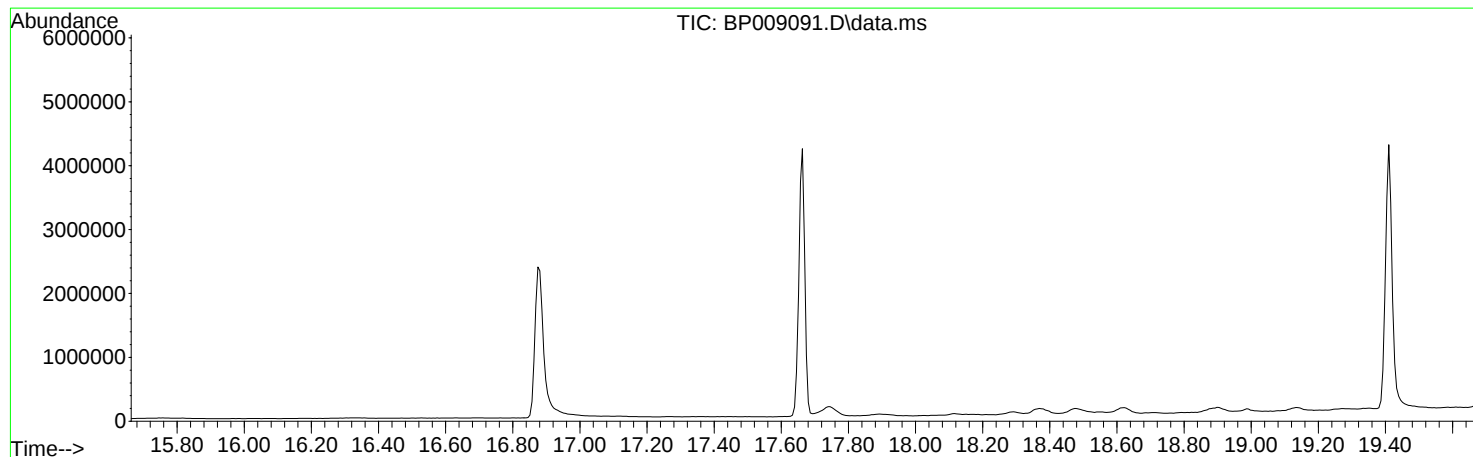




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.8	95213	PASS
68	69	0.00	2	1.7	1793	PASS
69	198	0.00	100	24.7	108190	PASS
70	69	0.00	2	0.6	693	PASS
127	198	10	80	37.0	161866	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	437331	PASS
199	198	5	9	6.8	29792	PASS
275	198	10	60	31.0	135713	PASS
365	198	1	100	4.3	18588	PASS
441	198	0.01	100	14.1	61603	PASS
442	442	100	100	100.0	403968	PASS
443	442	15	24	18.9	76456	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021022\
Data File : BP009091.D
Acq On : 10 Feb 2022 09:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 10 13:58:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 15:13:17 2022
Response via : Initial Calibration

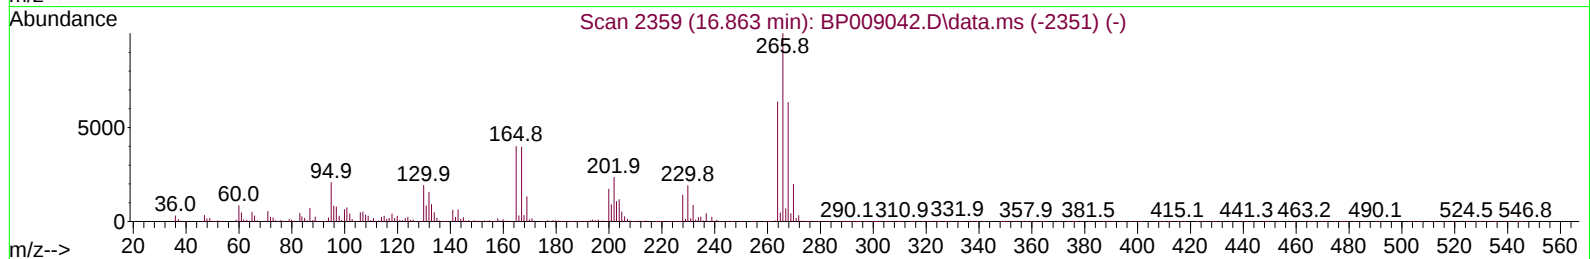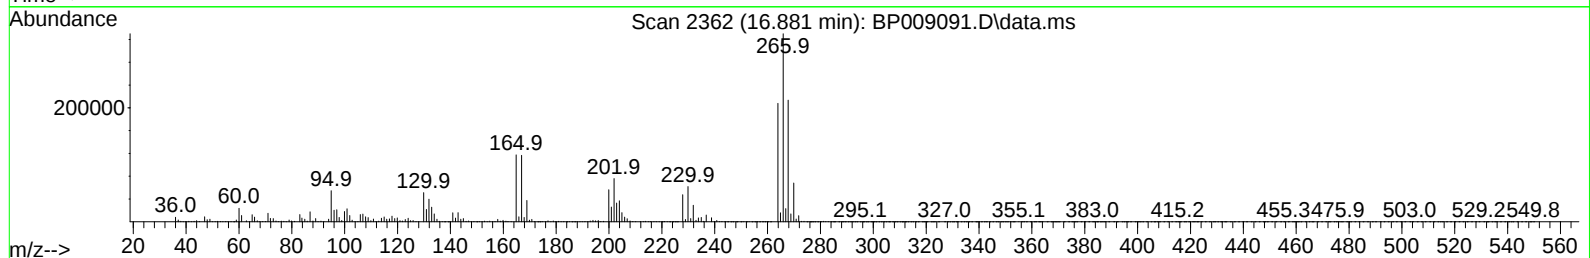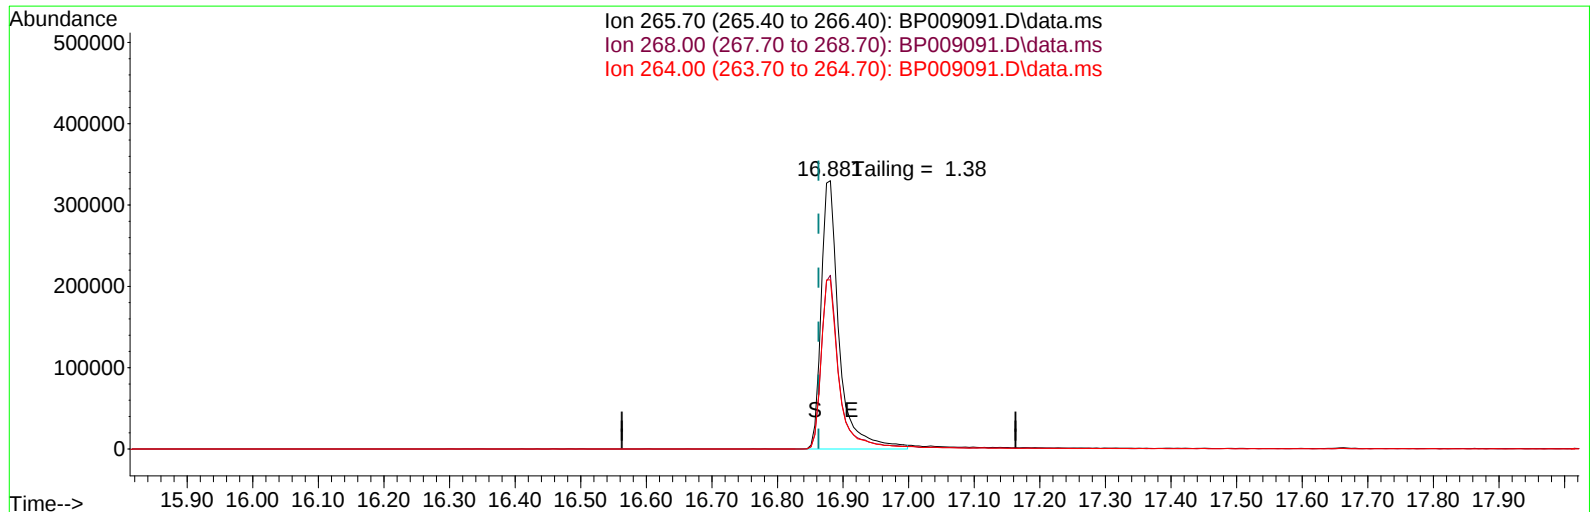

TIC: BP009091.D\data.ms

(70) Pentachlorophenol (C)

16.881min (+ 0.018) 1751262.46 ng




response 634394

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.73
264.00	62.90	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021022\
Data File : BP009091.D
Acq On : 10 Feb 2022 09:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 10 13:58:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 15:13:17 2022
Response via : Initial Calibration

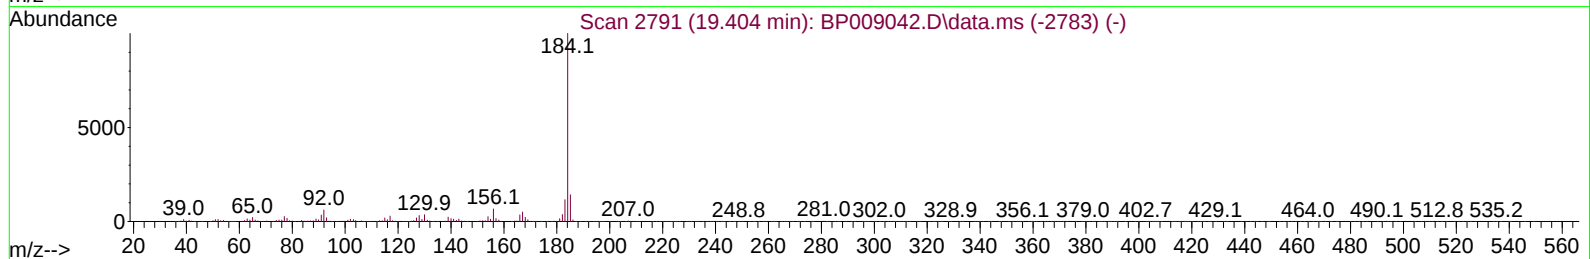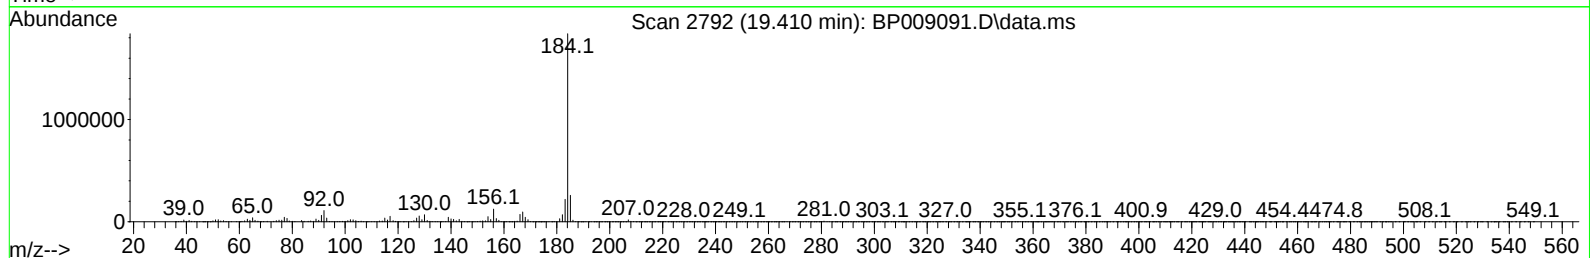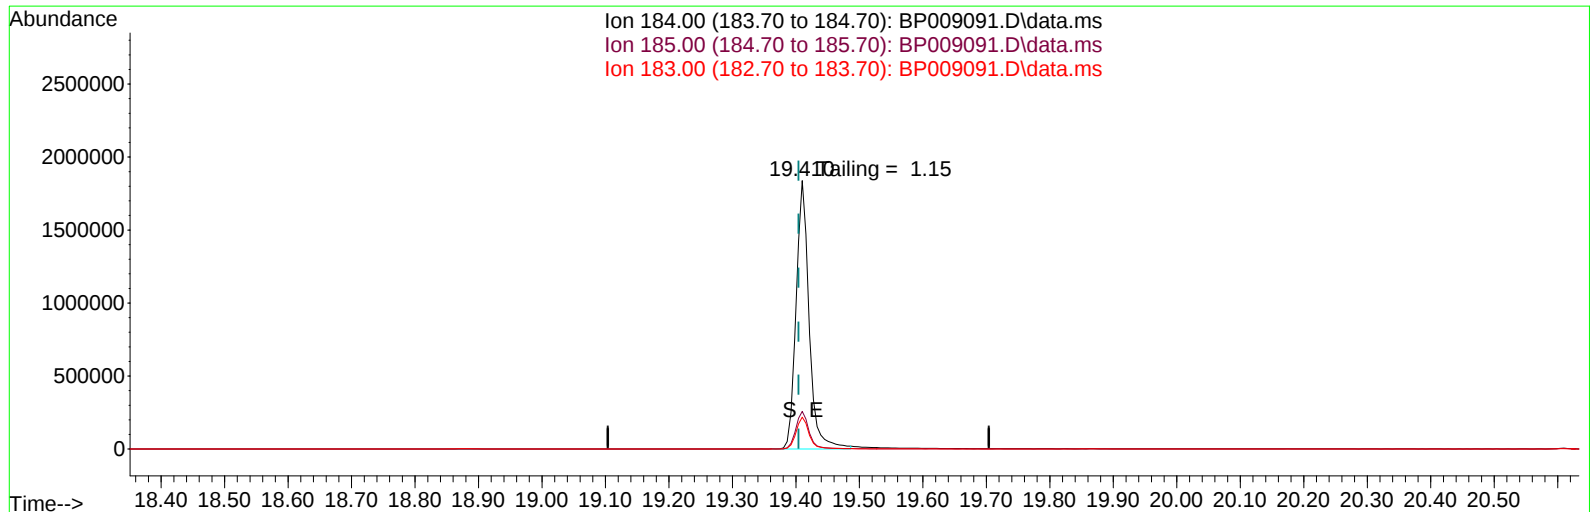

TIC: BP009091.D\data.ms

(77) Benzidine

19.410min (+ 0.006) 771026.22 ng

response 2690600

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.01
183.00	11.90	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/10/2022	BNA_P	<u>BP009091.D</u>
Compound Name	Response	Retention Time
DDT	1433052	20.61
DDD	38762	20.18
DDE	2911	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41673	1474725	2.83