

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
 Data File : BP024015.D
 Acq On : 10 Feb 2025 16:31
 Operator : RC/JU
 Sample : Q1336-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29C9

Quant Time: Feb 12 14:39:01 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.764	152	386623	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.540	136	1691169	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.387	164	1067417	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.169	188	2108944	20.000	ng/u1	-0.02
79) Chrysene-d12	21.610	240	1976664	20.000	ng/u1	-0.03
88) Perylene-d12	24.957	264	1985923	20.000	ng/u1	-0.05
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	50504	5.427	ng/uL	0.00
4) Pyridine-d5	3.711	84	108514	4.041	ng/u1	0.00
7) Phenol-d5	6.952	99	251508	7.351	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	494362	27.297	ng/u1	0.00
11) 2-Chlorophenol-d4	7.311	132	645443	24.023	ng/u1	0.00
15) 4-Methylphenol-d8	8.469	113	494687	17.699	ng/u1	0.00
21) Nitrobenzene-d5	8.911	128	341950	25.273	ng/u1	0.00
24) 2-Nitrophenol-d4	9.622	143	342481	23.458	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.169	165	682611	25.487	ng/u1	0.00
31) 4-Chloroaniline-d4	10.675	131	709521	17.714	ng/u1	0.00
46) Dimethylphthalate-d6	13.793	166	2256341	28.339	ng/u1	0.00
49) Acenaphthylene-d8	14.075	160	2465675	27.458	ng/u1	0.00
54) 4-Nitrophenol-d4	14.610	143	72906	4.611	ng/u1	0.00
60) Fluorene-d10	15.387	176	1983411	29.582	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.510	200	239131	18.380	ng/u1	0.00
73) Anthracene-d10	17.275	188	3337802	32.234	ng/u1	-0.01
81) Pyrene-d10	19.639	212	3791613	35.799	ng/u1	-0.02
92) Benzo(a)pyrene-d12	24.727	264	3286922	31.722	ng/u1	-0.05
Target Compounds						
					Qvalue	
8) Phenol	6.975	94	49217	1.401	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024015.D
Acq On : 10 Feb 2025 16:31
Operator : RC/JU
Sample : Q1336-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29C9

Quant Time: Feb 12 14:39:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

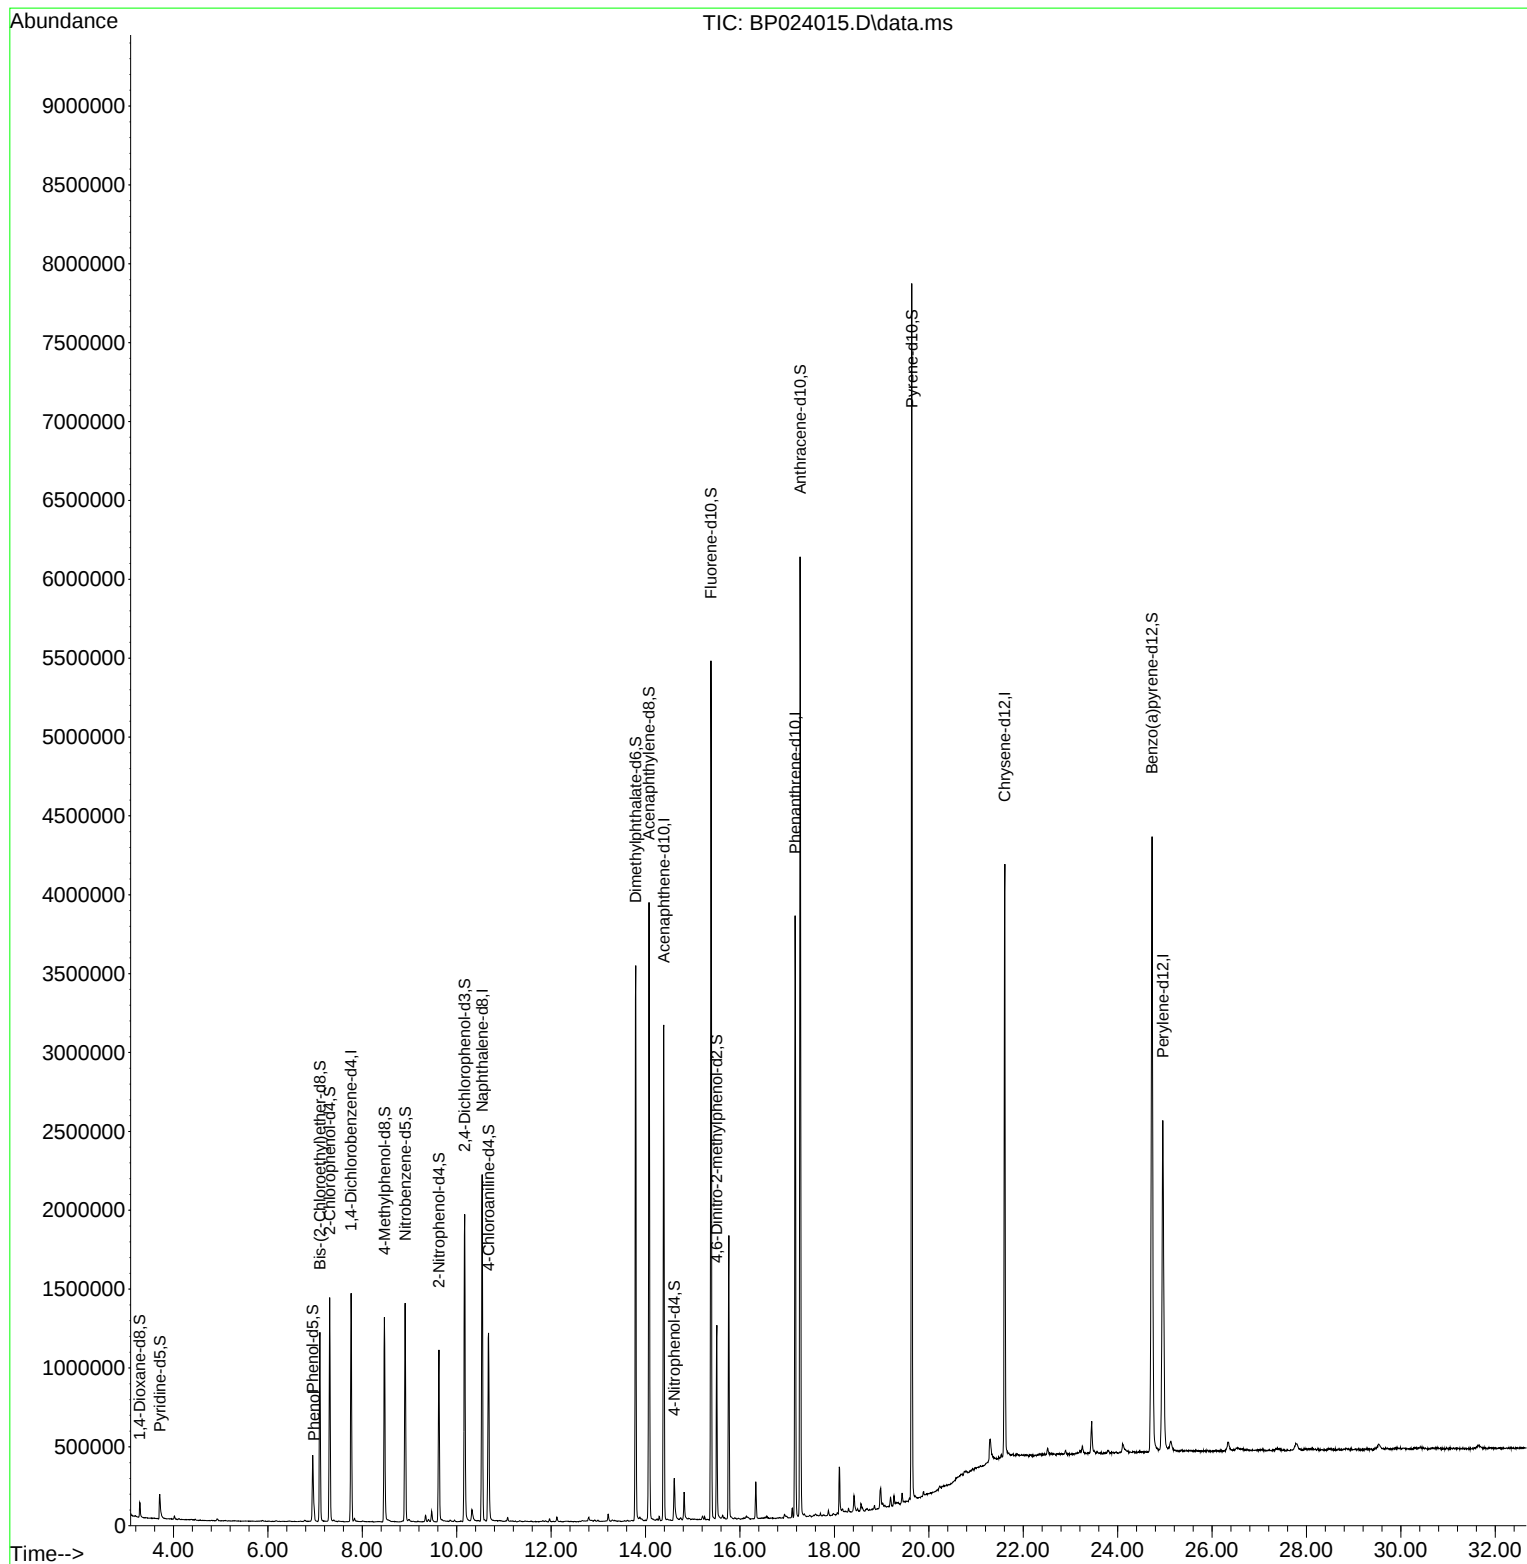

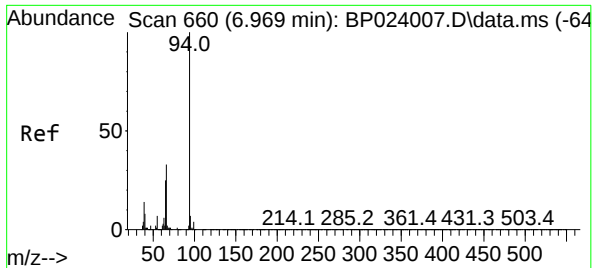

#8
Phenol
Concen: 1.401 ng/ul
RT: 6.975 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP024015.D
Acq: 10 Feb 2025 16:31

Instrument :
BNA_P
ClientSampleId :
E29C9

Tgt Ion:	94	Resp:	49217
Ion	Ratio	Lower	Upper
94	100		
65	27.0	20.1	30.1
66	34.3	26.0	39.0

