

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
 Data File : BP024016.D
 Acq On : 10 Feb 2025 17:12
 Operator : RC/JU
 Sample : Q1336-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29D1

Quant Time: Feb 12 14:43:29 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.764	152	408760	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.534	136	1755750	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.381	164	1081599	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.169	188	2192087	20.000	ng/u1	-0.02
79) Chrysene-d12	21.616	240	2045217	20.000	ng/u1	-0.02
88) Perylene-d12	24.963	264	2105800	20.000	ng/u1	-0.05
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	50912	5.175	ng/uL	0.00
4) Pyridine-d5	3.705	84	154418	5.440	ng/u1	0.00
7) Phenol-d5	6.952	99	357727	9.889	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.099	67	648752	33.882	ng/u1	0.00
11) 2-Chlorophenol-d4	7.305	132	883198	31.091	ng/u1	-0.01
15) 4-Methylphenol-d8	8.469	113	653852	22.127	ng/u1	0.00
21) Nitrobenzene-d5	8.905	128	454572	32.361	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.622	143	474384	31.298	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.163	165	927999	33.374	ng/u1	0.00
31) 4-Chloroaniline-d4	10.669	131	700916	16.855	ng/u1	0.00
46) Dimethylphthalate-d6	13.787	166	2690294	33.347	ng/u1	0.00
49) Acenaphthylene-d8	14.069	160	3169763	34.836	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.598	143	107656	6.719	ng/u1	-0.01
60) Fluorene-d10	15.387	176	2485851	36.589	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.504	200	336387	24.874	ng/u1	0.00
73) Anthracene-d10	17.275	188	3962659	36.817	ng/u1	-0.01
81) Pyrene-d10	19.645	212	4510241	41.157	ng/u1	-0.02
92) Benzo(a)pyrene-d12	24.739	264	3987902	36.296	ng/u1	-0.04
Target Compounds						
					Qvalue	
8) Phenol	6.975	94	78260	2.107	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024016.D
Acq On : 10 Feb 2025 17:12
Operator : RC/JU
Sample : Q1336-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29D1

Quant Time: Feb 12 14:43:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

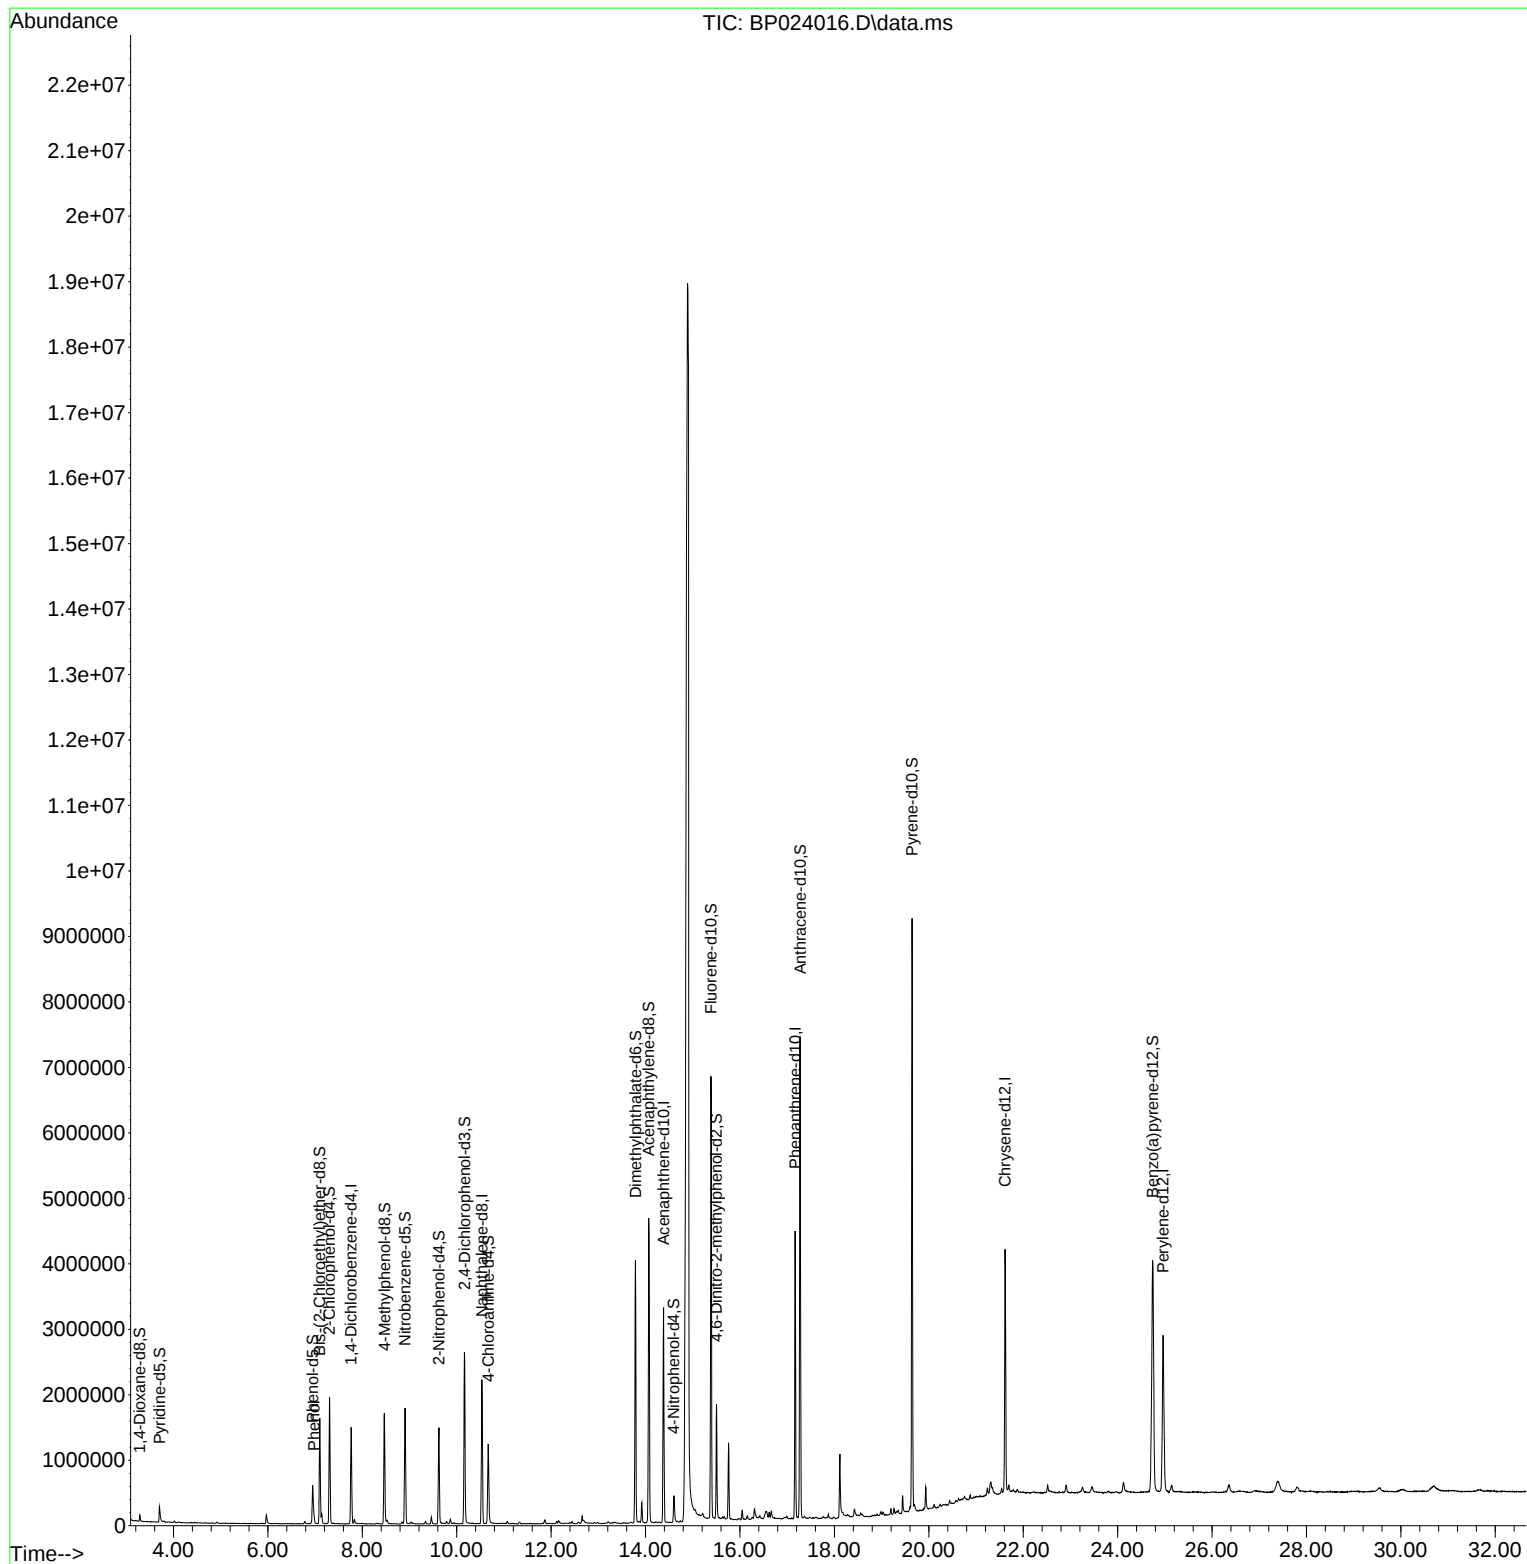

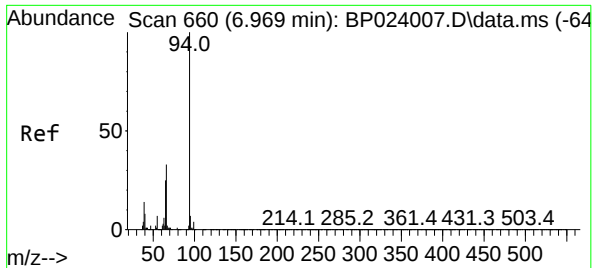

Phenol

Concen: 2.107 ng/ul

RT: 6.975 min Scan# 60

Delta R.T. -0.006 min

Lab File: BP024016.D


Acq: 10 Feb 2025 17:12

Instrument :

BNA_P

ClientSampleId :

E29D1

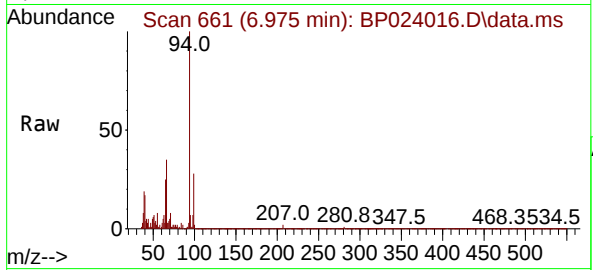

Tgt Ion: 94 Resp: 78260

Ion Ratio Lower Upper

94 100

65 25.3 20.1 30.1

66 35.3 26.0 39.0

