

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
 Data File : BP024022.D
 Acq On : 10 Feb 2025 21:55
 Operator : RC/JU
 Sample : Q1336-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29D4

Quant Time: Feb 12 15:06:12 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 11:19:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	460639	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.540	136	1978179	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.387	164	1185957	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.169	188	2233752	20.000	ng/u1	-0.02
79) Chrysene-d12	21.598	240	2193502	20.000	ng/u1	-0.04
88) Perylene-d12	24.957	264	2357707	20.000	ng/u1	-0.05
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	60900	5.493	ng/uL	0.00
4) Pyridine-d5	3.717	84	75053	2.346	ng/u1	0.01
7) Phenol-d5	6.952	99	366582	8.993	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.099	67	775032	35.918	ng/u1	0.00
11) 2-Chlorophenol-d4	7.311	132	1010189	31.557	ng/u1	0.00
15) 4-Methylphenol-d8	8.463	113	457251	13.731	ng/u1	-0.01
21) Nitrobenzene-d5	8.910	128	550489	34.782	ng/u1	0.00
24) 2-Nitrophenol-d4	9.622	143	583063	34.142	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.163	165	977349	31.197	ng/u1	0.00
31) 4-Chloroaniline-d4	10.675	131	56807	1.212	ng/u1	0.00
46) Dimethylphthalate-d6	13.793	166	2996381	33.872	ng/u1	0.00
49) Acenaphthylene-d8	14.075	160	3503975	35.120	ng/u1	0.00
54) 4-Nitrophenol-d4	14.610	143	95047	5.410	ng/u1	0.00
60) Fluorene-d10	15.387	176	2671050	35.856	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.504	200	358502	26.015	ng/u1	0.00
73) Anthracene-d10	17.269	188	3458176	31.530	ng/u1	-0.02
81) Pyrene-d10	19.633	212	4345143	36.970	ng/u1	-0.03
92) Benzo(a)pyrene-d12	24.727	264	3833497	31.163	ng/u1	-0.05
Target Compounds						
					Qvalue	
8) Phenol	6.975	94	71554	1.709	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024022.D
Acq On : 10 Feb 2025 21:55
Operator : RC/JU
Sample : Q1336-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29D4

Quant Time: Feb 12 15:06:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 11:19:36 2025
Response via : Initial Calibration

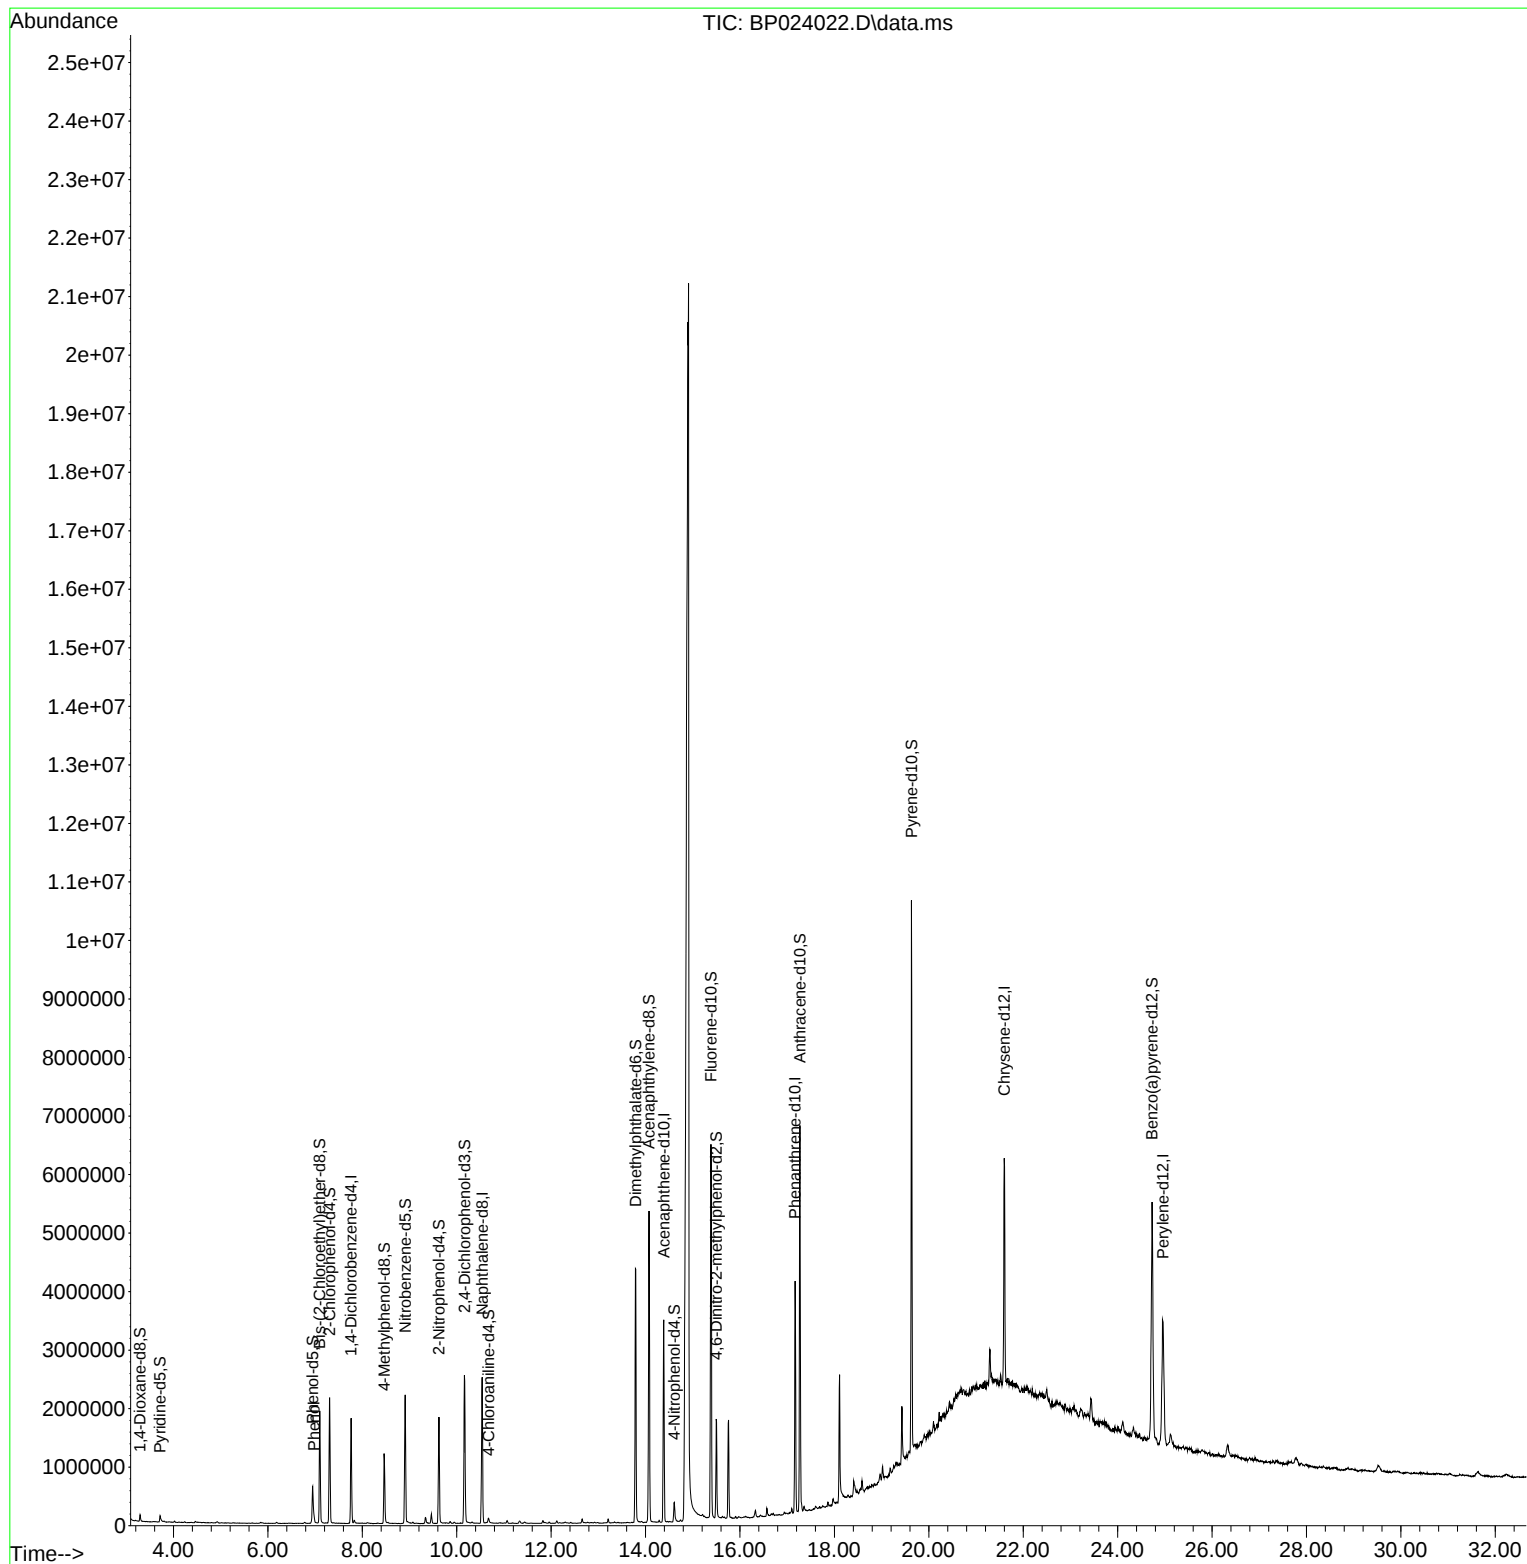

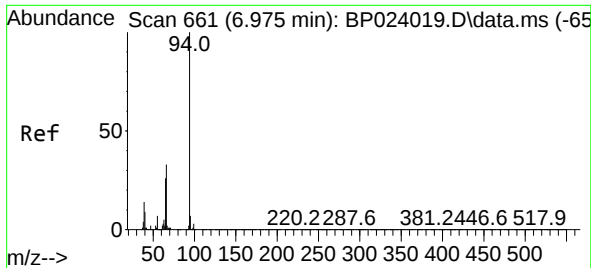

#8
Phenol
Concen: 1.709 ng/ul
RT: 6.975 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP024022.D
Acq: 10 Feb 2025 21:55

Instrument :
BNA_P
ClientSampleId :
E29D4

Tgt Ion: 94 Resp: 71554
Ion Ratio Lower Upper
94 100
65 27.1 20.1 30.1
66 35.1 26.0 39.0

