

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
 Data File : BP024012.D
 Acq On : 10 Feb 2025 14:30
 Operator : RC/JU
 Sample : Q1336-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29C5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP024012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	43	rVB	86238	110789	1.06%	0.116%
2	3.699	101	104	119	rBV	432575	731027	7.02%	0.765%
3	4.017	155	158	164	rVB	18240	25024	0.24%	0.026%
4	4.458	229	233	237	rVB	13955	19663	0.19%	0.021%
5	4.928	307	313	319	rBV2	16830	32134	0.31%	0.034%
6	6.175	520	525	529	rBV4	7538	12527	0.12%	0.013%
7	6.946	647	656	668	rBV	495570	814156	7.82%	0.852%
8	7.099	673	682	695	rBV	1498519	2201486	21.13%	2.304%
9	7.305	710	717	729	rBV	1504720	2421160	23.24%	2.534%
10	7.399	729	733	738	rVB5	7952	14263	0.14%	0.015%
11	7.763	786	795	804	rBV	1314183	1972761	18.94%	2.065%
12	8.463	906	914	931	rBV	1514291	2474508	23.76%	2.590%
13	8.905	978	989	999	rBV	1683482	2693456	25.86%	2.819%
14	9.340	1056	1063	1070	rVB	15738	27200	0.26%	0.028%
15	9.622	1103	1111	1130	rBV	1273631	2070184	19.87%	2.166%
16	10.163	1195	1203	1225	rBV	2072955	3520219	33.79%	3.684%
17	10.534	1259	1266	1279	rVB	1939330	3038582	29.17%	3.180%
18	10.669	1279	1289	1302	rBV	2008701	3560008	34.18%	3.726%
19	11.822	1481	1485	1490	rVB4	7246	10583	0.10%	0.011%
20	11.957	1504	1508	1515	rVB8	7068	11426	0.11%	0.012%
21	12.063	1520	1526	1531	rVV	36133	55477	0.53%	0.058%
22	12.116	1531	1535	1542	rVB	32435	57497	0.55%	0.060%
23	13.204	1715	1720	1726	rVB2	14346	22854	0.22%	0.024%
24	13.346	1740	1744	1752	rVB7	7944	16880	0.16%	0.018%
25	13.787	1811	1819	1830	rBV	3950515	5226447	50.17%	5.470%
26	14.075	1858	1868	1883	rBV	4213123	6620805	63.56%	6.929%
27	14.287	1901	1904	1909	rVB	11966	14643	0.14%	0.015%
28	14.381	1913	1920	1934	rBV	2913358	4135244	39.70%	4.328%
29	14.610	1950	1959	1974	rBV	225828	449589	4.32%	0.471%
30	14.745	1977	1982	1986	rVV8	9173	20802	0.20%	0.022%
31	14.810	1988	1993	2002	rVB8	9366	20587	0.20%	0.022%
32	15.222	2055	2063	2067	rBV4	8782	19129	0.18%	0.020%
33	15.263	2067	2070	2073	rVV	10211	10621	0.10%	0.011%
34	15.387	2084	2091	2102	rBV	6231793	8486919	81.47%	8.882%
35	15.510	2106	2112	2126	rBV	1178568	1580457	15.17%	1.654%
36	15.634	2129	2133	2138	rVB	27256	36484	0.35%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
 Data File : BP024012.D
 Acq On : 10 Feb 2025 14:30
 Operator : RC/JU
 Sample : Q1336-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29C5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

37	15.763	2148	2155	2165	rBV	220683	350326	3.36%	0.367%
38	16.140	2215	2219	2221	rBV5	6741	10494	0.10%	0.011%
39	16.339	2248	2253	2260	rVB	43598	58930	0.57%	0.062%
40	16.687	2308	2312	2317	rVB3	8646	11709	0.11%	0.012%
41	16.963	2353	2359	2363	rBV3	16522	34444	0.33%	0.036%
42	17.116	2381	2385	2389	rBV7	10812	16334	0.16%	0.017%
43	17.187	2390	2397	2407	rBV	3286016	4692786	45.05%	4.911%
44	17.287	2407	2414	2427	rBV2	6638436	9354234	89.80%	9.789%
45	18.116	2550	2555	2564	rBV2	55252	91638	0.88%	0.096%
46	18.428	2605	2608	2615	rVB3	22491	33500	0.32%	0.035%
47	18.581	2630	2634	2636	rBV5	18353	27345	0.26%	0.029%
48	19.004	2701	2706	2710	rBV4	28434	59479	0.57%	0.062%
49	19.204	2736	2740	2746	rVB	67117	95777	0.92%	0.100%
50	19.281	2748	2753	2757	rBV	61455	88632	0.85%	0.093%
51	19.657	2811	2817	2829	rBV	7465405	10416623	100.00%	10.901%
52	21.610	3143	3149	3159	rBV	2574422	4540717	43.59%	4.752%
53	24.721	3670	3678	3700	rVB	3479988	8764483	84.14%	9.172%
54	24.957	3708	3718	3735	rVB	1404395	4372493	41.98%	4.576%


Sum of corrected areas: 95555535

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024012.D
Acq On : 10 Feb 2025 14:30
Operator : RC/JU
Sample : Q1336-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29C5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

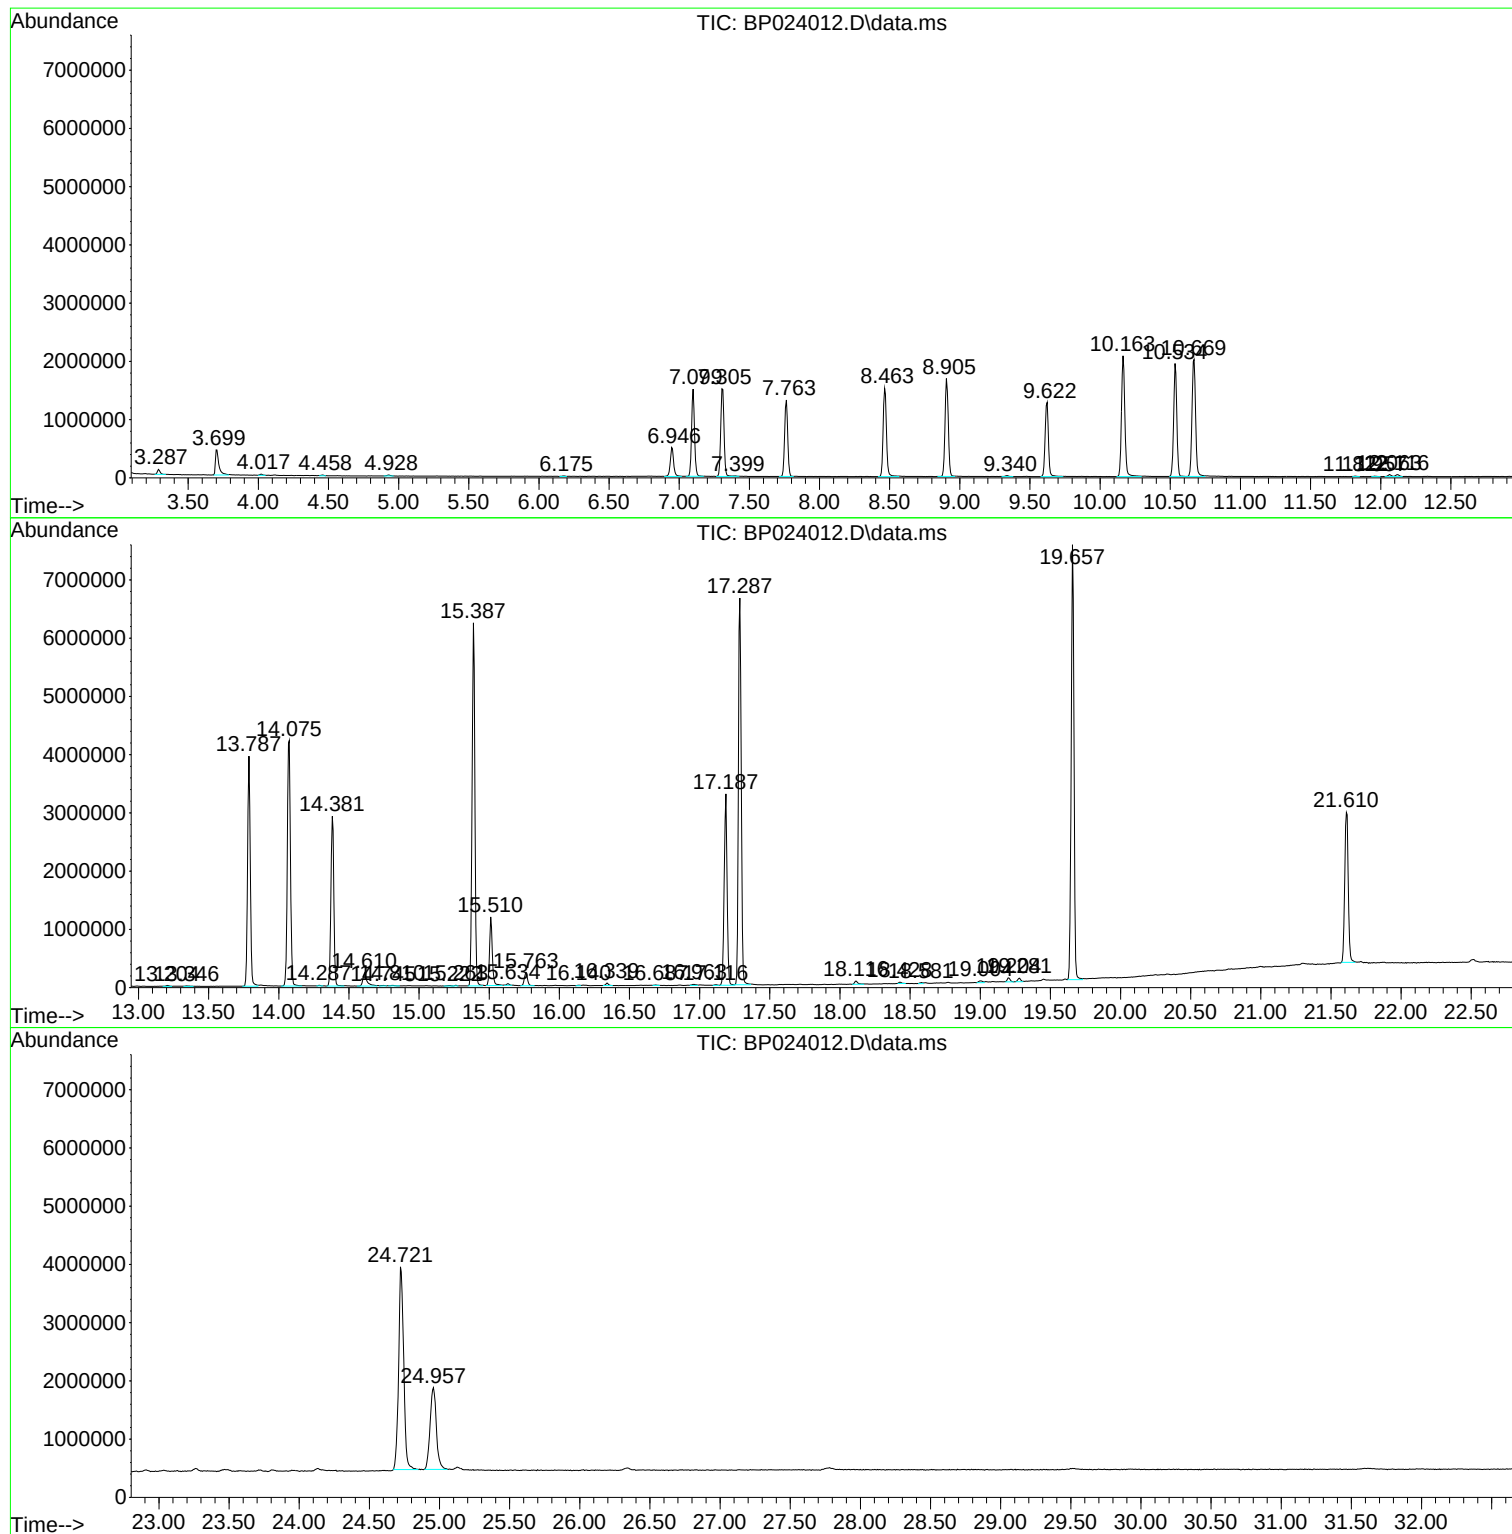

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024012.D
Acq On : 10 Feb 2025 14:30
Operator : RC/JU
Sample : Q1336-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29C5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024012.D
Acq On : 10 Feb 2025 14:30
Operator : RC/JU
Sample : Q1336-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29C5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
