

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
 Data File : BP024014.D
 Acq On : 10 Feb 2025 15:51
 Operator : RC/JU
 Sample : Q1336-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E29C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP024014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	41	rVB	83403	104583	0.91%	0.106%
2	3.705	102	105	127	rVB	230811	406972	3.53%	0.411%
3	4.022	156	159	168	rVB2	16786	26578	0.23%	0.027%
4	4.458	230	233	238	rVB2	12623	17988	0.16%	0.018%
5	4.934	308	314	320	rVB3	15096	28636	0.25%	0.029%
6	6.952	648	657	668	rBV	471096	754327	6.55%	0.762%
7	7.099	674	682	697	rBV	1470094	2295481	19.94%	2.320%
8	7.311	711	718	727	rBV	1666974	2551126	22.16%	2.579%
9	7.399	731	733	742	rVB6	10178	13473	0.12%	0.014%
10	7.763	786	795	805	rBV	1309354	1968754	17.10%	1.990%
11	8.469	908	915	930	rBV	1469421	2296726	19.95%	2.322%
12	8.910	982	990	1000	rBV	1883550	2781295	24.15%	2.811%
13	9.340	1058	1063	1069	rVB2	14493	23689	0.21%	0.024%
14	9.469	1079	1085	1095	rBV2	6732	14827	0.13%	0.015%
15	9.628	1103	1112	1128	rBV	1352153	2190352	19.02%	2.214%
16	10.169	1193	1204	1229	rBV	2205264	3777495	32.81%	3.818%
17	10.540	1259	1267	1275	rBV	1783608	2964729	25.75%	2.997%
18	10.675	1281	1290	1309	rBV	1924543	3467846	30.12%	3.505%
19	12.122	1529	1536	1543	rBV2	31760	54795	0.48%	0.055%
20	13.351	1739	1745	1751	rVB8	5458	11577	0.10%	0.012%
21	13.787	1812	1819	1835	rBV	3894448	5519033	47.93%	5.579%
22	14.075	1858	1868	1879	rBV	4510015	6748907	58.61%	6.822%
23	14.381	1912	1920	1932	rBV	2707751	3971510	34.49%	4.014%
24	14.604	1950	1958	1978	rBV	271037	532678	4.63%	0.538%
25	14.745	1978	1982	1985	rVV6	10230	17246	0.15%	0.017%
26	14.804	1988	1992	1996	rVB7	8654	13822	0.12%	0.014%
27	14.934	2010	2014	2020	rVB3	16378	29062	0.25%	0.029%
28	15.204	2056	2060	2065	rVB4	12971	19609	0.17%	0.020%
29	15.387	2083	2091	2104	rBV	5951502	8901659	77.31%	8.998%
30	15.498	2104	2110	2127	rVV	1546606	1911963	16.60%	1.933%
31	15.628	2127	2132	2138	rVB	26606	49088	0.43%	0.050%
32	15.751	2148	2153	2161	rBV	68861	101085	0.88%	0.102%
33	16.951	2353	2357	2364	rVB	12564	24313	0.21%	0.025%
34	17.169	2387	2394	2404	rBV	3327963	4685503	40.69%	4.736%
35	17.275	2405	2412	2424	rBV	6940444	9905802	86.03%	10.013%
36	17.869	2511	2513	2519	rVB7	11620	15826	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024014.D
Acq On : 10 Feb 2025 15:51
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29C6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	18.104	2550	2553	2558	rBV5	39502	53606	0.47%	0.054%
38	19.192	2734	2738	2744	rBV	65156	91046	0.79%	0.092%
39	19.269	2747	2751	2755	rVV	63385	83411	0.72%	0.084%
40	19.651	2809	2816	2825	rBV	9505253	11514738	100.00%	11.639%
41	21.616	3144	3150	3158	rVB	2956799	4504728	39.12%	4.553%
42	24.745	3672	3682	3699	rVB	4030904	9956565	86.47%	10.064%
43	24.963	3711	3719	3739	rVB	1604789	4528127	39.32%	4.577%




Sum of corrected areas: 98930576

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024014.D
Acq On : 10 Feb 2025 15:51
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

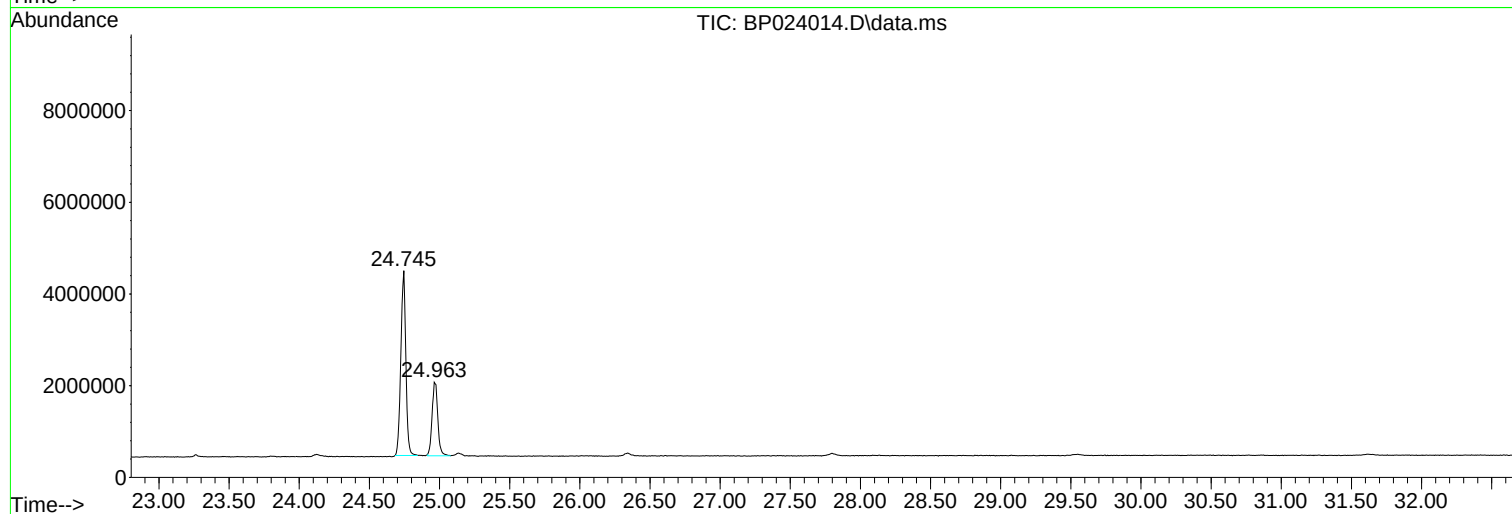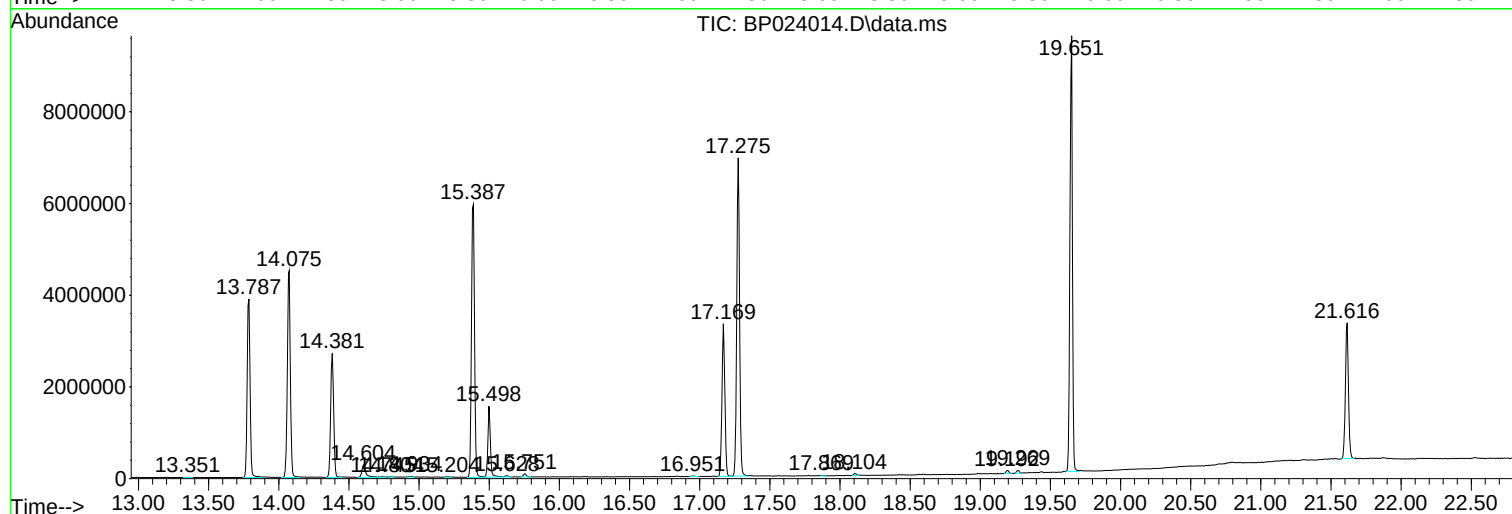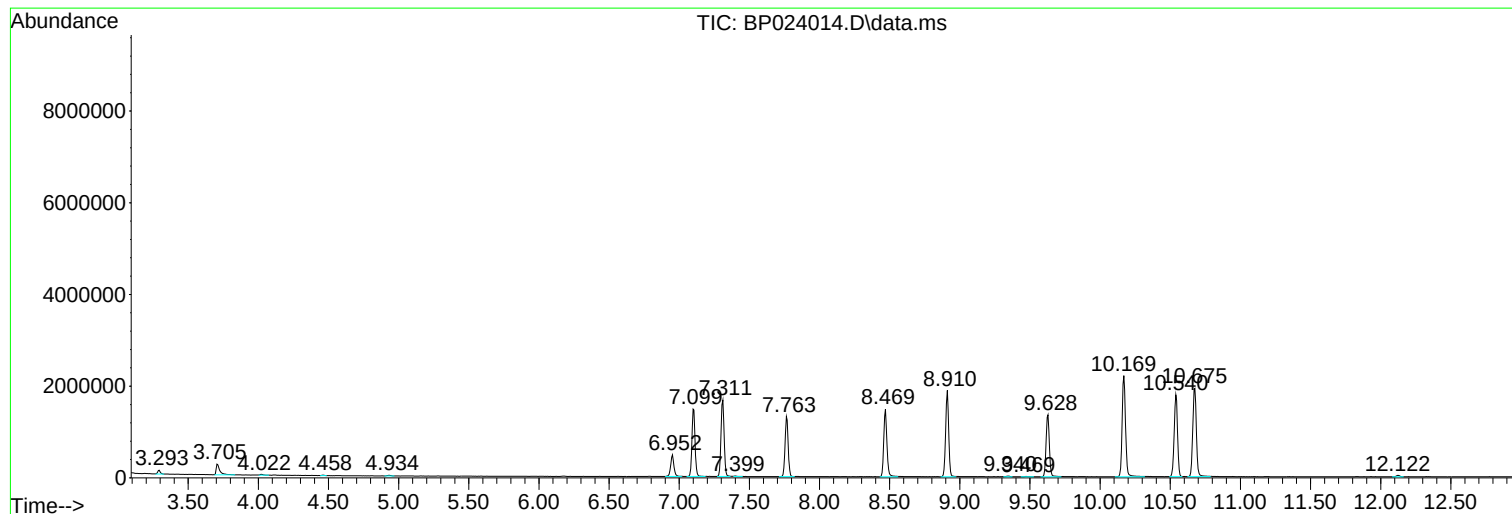

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024014.D
Acq On : 10 Feb 2025 15:51
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024014.D
Acq On : 10 Feb 2025 15:51
Operator : RC/JU
Sample : Q1336-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E29C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc