

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
 Data File : BP024020.D
 Acq On : 10 Feb 2025 20:34
 Operator : RC/JU
 Sample : PB166622BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK622

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP024020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	43	rVB	109922	152352	1.51%	0.150%
2	3.699	100	104	128	rBV	1407406	2255694	22.32%	2.218%
3	4.022	154	159	166	rBV	45860	68593	0.68%	0.067%
4	6.946	645	656	674	rBV	1762913	2813381	27.84%	2.766%
5	7.099	676	682	693	rVB	1425975	2209281	21.86%	2.172%
6	7.310	710	718	730	rBV	1855252	2844788	28.15%	2.797%
7	7.763	788	795	805	rVB	1414454	2211114	21.88%	2.174%
8	8.469	906	915	929	rBV	2172982	3506133	34.69%	3.447%
9	8.910	981	990	1002	rBV	1617528	2625075	25.97%	2.581%
10	9.622	1103	1111	1125	rBV	1223451	2055702	20.34%	2.021%
11	10.163	1194	1203	1227	rBV	2119849	3471376	34.35%	3.413%
12	10.534	1258	1266	1276	rBV	1827389	3167706	31.34%	3.114%
13	10.669	1281	1289	1309	rBV	2047608	3517507	34.80%	3.458%
14	11.181	1370	1376	1385	rVB3	11066	22374	0.22%	0.022%
15	12.116	1529	1535	1542	rBV2	35367	63296	0.63%	0.062%
16	13.363	1740	1747	1753	rVB	54894	79962	0.79%	0.079%
17	13.781	1812	1818	1835	rBV	3664864	4735690	46.86%	4.656%
18	13.898	1835	1838	1844	rVB7	6187	10887	0.11%	0.011%
19	14.069	1860	1867	1884	rBV	4406624	6127296	60.63%	6.024%
20	14.381	1909	1920	1931	rBV	2734700	4128715	40.85%	4.059%
21	14.604	1946	1958	1980	rBV	1137862	2262264	22.38%	2.224%
22	14.798	1989	1991	1998	rVB7	6755	10414	0.10%	0.010%
23	15.045	2028	2033	2038	rVB7	9734	14763	0.15%	0.015%
24	15.386	2084	2091	2105	rBV	5180413	7635891	75.55%	7.507%
25	15.510	2105	2112	2126	rVV	1099004	1497891	14.82%	1.473%
26	15.628	2129	2132	2138	rVB2	24341	38771	0.38%	0.038%
27	15.963	2185	2189	2194	rVB6	6760	11269	0.11%	0.011%
28	16.192	2223	2228	2231	rVB5	8297	11191	0.11%	0.011%
29	16.845	2335	2339	2346	rBV10	6242	11899	0.12%	0.012%
30	16.957	2352	2358	2362	rBV2	16227	26691	0.26%	0.026%
31	17.180	2388	2396	2406	rBV	3496636	5056137	50.03%	4.971%
32	17.280	2406	2413	2428	rVV	6366471	8792493	87.00%	8.644%
33	17.880	2512	2515	2521	rBV7	13191	16927	0.17%	0.017%
34	18.110	2550	2554	2557	rBV5	10507	13665	0.14%	0.013%
35	19.192	2735	2738	2745	rBV	65577	85233	0.84%	0.084%
36	19.269	2747	2751	2755	rBV	60476	81896	0.81%	0.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024020.D
Acq On : 10 Feb 2025 20:34
Operator : RC/JU
Sample : PB166622BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK622

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	19.351	2761	2765	2771	rBV2	75848	87253	0.86%	0.086%
38	19.598	2803	2807	2810	rBV	178524	196388	1.94%	0.193%
39	19.645	2810	2815	2825	rVV	7834242	10106578	100.00%	9.936%
40	20.686	2989	2992	2997	rBV	119722	132927	1.32%	0.131%
41	21.604	3141	3148	3159	rBV	3409679	5365891	53.09%	5.275%
42	24.715	3668	3677	3693	rVB	3661664	9098519	90.03%	8.945%
43	24.951	3709	3717	3734	rVB	1883517	5091965	50.38%	5.006%




Sum of corrected areas: 101713838

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024020.D
Acq On : 10 Feb 2025 20:34
Operator : RC/JU
Sample : PB166622BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

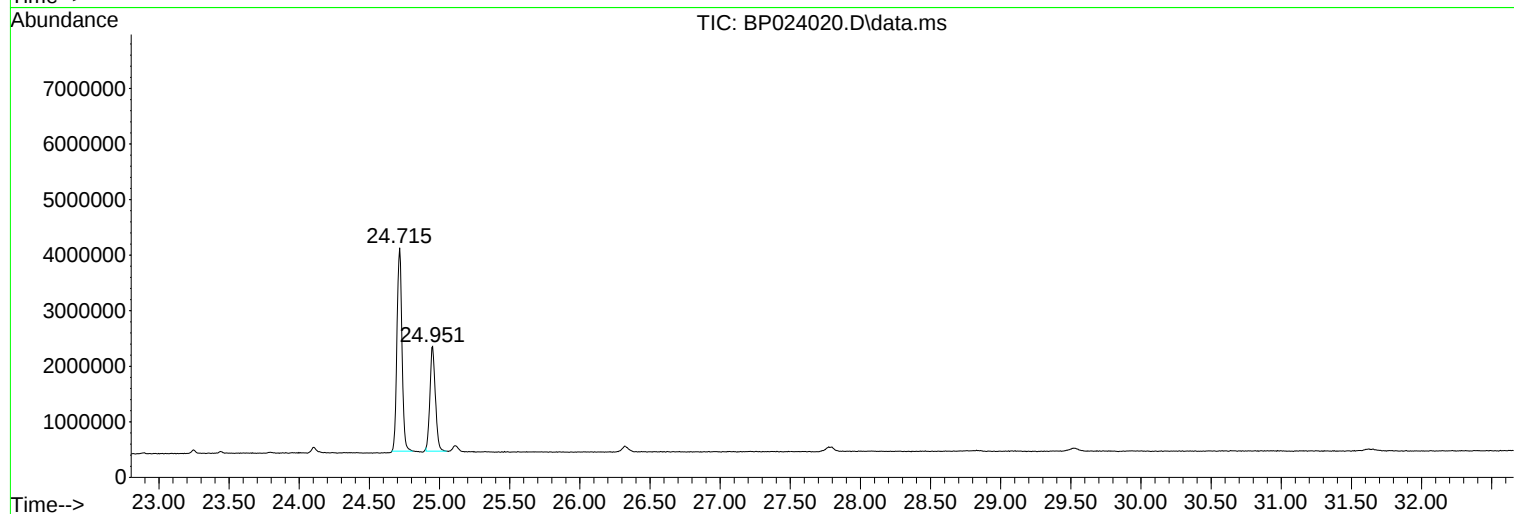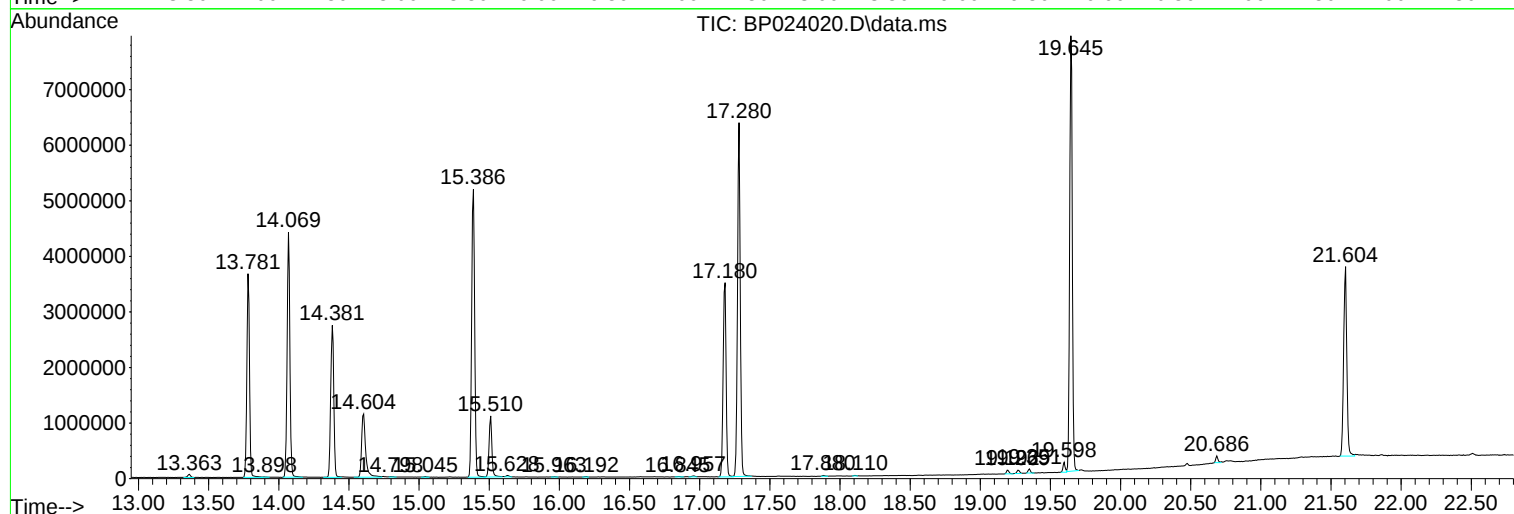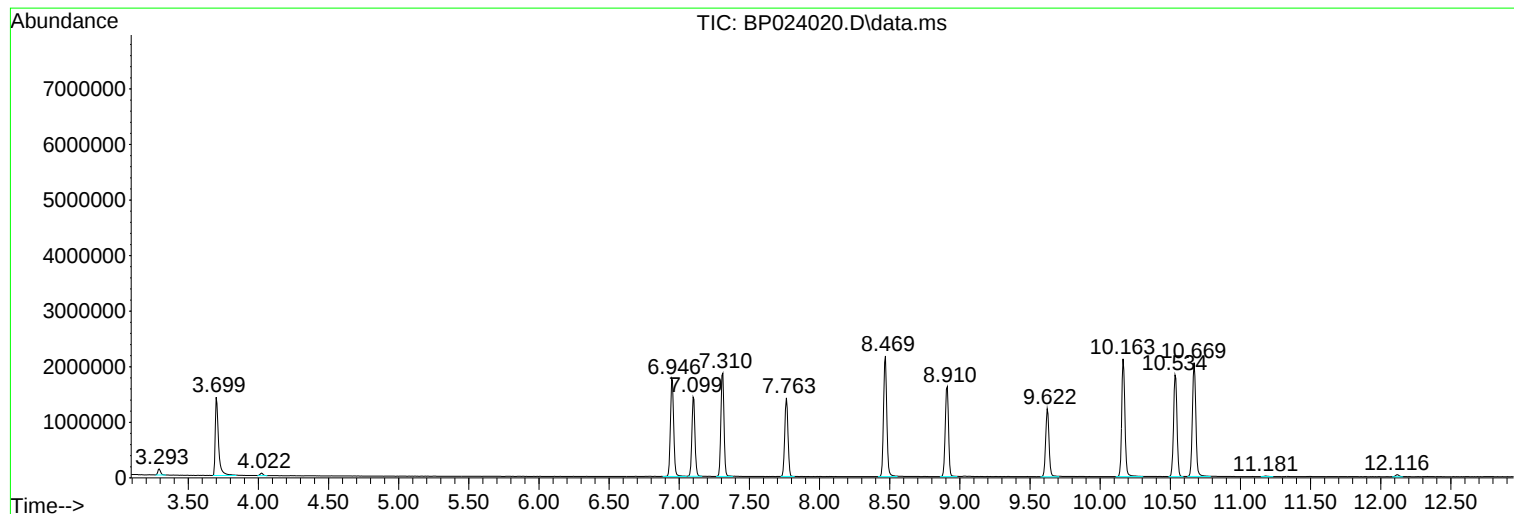

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024020.D
Acq On : 10 Feb 2025 20:34
Operator : RC/JU
Sample : PB166622BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021025\
Data File : BP024020.D
Acq On : 10 Feb 2025 20:34
Operator : RC/JU
Sample : PB166622BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------