
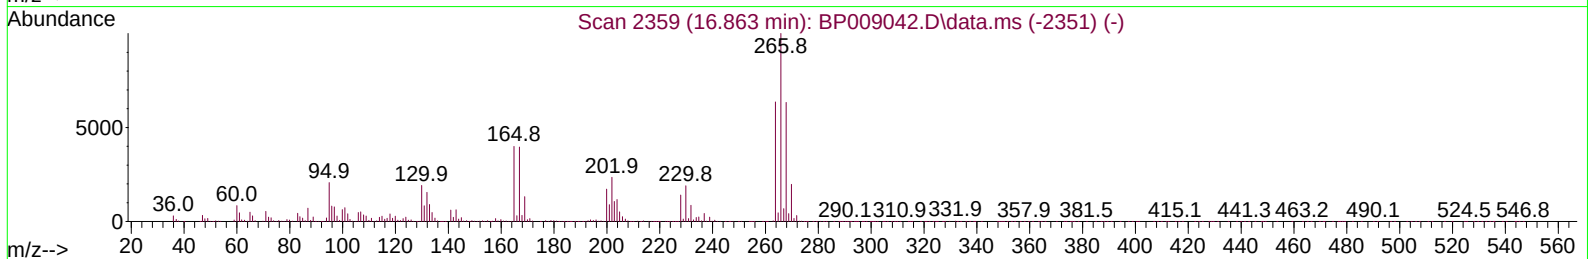
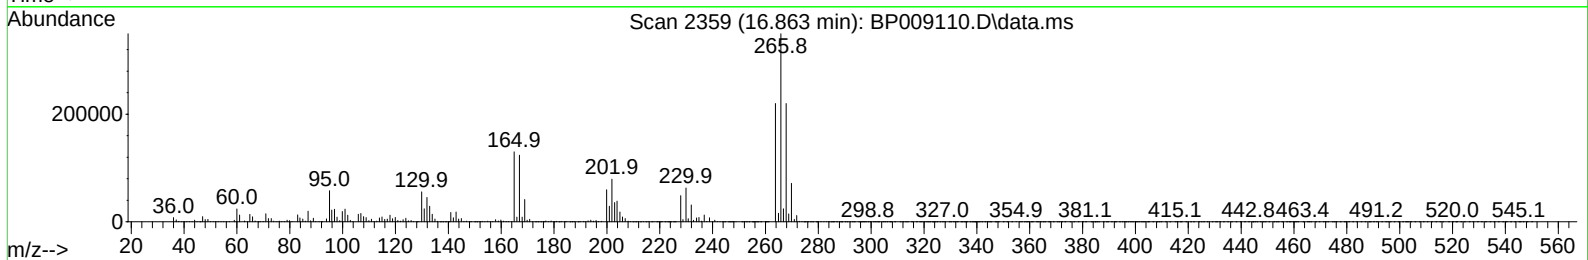


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
 Data File : BP009110.D
 Acq On : 11 Feb 2022 12:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 00:55:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 07 15:13:17 2022
 Response via : Initial Calibration

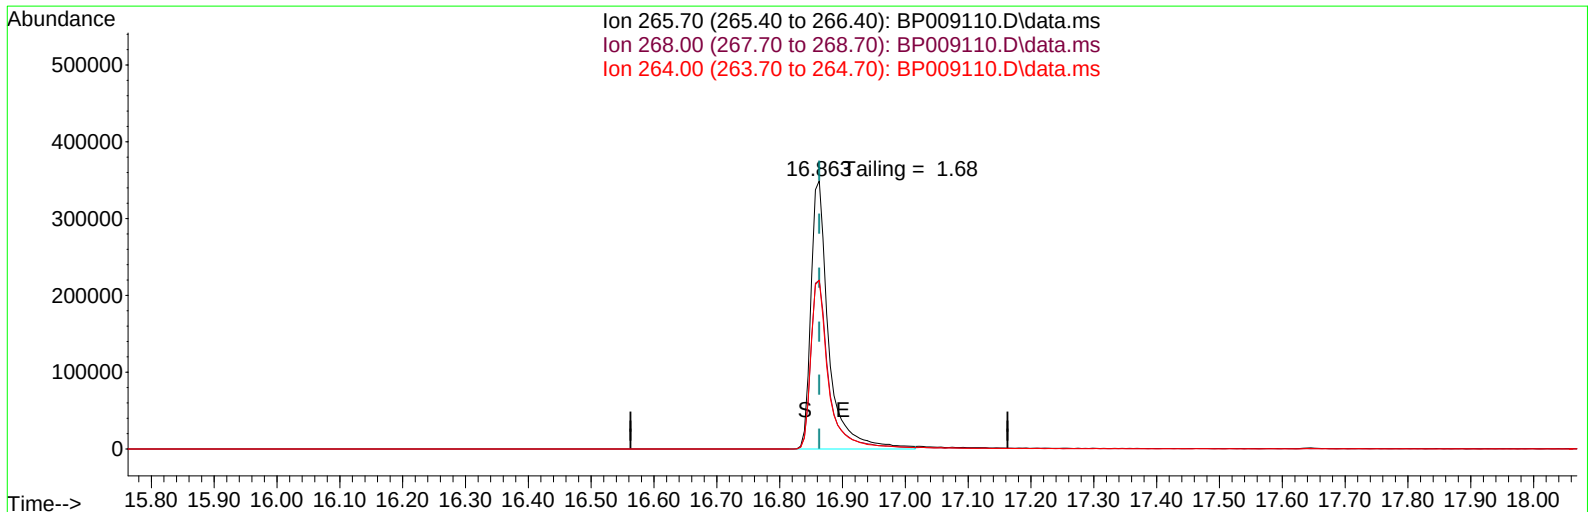

TIC: BP009110.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.000) 1439060.66 ng

response 698344

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.89
264.00	62.90	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
 Data File : BP009110.D
 Acq On : 11 Feb 2022 12:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 00:55:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 07 15:13:17 2022
 Response via : Initial Calibration

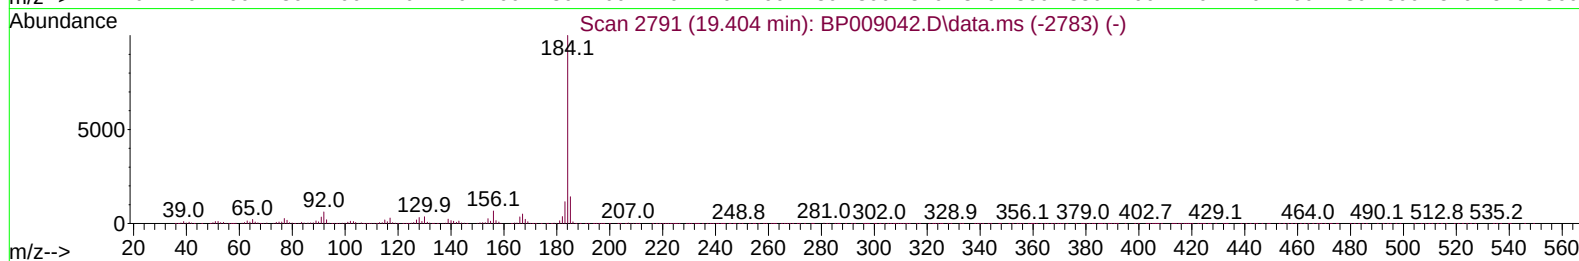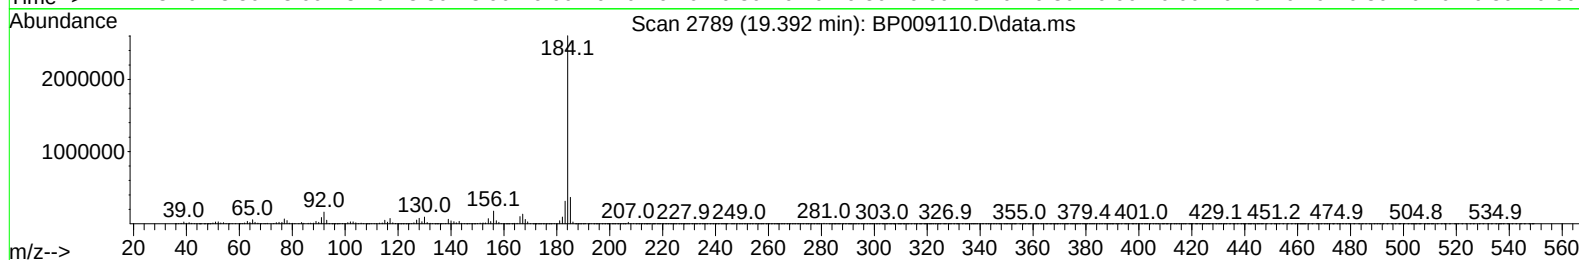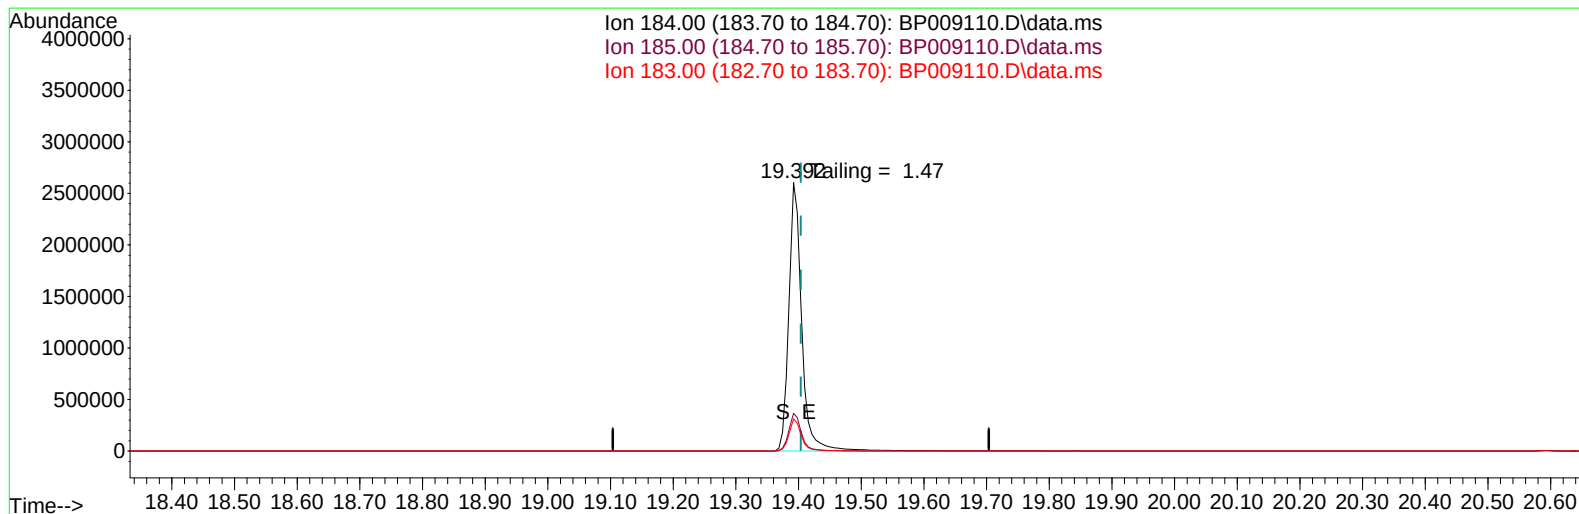

TIC: BP009110.D\data.ms

(77) Benzidine

19.392min (-0.012) 821499.55 ng

response 3742203

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.08
183.00	11.90	12.01
0.00	0.00	0.00