

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
Data File : BP009112.D
Acq On : 11 Feb 2022 14:23
Operator : CG/JU
Sample : PB142549BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142549BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	402	409	430	rBV	3072246	5170326	41.57%	9.160%
2	6.987	673	680	698	rBV	2914924	5360187	43.10%	9.496%
3	7.793	810	817	835	rVB	711825	1204177	9.68%	2.133%
4	8.957	1007	1015	1036	rBV	1911220	3538448	28.45%	6.269%
5	10.593	1284	1293	1316	rBV	809184	1679097	13.50%	2.975%
6	13.057	1701	1712	1738	rBV	5801611	9663964	77.70%	17.121%
7	14.440	1939	1947	1967	rBV	1451877	2416450	19.43%	4.281%
8	15.939	2194	2202	2230	rBV	4393272	7340683	59.02%	13.005%
9	17.198	2409	2416	2433	rBV	1650559	2779962	22.35%	4.925%
10	19.757	2846	2851	2866	rBV	9929364	12437076	100.00%	22.034%
11	21.292	3107	3112	3122	rBV	1791869	2604470	20.94%	4.614%
12	23.686	3513	3519	3531	rVB2	987835	2249917	18.09%	3.986%




Sum of corrected areas: 56444757

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
Data File : BP009112.D
Acq On : 11 Feb 2022 14:23
Operator : CG/JU
Sample : PB142549BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142549BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

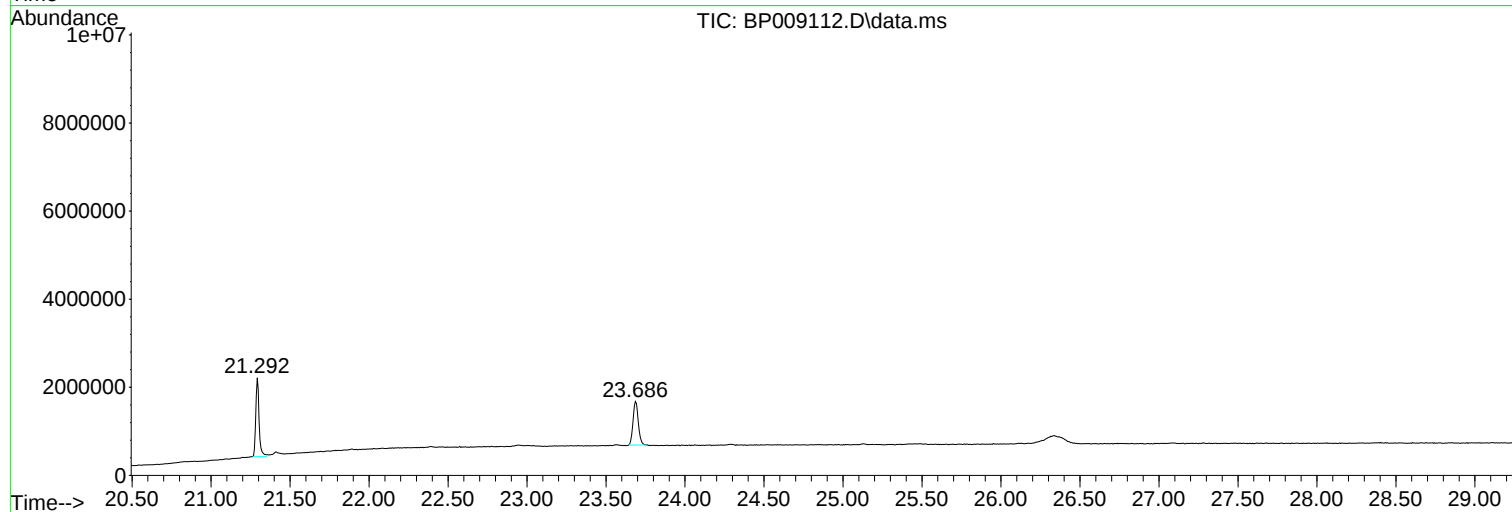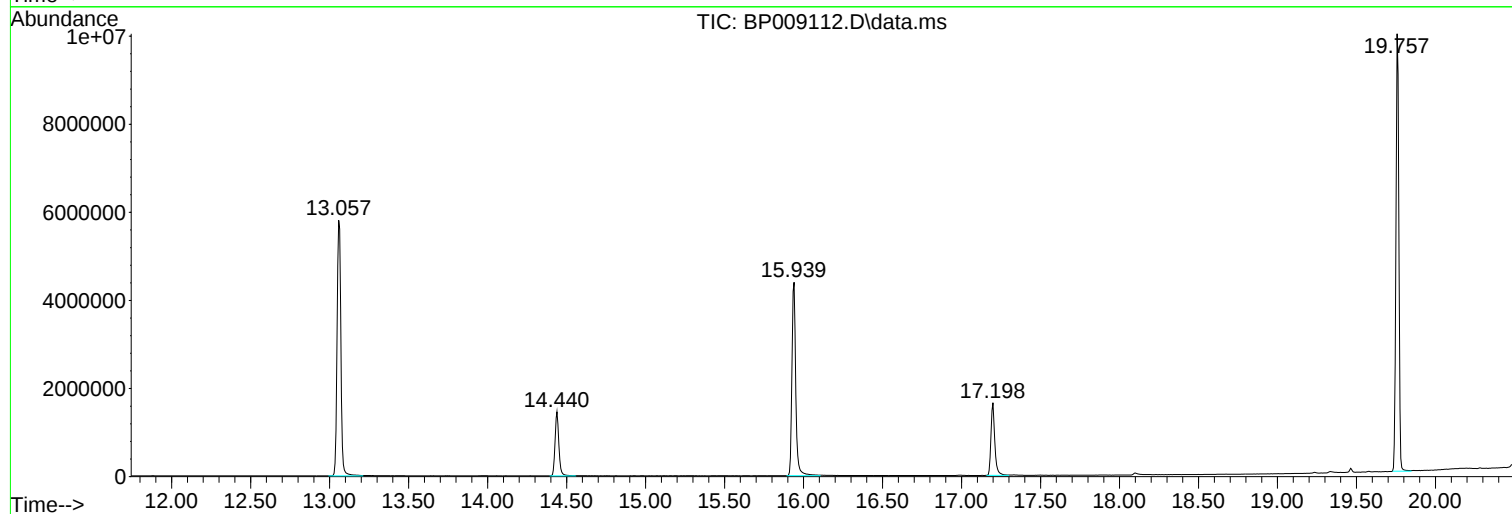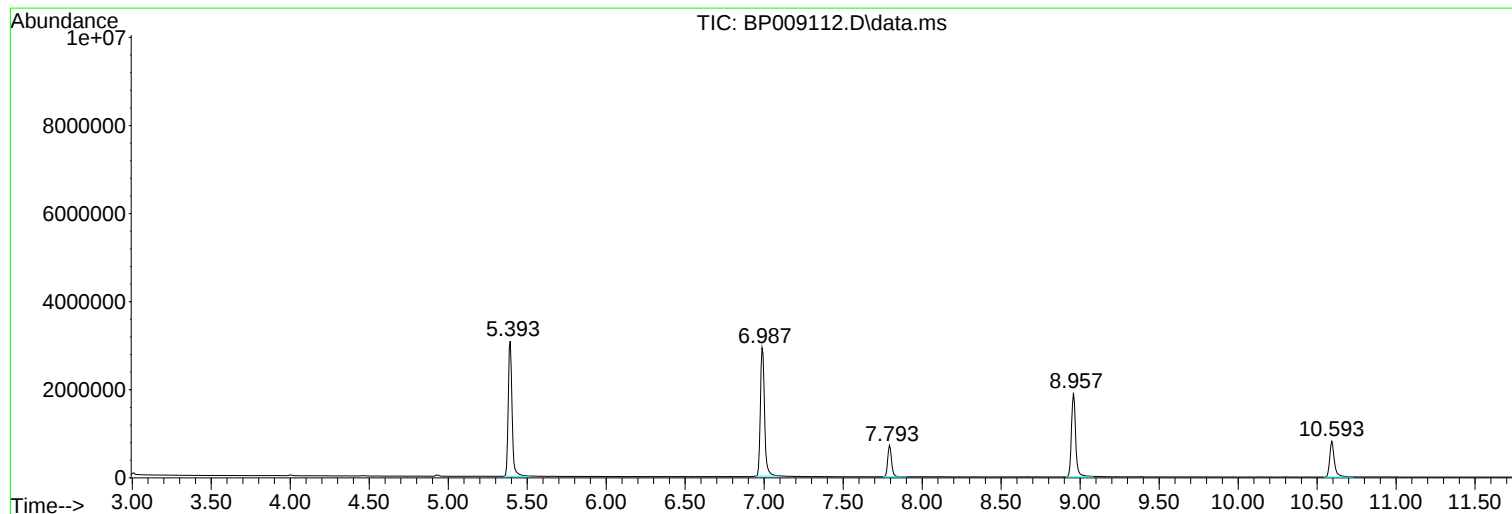

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
Data File : BP009112.D
Acq On : 11 Feb 2022 14:23
Operator : CG/JU
Sample : PB142549BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142549BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
Data File : BP009112.D
Acq On : 11 Feb 2022 14:23
Operator : CG/JU
Sample : PB142549BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142549BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------