

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
Data File : BP009116.D
Acq On : 11 Feb 2022 16:47
Operator : CG/JU
Sample : PB142544BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142544BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	403	409	429	rBV	2993145	5028304	36.90%	8.830%
2	6.993	674	681	710	rVB	2867302	5227259	38.36%	9.180%
3	7.799	810	818	835	rBV	678519	1159885	8.51%	2.037%
4	8.957	1008	1015	1048	rBV	1768752	3432954	25.19%	6.029%
5	10.599	1283	1294	1316	rBV	762471	1625470	11.93%	2.855%
6	13.063	1705	1713	1739	rBV	6029951	9387791	68.89%	16.486%
7	14.439	1940	1947	1968	rBV	1333941	2335687	17.14%	4.102%
8	15.939	2195	2202	2230	rBV	4403239	7152522	52.49%	12.561%
9	17.198	2409	2416	2433	rBV	1595852	2734446	20.07%	4.802%
10	19.763	2846	2852	2865	rBV	11061304	13627077	100.00%	23.931%
11	21.298	3108	3113	3126	rBV	1833656	2799211	20.54%	4.916%
12	23.692	3513	3520	3530	rVB2	1114678	2433017	17.85%	4.273%




Sum of corrected areas: 56943623

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
Data File : BP009116.D
Acq On : 11 Feb 2022 16:47
Operator : CG/JU
Sample : PB142544BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142544BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

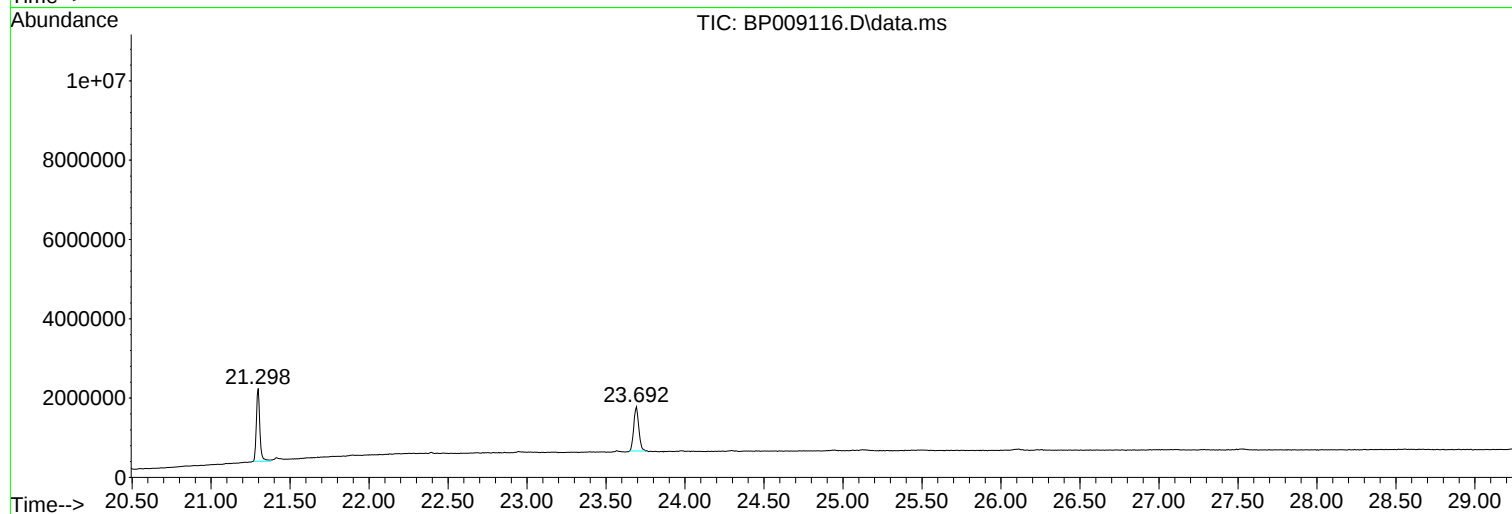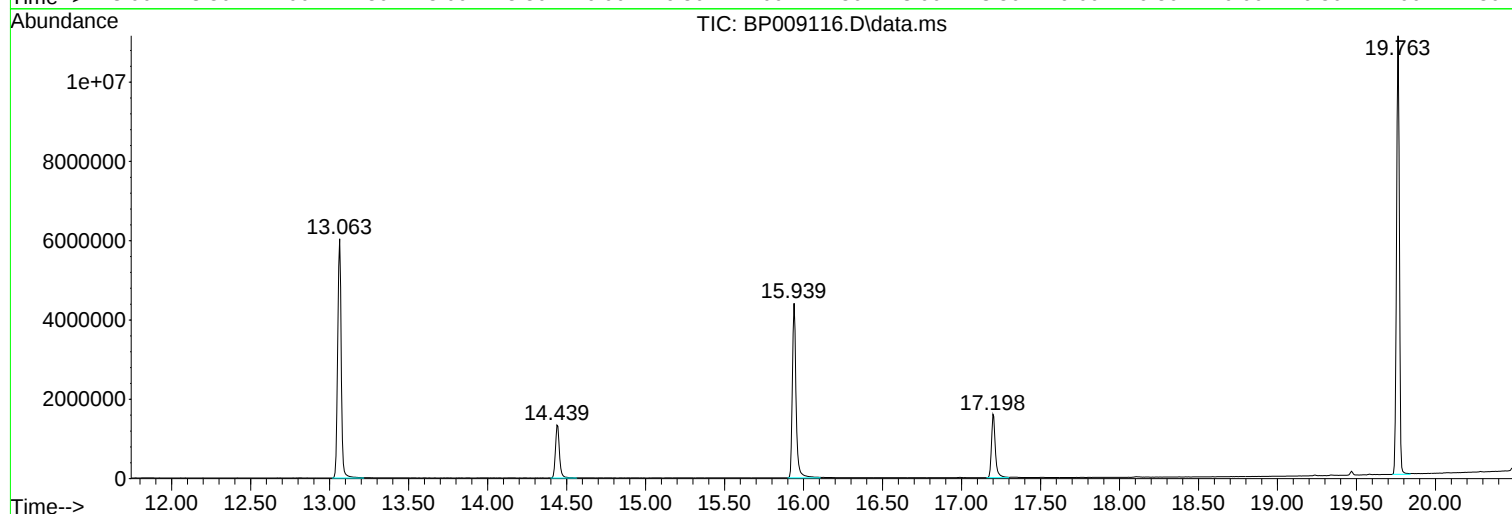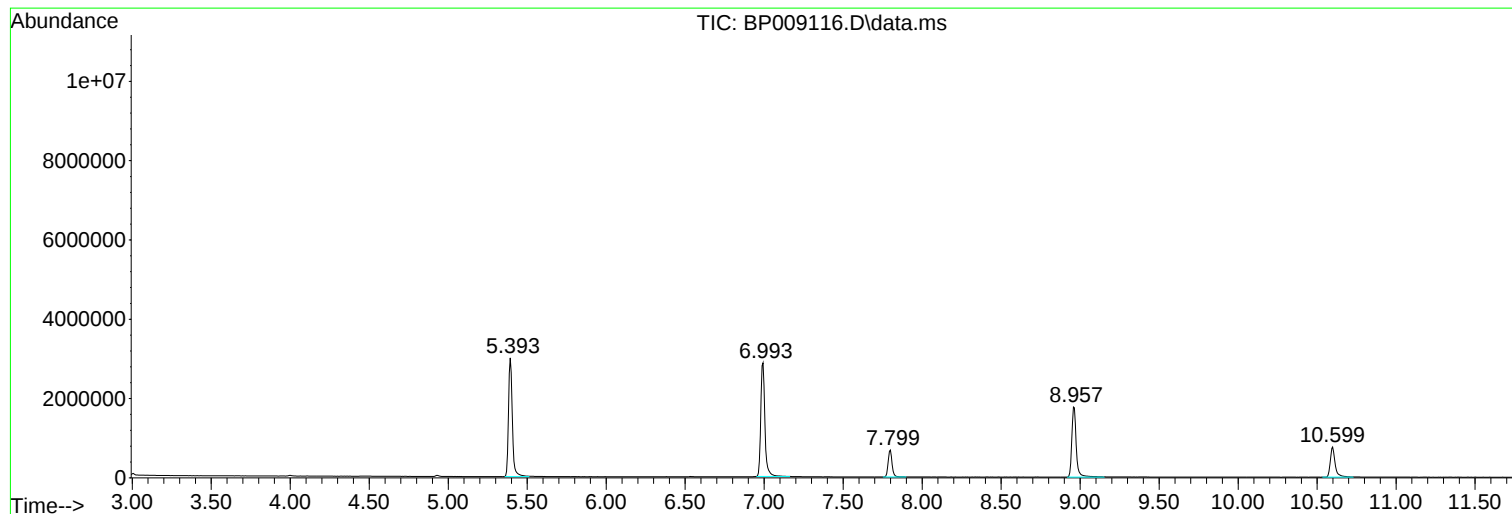

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
Data File : BP009116.D
Acq On : 11 Feb 2022 16:47
Operator : CG/JU
Sample : PB142544BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142544BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
Data File : BP009116.D
Acq On : 11 Feb 2022 16:47
Operator : CG/JU
Sample : PB142544BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142544BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------