


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
 Data File : BP009110.D
 Acq On : 11 Feb 2022 12:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 07 15:13:17 2022

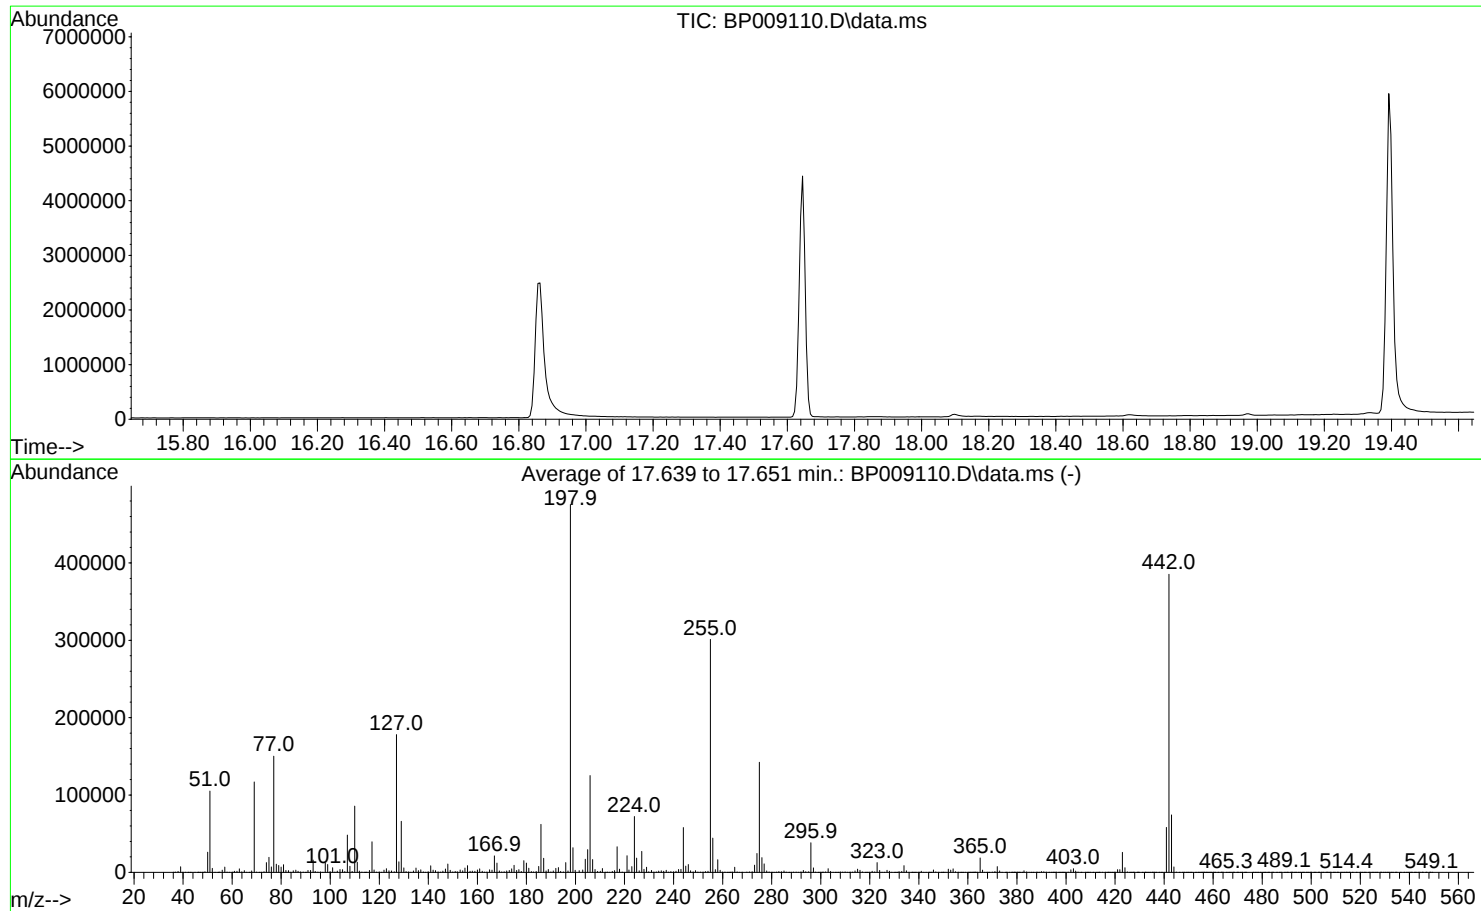

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.1	105012	PASS
68	69	0.00	2	1.6	1853	PASS
69	198	0.00	100	24.6	116917	PASS
70	69	0.00	2	0.4	526	PASS
127	198	10	80	37.5	178105	PASS
197	198	0.00	2	0.4	1911	PASS
198	198	100	100	100.0	475522	PASS
199	198	5	9	6.7	31905	PASS
275	198	10	60	29.9	142219	PASS
365	198	1	100	3.9	18581	PASS
441	198	0.01	100	12.2	58189	PASS
442	442	100	100	100.0	385323	PASS
443	442	15	24	19.3	74315	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/11/2022	BNA_P	<u>BP009110.D</u>
Compound Name	Response	Retention Time
DDT	1807313	20.592
DDD	16790	20.21
DDE	2506	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19296	1826609	1.06

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
 Data File : BP009110.D
 Acq On : 11 Feb 2022 12:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 12 00:55:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 07 15:13:17 2022
 Response via : Initial Calibration

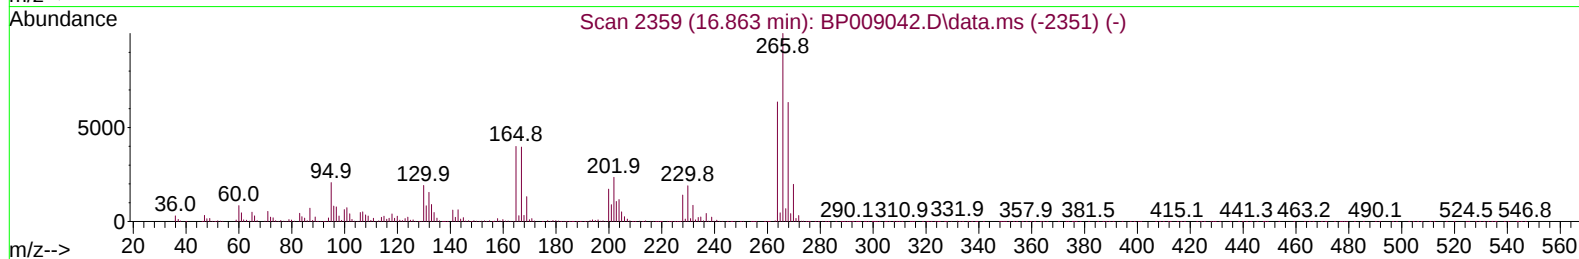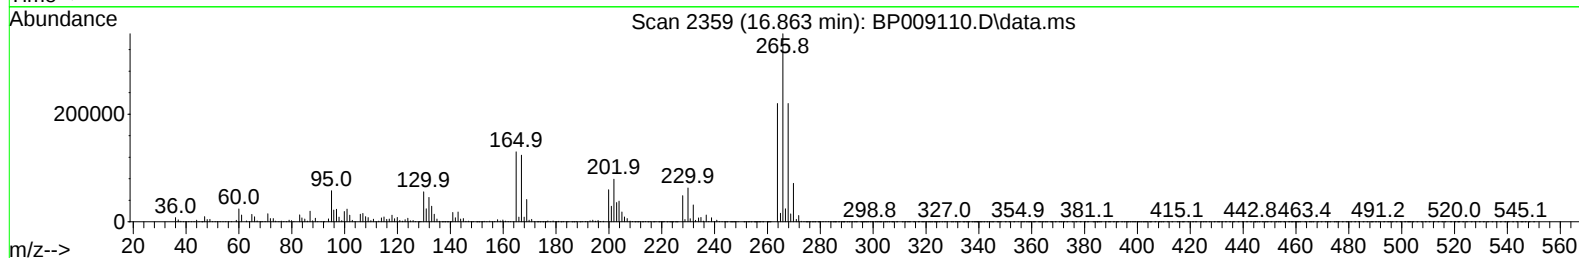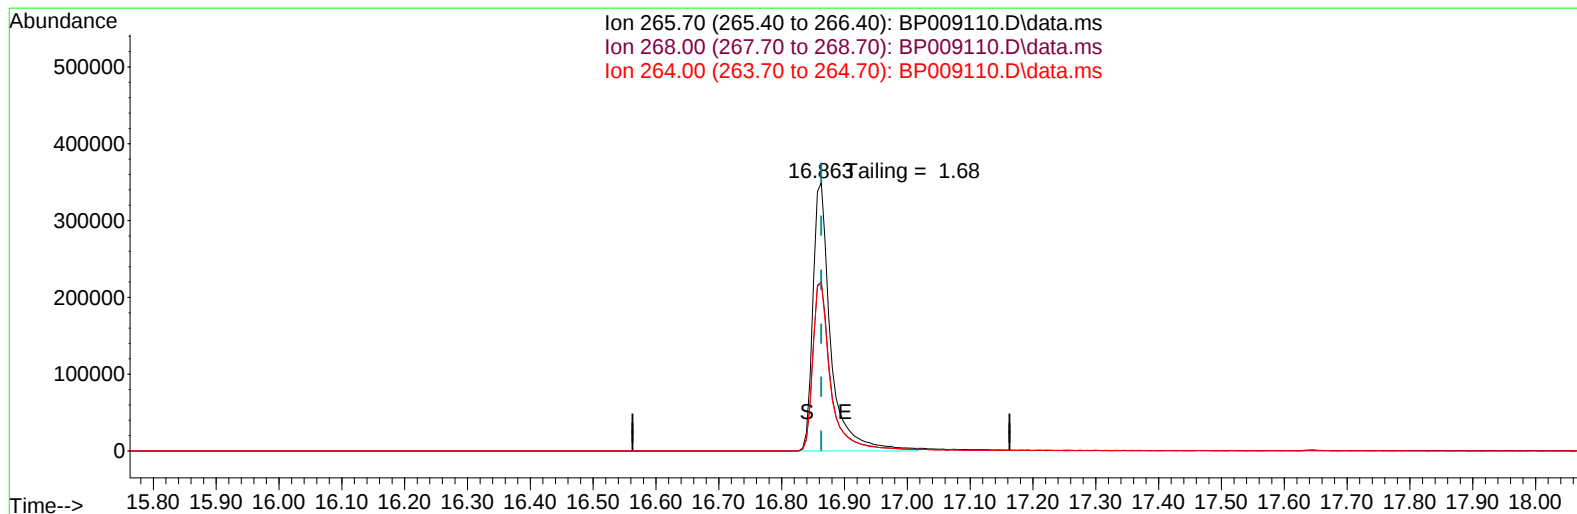

TIC: BP009110.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.000) 1439060.66 ng




response 698344

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.89
264.00	62.90	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021122\
 Data File : BP009110.D
 Acq On : 11 Feb 2022 12:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 12 00:55:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 07 15:13:17 2022
 Response via : Initial Calibration

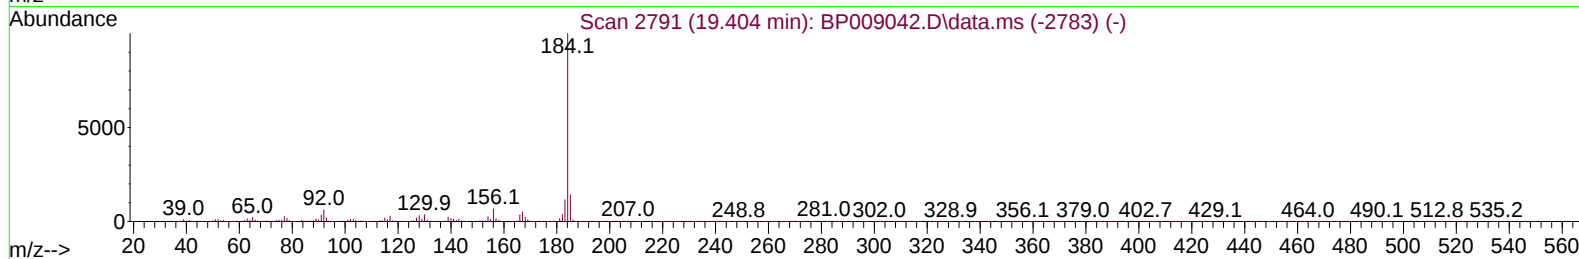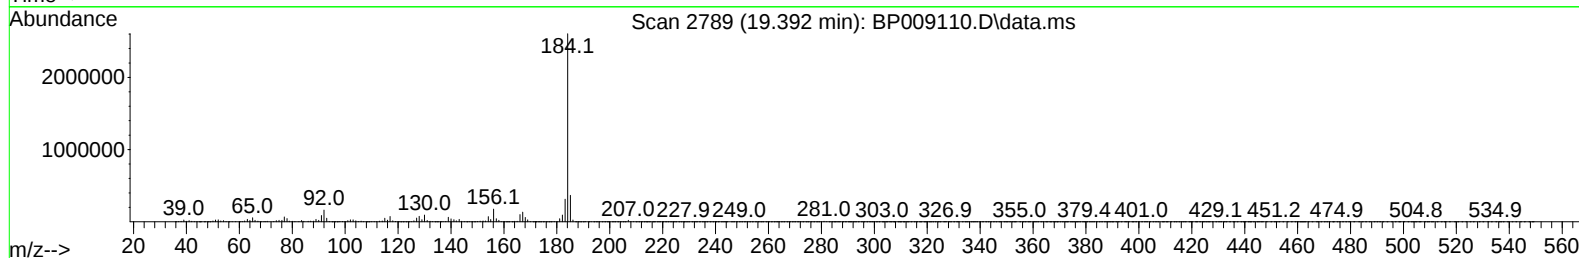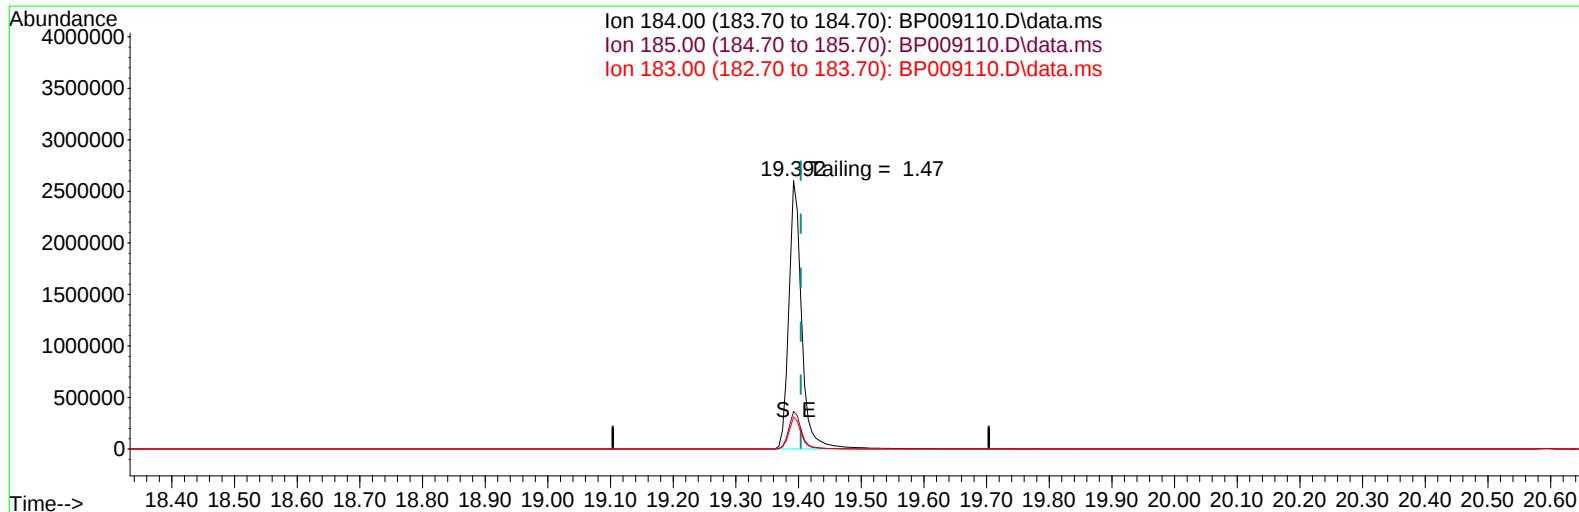

TIC: BP009110.D\data.ms

(77) Benzidine

19.392min (-0.012) 821499.55 ng

response 3742203

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.08
183.00	11.90	12.01
0.00	0.00	0.00