
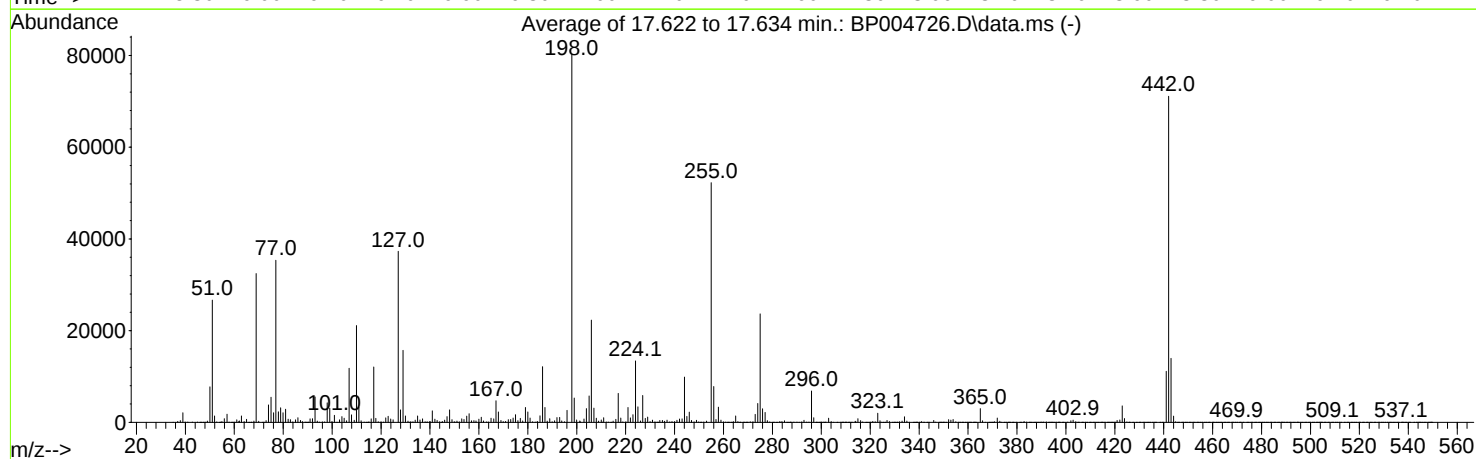


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021221\
 Data File : BP004726.D
 Acq On : 12 Feb 2021 12:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 05 18:04:48 2021

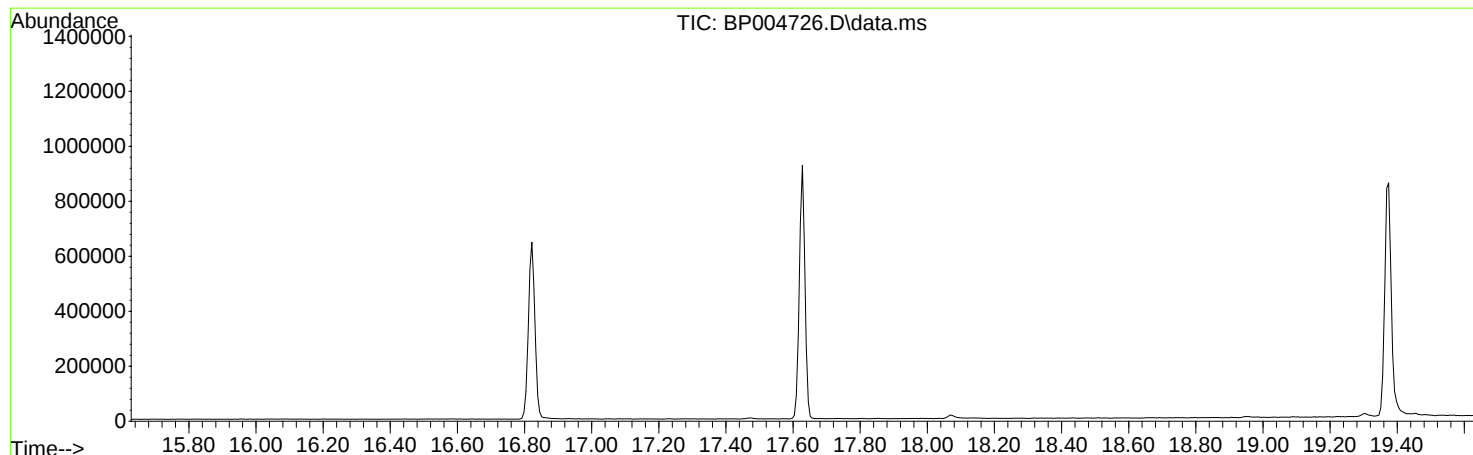

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	26642	PASS
68	69	0.00	2	0.9	284	PASS
69	198	0.00	100	40.4	32432	PASS
70	69	0.00	2	0.7	232	PASS
127	198	10	80	46.5	37288	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80213	PASS
199	198	5	9	6.6	5288	PASS
275	198	10	60	29.5	23658	PASS
365	198	1	100	3.8	3011	PASS
441	198	0.01	100	13.9	11124	PASS
442	442	100	100	100.0	71120	PASS
443	442	15	24	19.6	13972	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/12/2021	BNA_P	<u>BP004726.D</u>
Compound Name	Response	Retention Time
DDT	286508	20.57
DDD	5321	20.14
DDE	461	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5782	292290	1.98

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021221\
 Data File : BP004726.D
 Acq On : 12 Feb 2021 12:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 12 14:11:23 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 05 18:04:48 2021
 Response via : Initial Calibration

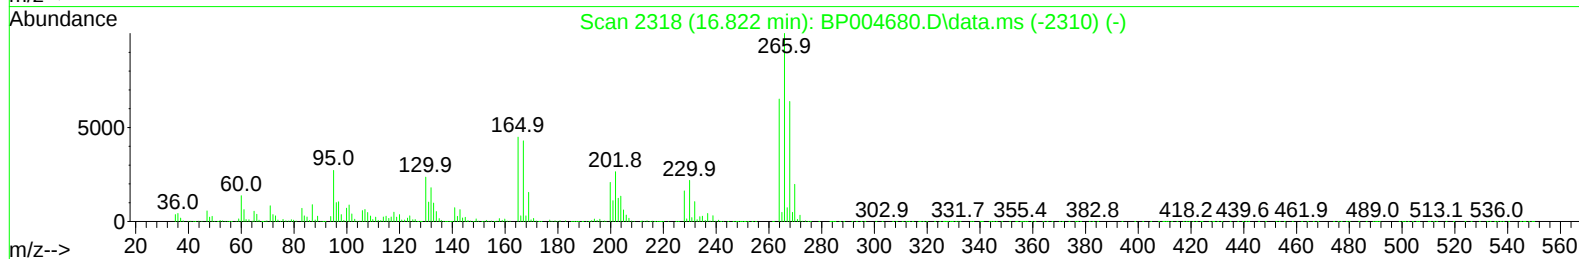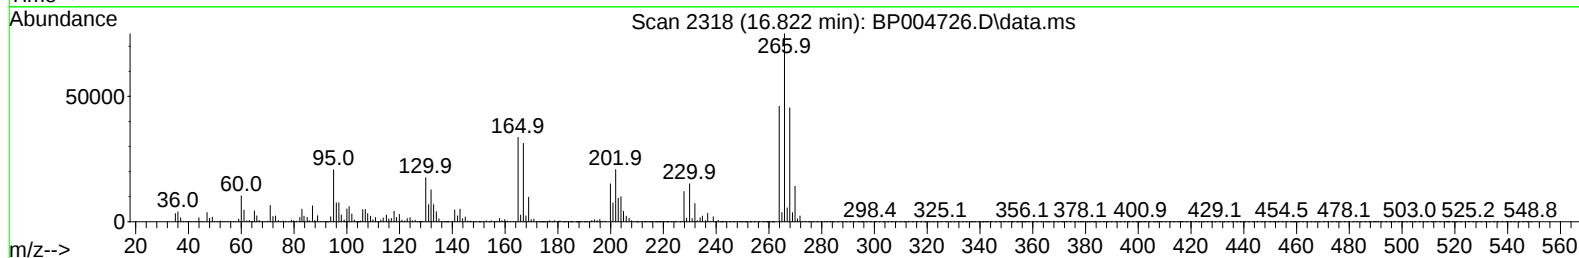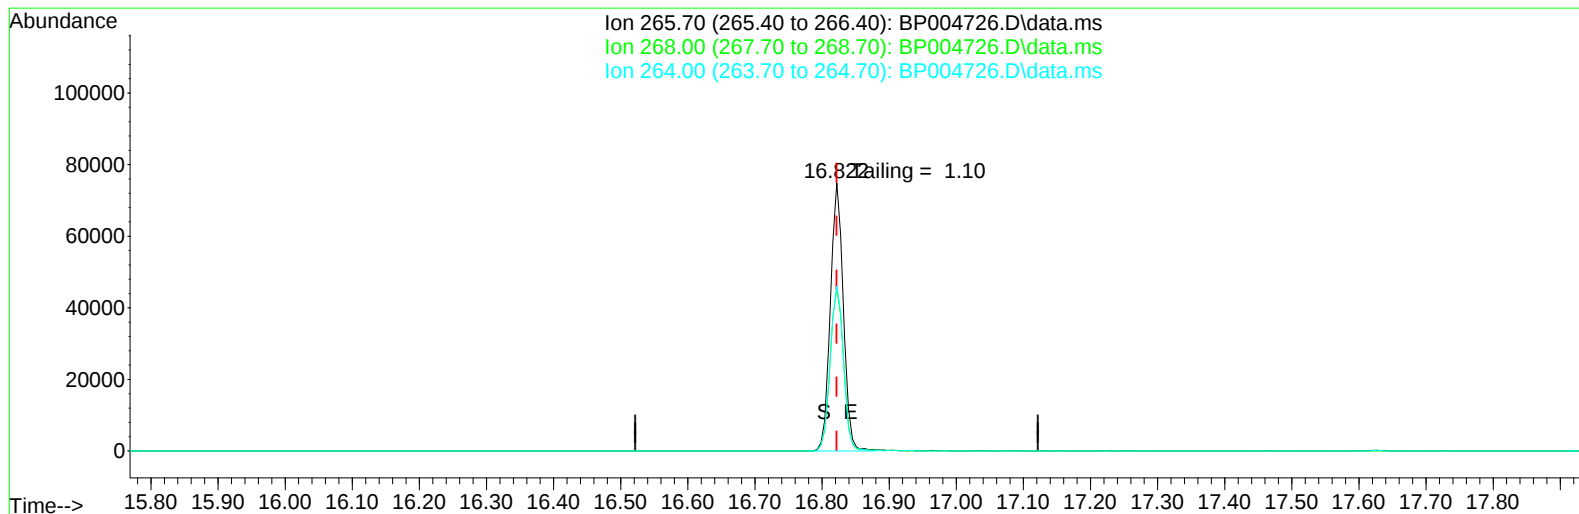

TIC: BP004726.D\data.ms

(70) Pentachlorophenol (C)

16.822min (+ 0.000) 1431587.67 ng




response 101146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	60.60
264.00	63.30	61.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021221\
 Data File : BP004726.D
 Acq On : 12 Feb 2021 12:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 12 14:11:23 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 05 18:04:48 2021
 Response via : Initial Calibration

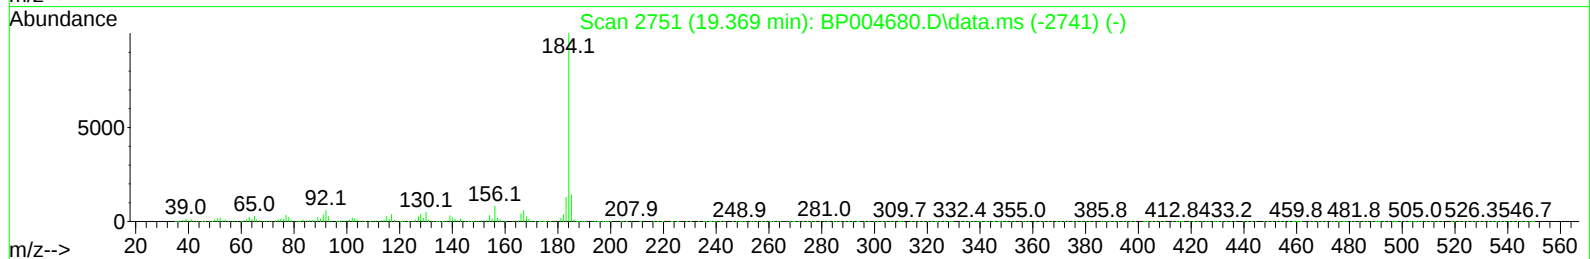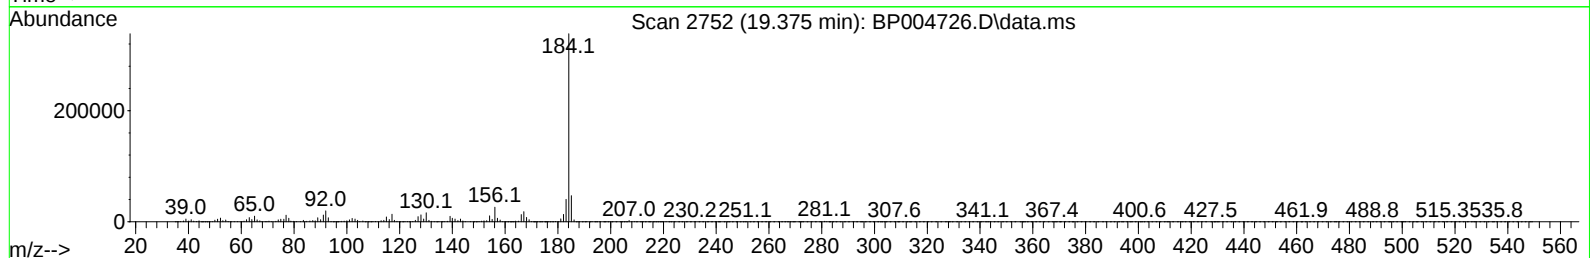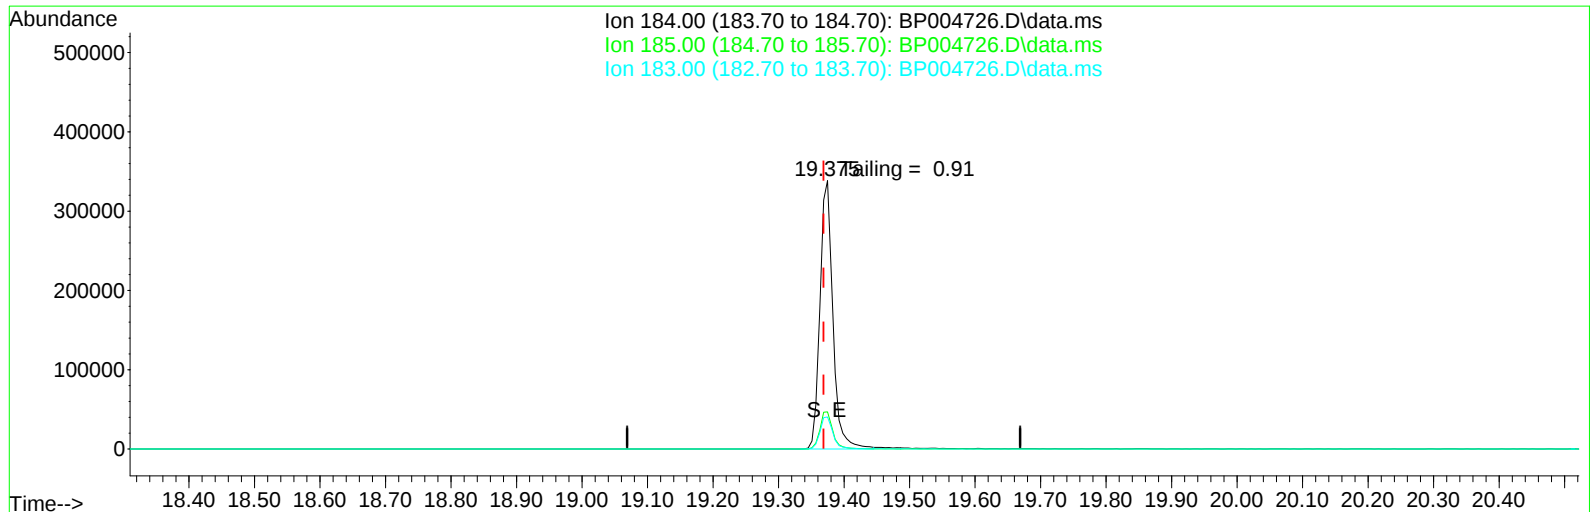

TIC: BP004726.D\data.ms

(77) Benzidine

19.375min (+ 0.006) 91628.29 ng

response 469634

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.84
183.00	12.00	11.92
0.00	0.00	0.00