
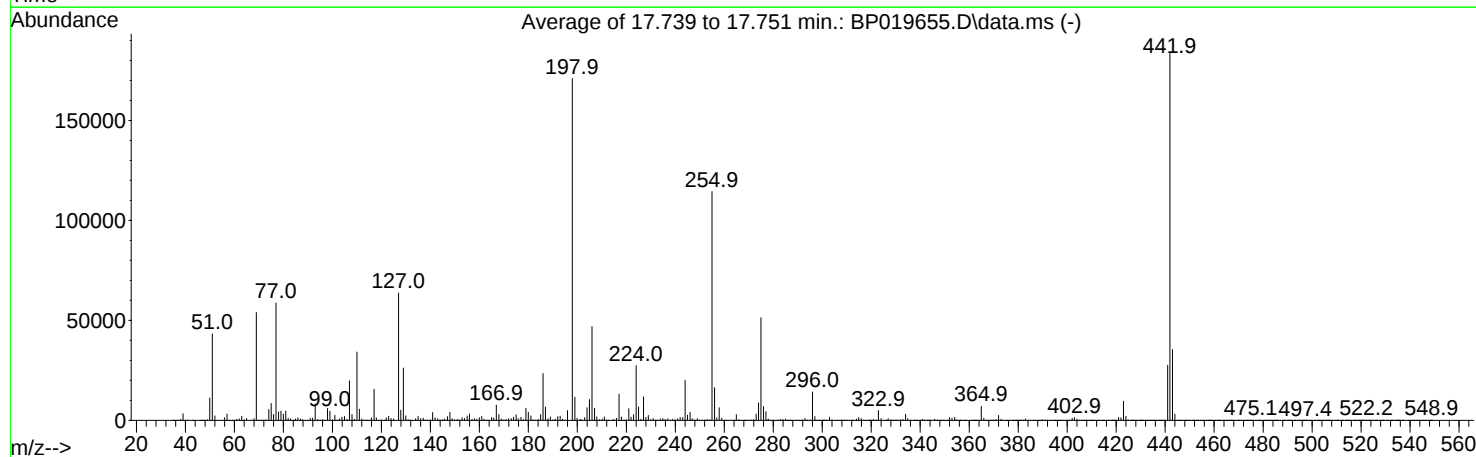


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021224\
Data File : BP019655.D
Acq On : 12 Feb 2024 10:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

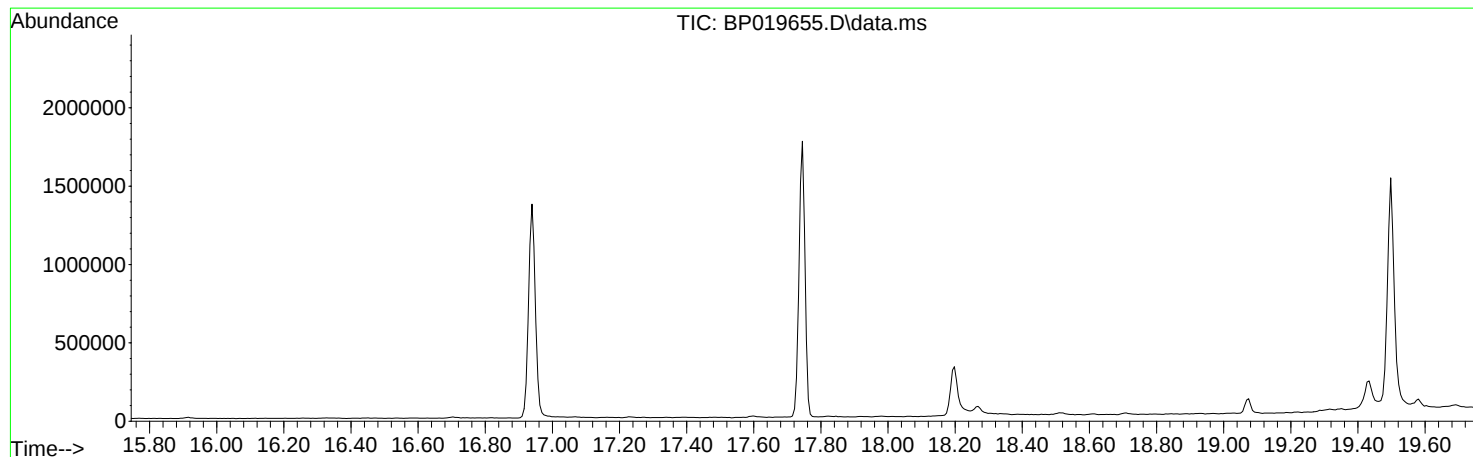




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	43298	PASS
68	69	0.00	2	1.6	864	PASS
69	198	0.00	100	31.6	53960	PASS
70	69	0.00	2	0.3	168	PASS
127	198	10	80	37.3	63702	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	170972	PASS
199	198	5	9	6.8	11582	PASS
275	198	10	60	30.0	51320	PASS
365	198	1	100	4.1	7003	PASS
441	198	0.01	100	16.1	27521	PASS
442	442	100	100	100.0	183978	PASS
443	442	15	24	19.3	35443	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021224\
Data File : BP019655.D
Acq On : 12 Feb 2024 10:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 12 23:57:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

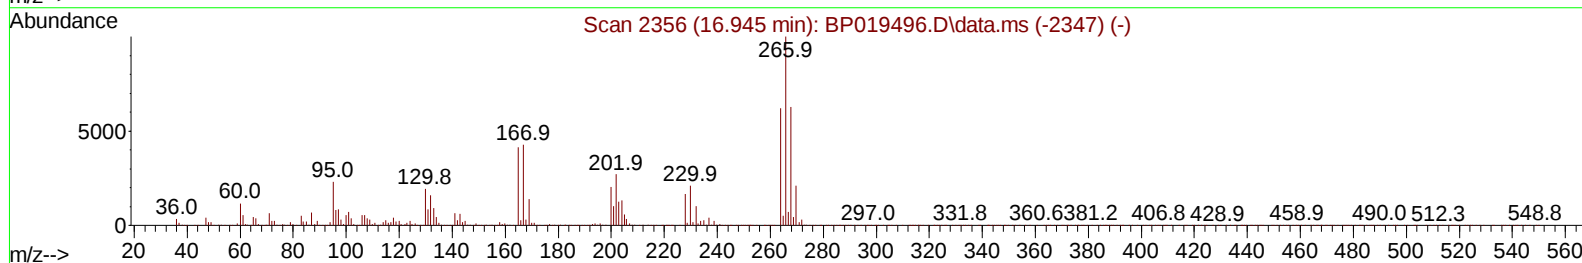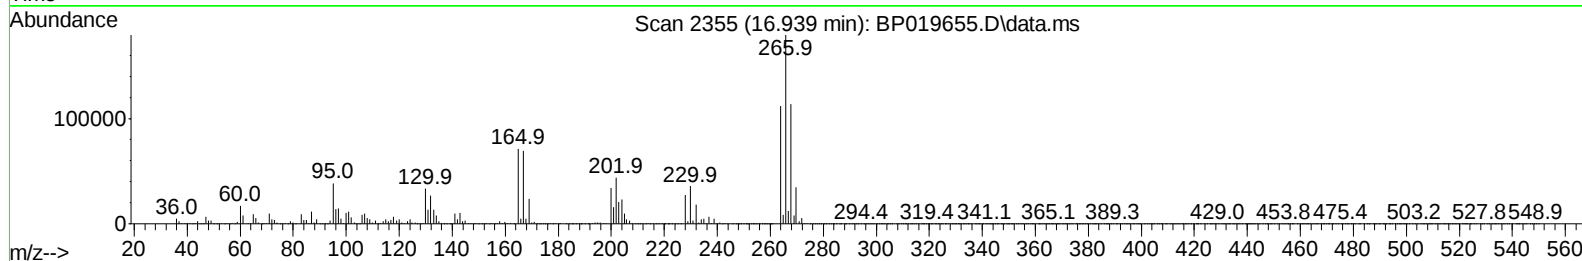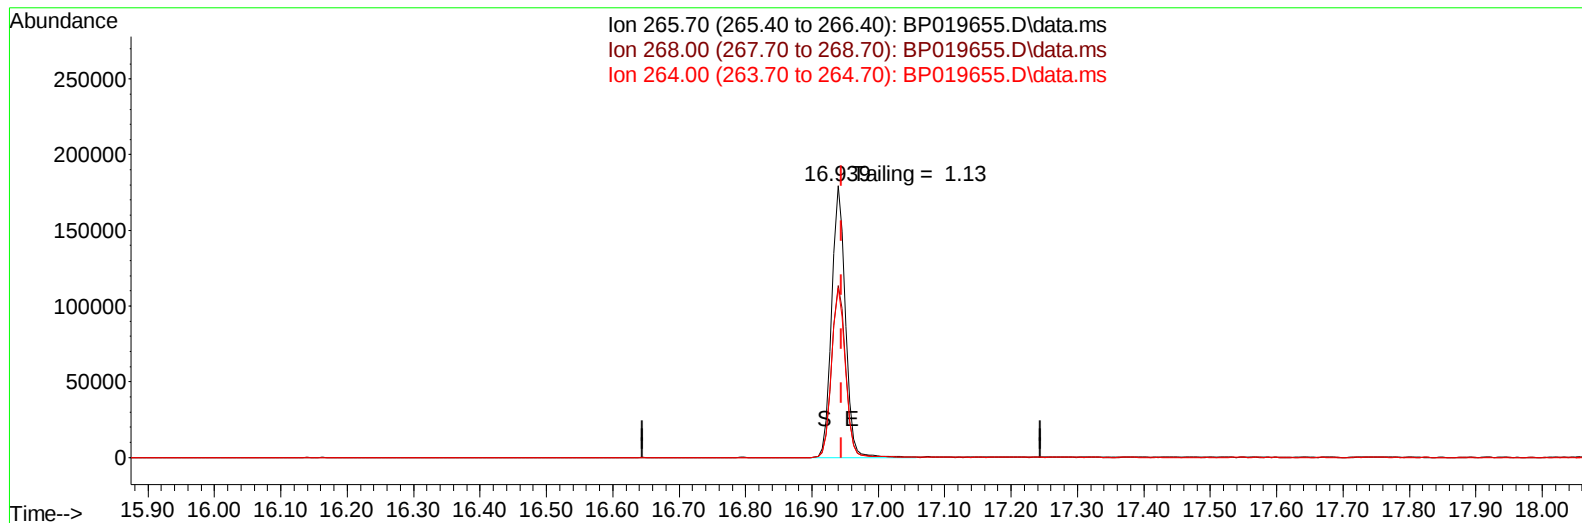

TIC: BP019655.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.006) 208057.75 ng




response 253460

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.27
264.00	62.10	62.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021224\
Data File : BP019655.D
Acq On : 12 Feb 2024 10:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 12 23:57:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

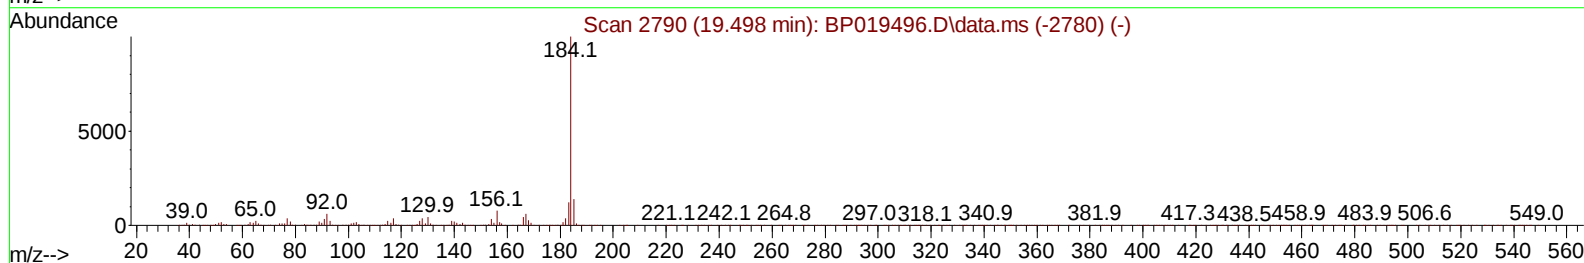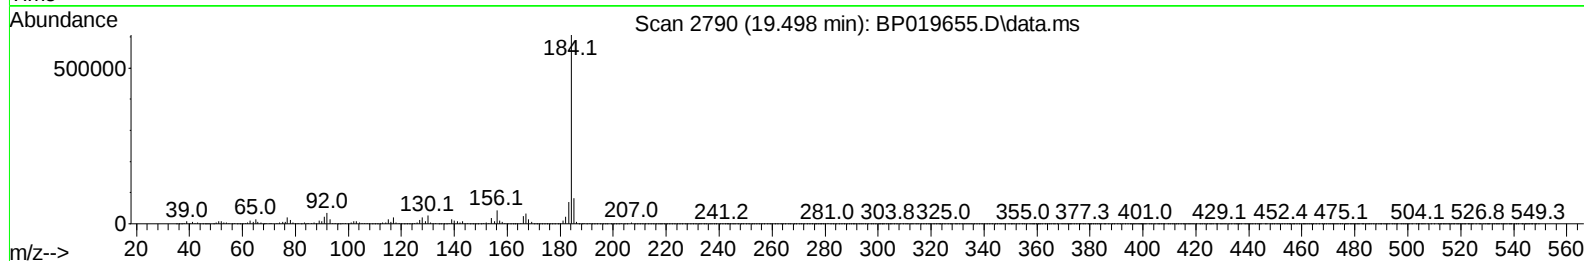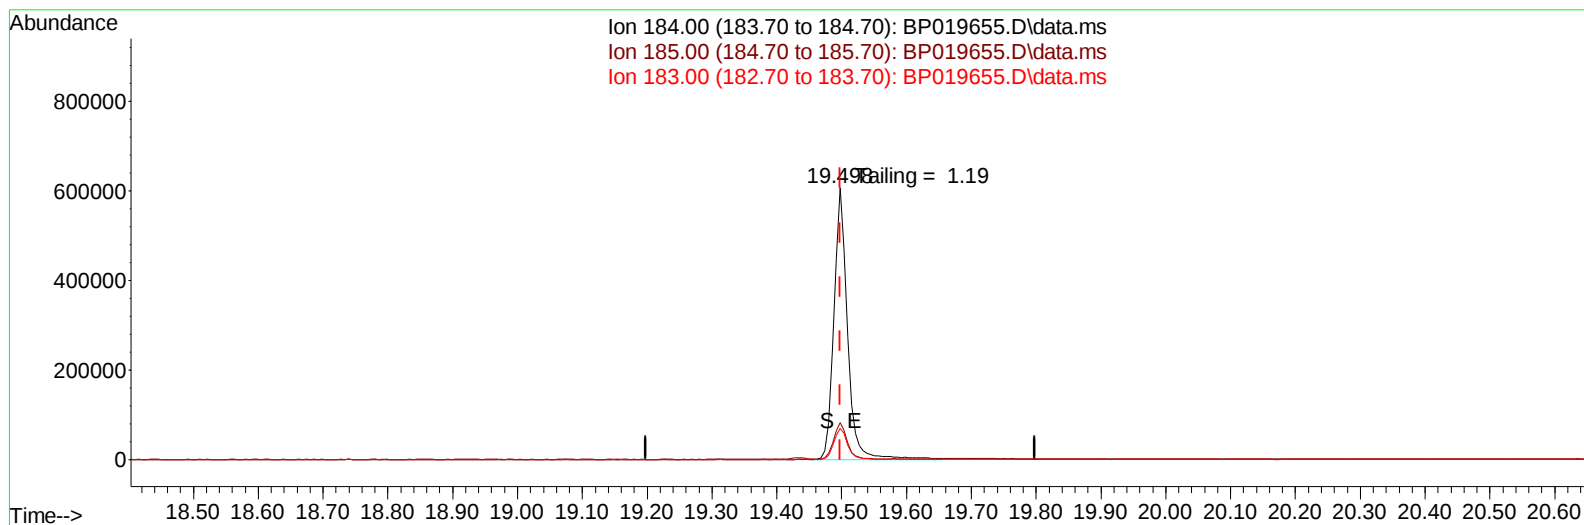

TIC: BP019655.D\data.ms

(77) Benzidine

19.498min (-0.000) 498856.38 ng

response 876072

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.62
183.00	12.10	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/12/2024	BNA_P	<u>BP019655.D</u>
Compound Name	Response	Retention Time
DDT	571910	20.698
DDD	92730	20.268
DDE	678	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
93408	665318	14.04

Instrument :
BNA_P
ClientSampleId :
DFTPP