

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021225\
 Data File : BP024048.D
 Acq On : 12 Feb 2025 13:41
 Operator : RC/JU
 Sample : PB166649BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP024048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	42	rVB	106211	146292	1.60%	0.156%
2	3.675	96	100	122	rBV	1302887	2070584	22.67%	2.215%
3	3.993	150	154	160	rVB	24238	34947	0.38%	0.037%
4	6.916	642	651	663	rBV	1804678	2739646	29.99%	2.930%
5	7.075	671	678	690	rBV	1351126	2041342	22.35%	2.183%
6	7.275	705	712	725	rBV	1736836	2795885	30.61%	2.990%
7	7.740	782	791	802	rBV	1254345	1907409	20.88%	2.040%
8	8.440	902	910	926	rBV	2316449	3499573	38.31%	3.743%
9	8.881	977	985	998	rBV	1518562	2463858	26.97%	2.635%
10	9.010	1003	1007	1012	rVB2	14102	19845	0.22%	0.021%
11	9.599	1100	1107	1119	rBV	1278080	1921552	21.04%	2.055%
12	10.140	1189	1199	1216	rBV	1953976	3438256	37.64%	3.677%
13	10.516	1254	1263	1273	rBV	1748565	2886082	31.60%	3.087%
14	10.640	1277	1284	1306	rVV	1989964	3401799	37.24%	3.638%
15	12.098	1527	1532	1539	rBV	35391	58203	0.64%	0.062%
16	13.334	1733	1742	1751	rVB9	5787	16225	0.18%	0.017%
17	13.781	1808	1818	1831	rBV	3127410	4613504	50.51%	4.934%
18	14.063	1859	1866	1882	rBV	4163487	6027741	65.99%	6.447%
19	14.375	1910	1919	1927	rBV	2779946	3885437	42.54%	4.156%
20	14.592	1948	1956	1972	rBV	950486	1802450	19.73%	1.928%
21	14.734	1978	1980	1987	rVB7	9525	12558	0.14%	0.013%
22	14.792	1987	1990	1994	rVB6	7300	10581	0.12%	0.011%
23	15.051	2031	2034	2040	rVB8	8404	13371	0.15%	0.014%
24	15.386	2085	2091	2104	rBV	5966941	7461956	81.69%	7.981%
25	15.504	2104	2111	2126	rVV	600599	1059244	11.60%	1.133%
26	15.634	2129	2133	2139	rVB2	22100	37577	0.41%	0.040%
27	15.957	2183	2188	2192	rBV4	9164	17643	0.19%	0.019%
28	16.663	2302	2308	2311	rBV4	14999	25055	0.27%	0.027%
29	16.822	2331	2335	2345	rVB4	31574	60090	0.66%	0.064%
30	16.963	2354	2359	2365	rVB2	13533	19339	0.21%	0.021%
31	17.063	2372	2376	2381	rBV7	8311	13292	0.15%	0.014%
32	17.180	2389	2396	2406	rBV	3178767	4549380	49.81%	4.866%
33	17.286	2406	2414	2431	rVV	5333244	8119816	88.90%	8.685%
34	18.122	2552	2556	2559	rBV5	8426	12696	0.14%	0.014%
35	19.198	2735	2739	2745	rBV3	56628	85436	0.94%	0.091%
36	19.274	2749	2752	2755	rBV	49281	71363	0.78%	0.076%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021225\
Data File : BP024048.D
Acq On : 12 Feb 2025 13:41
Operator : RC/JU
Sample : PB166649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK649

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	19.657	2811	2817	2827	rBV	6836378	9134159	100.00%	9.770%
38	19.751	2829	2833	2840	rVB4	61190	83666	0.92%	0.089%
39	21.621	3146	3151	3164	rBV	3018211	4592450	50.28%	4.912%
40	24.762	3676	3685	3707	rVB	2921344	7940663	86.93%	8.493%
41	24.980	3715	3722	3741	rVB	1526133	4404698	48.22%	4.711%




Sum of corrected areas: 93495663

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021225\
Data File : BP024048.D
Acq On : 12 Feb 2025 13:41
Operator : RC/JU
Sample : PB166649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

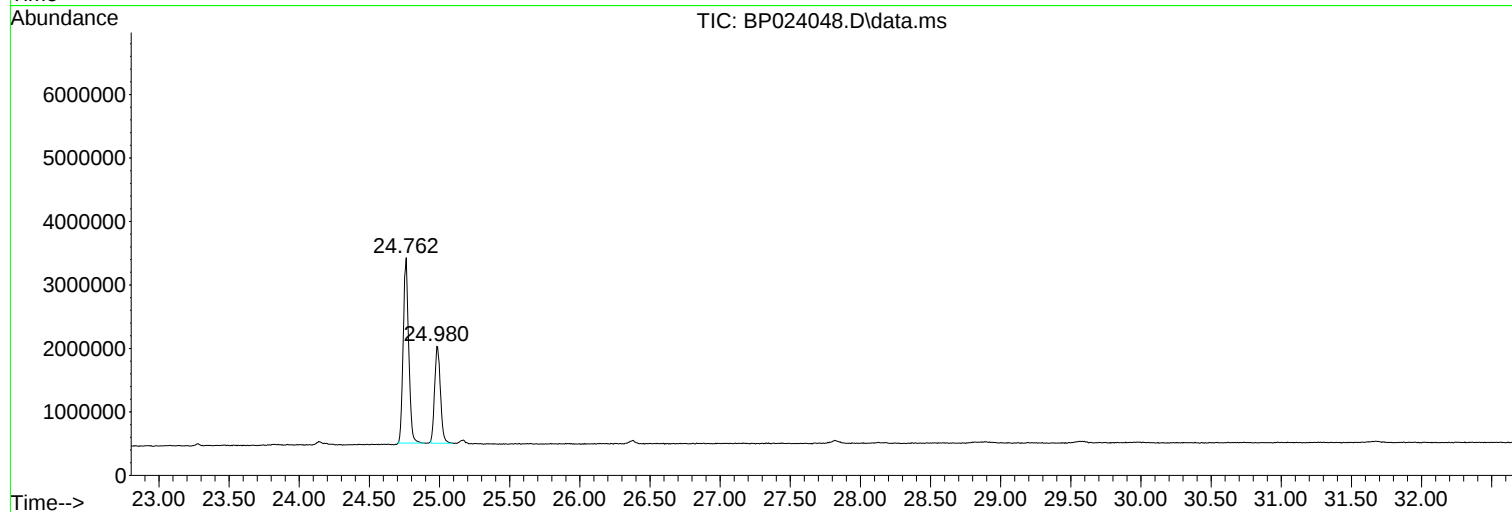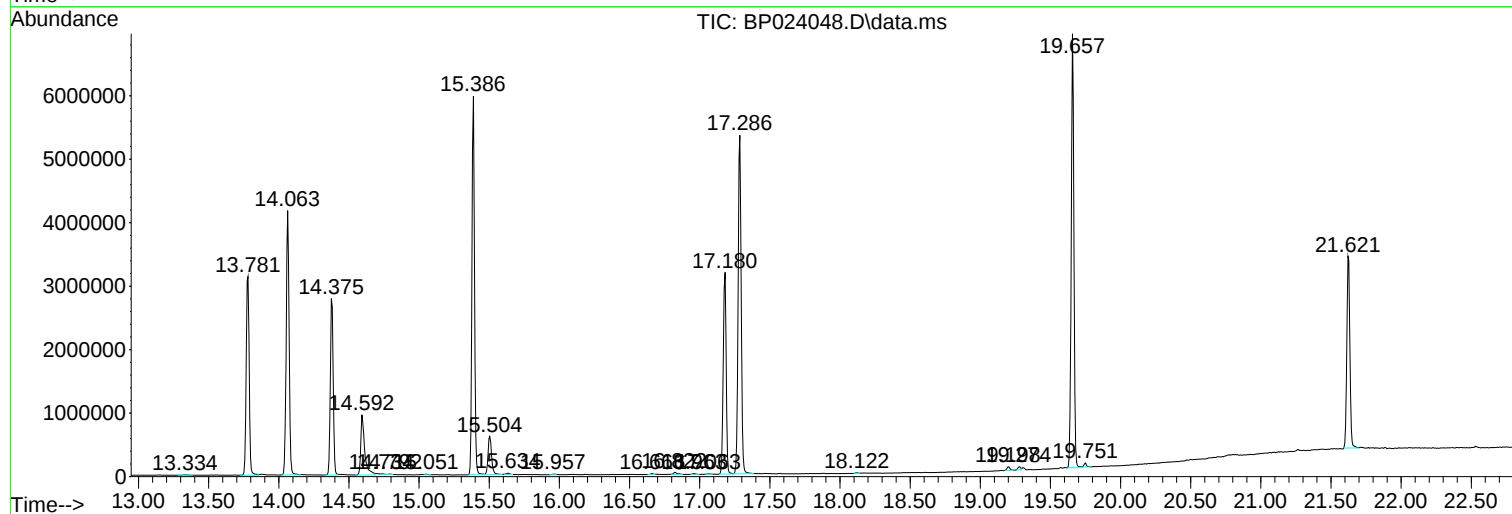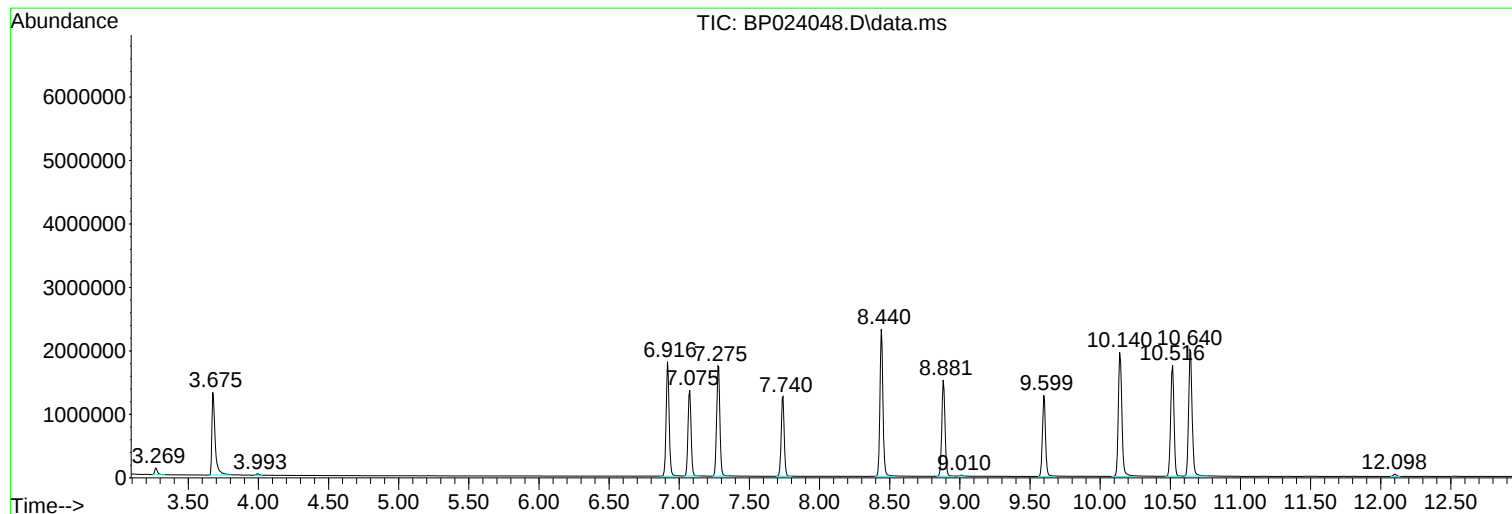

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021225\
Data File : BP024048.D
Acq On : 12 Feb 2025 13:41
Operator : RC/JU
Sample : PB166649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021225\
Data File : BP024048.D
Acq On : 12 Feb 2025 13:41
Operator : RC/JU
Sample : PB166649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc