
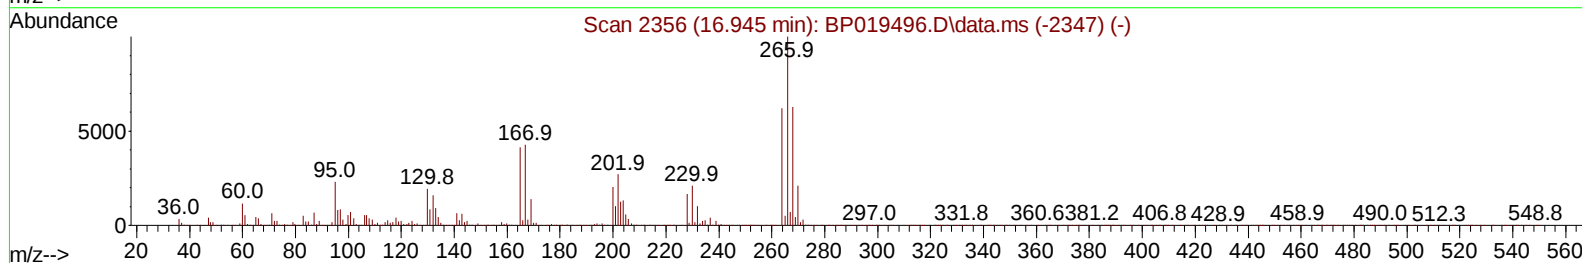
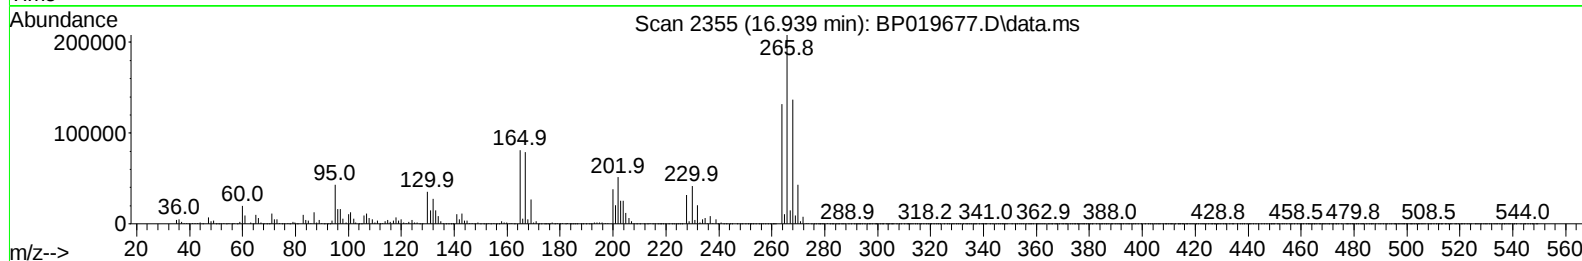


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021324\
Data File : BP019677.D
Acq On : 13 Feb 2024 10:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 00:20:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

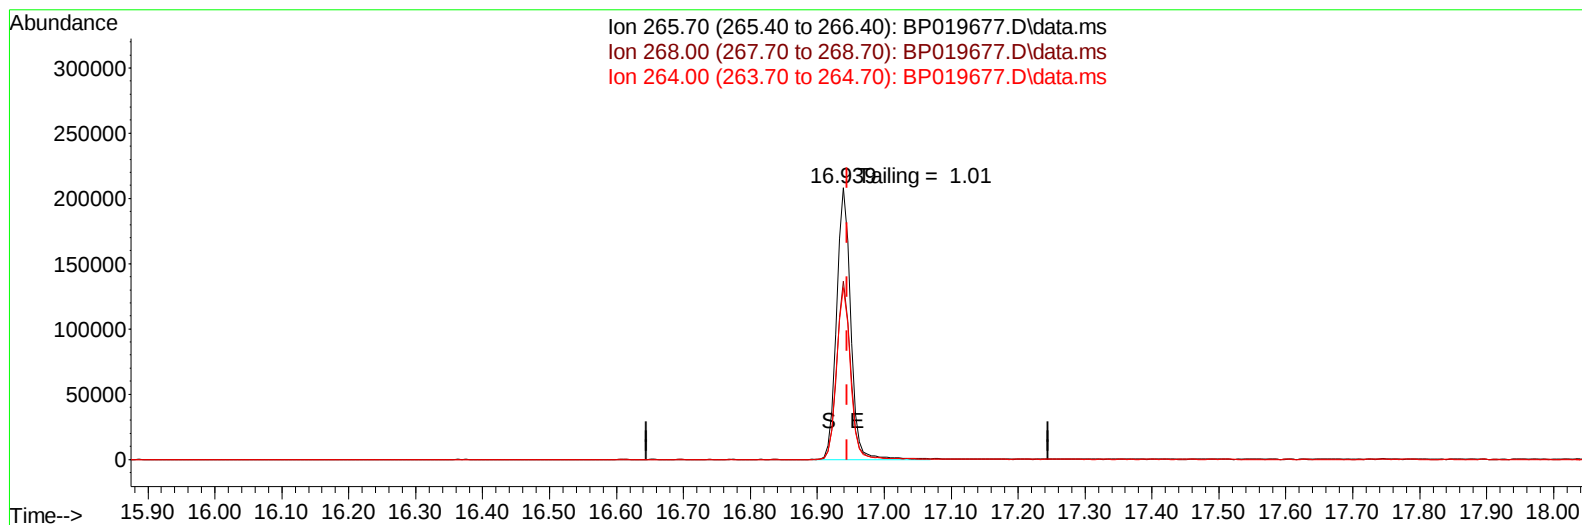




TIC: BP019677.D\data.ms

(70) Pentachlorophenol (C)**16.939min (-0.006) 101485.82 ng****response 301699**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.76
264.00	62.10	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021324\
Data File : BP019677.D
Acq On : 13 Feb 2024 10:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 00:20:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

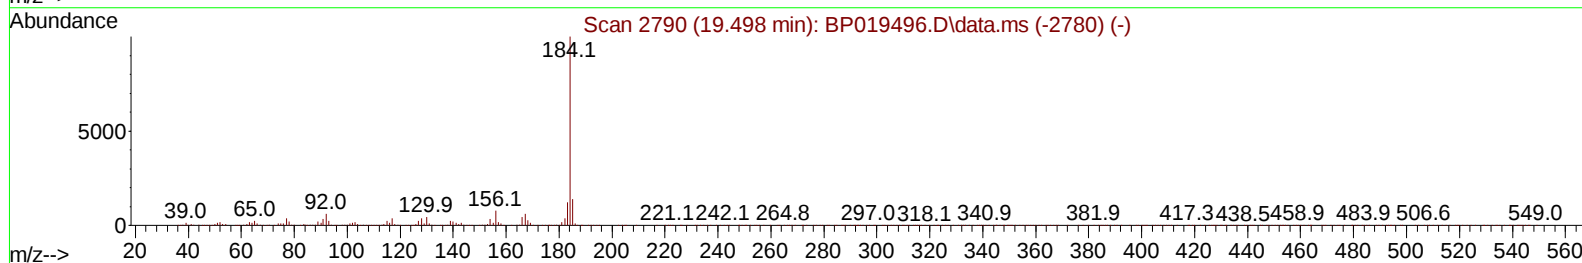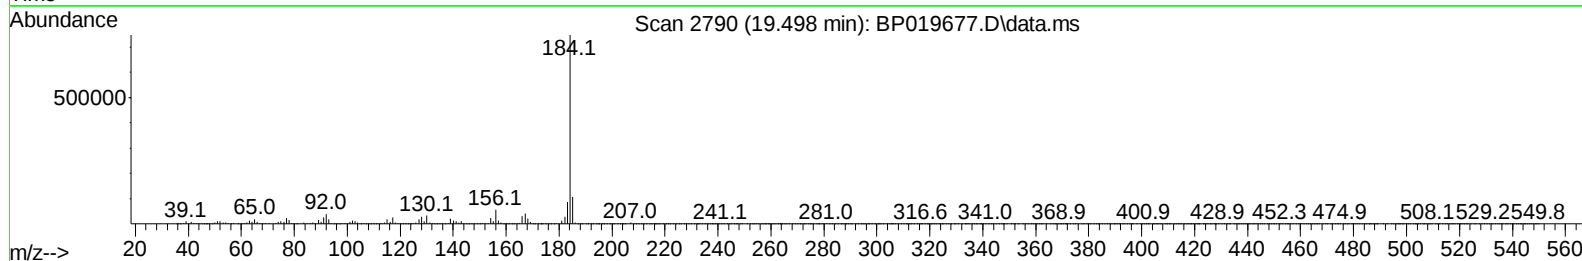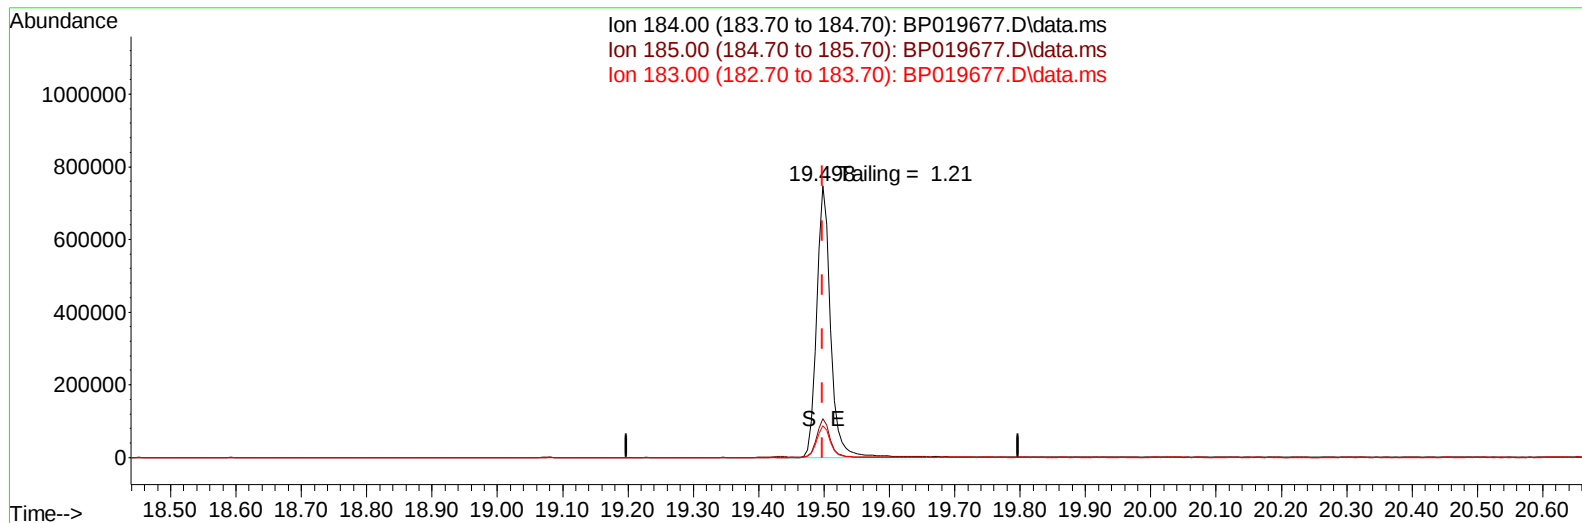

TIC: BP019677.D\data.ms

(77) Benzidine**19.498min (+ 0.000) 26702.79 ng****response 1109834**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.28
183.00	12.10	11.62
0.00	0.00	0.00