


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021324\
 Data File : BP019677.D
 Acq On : 13 Feb 2024 10:38
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 01 00:51:48 2024

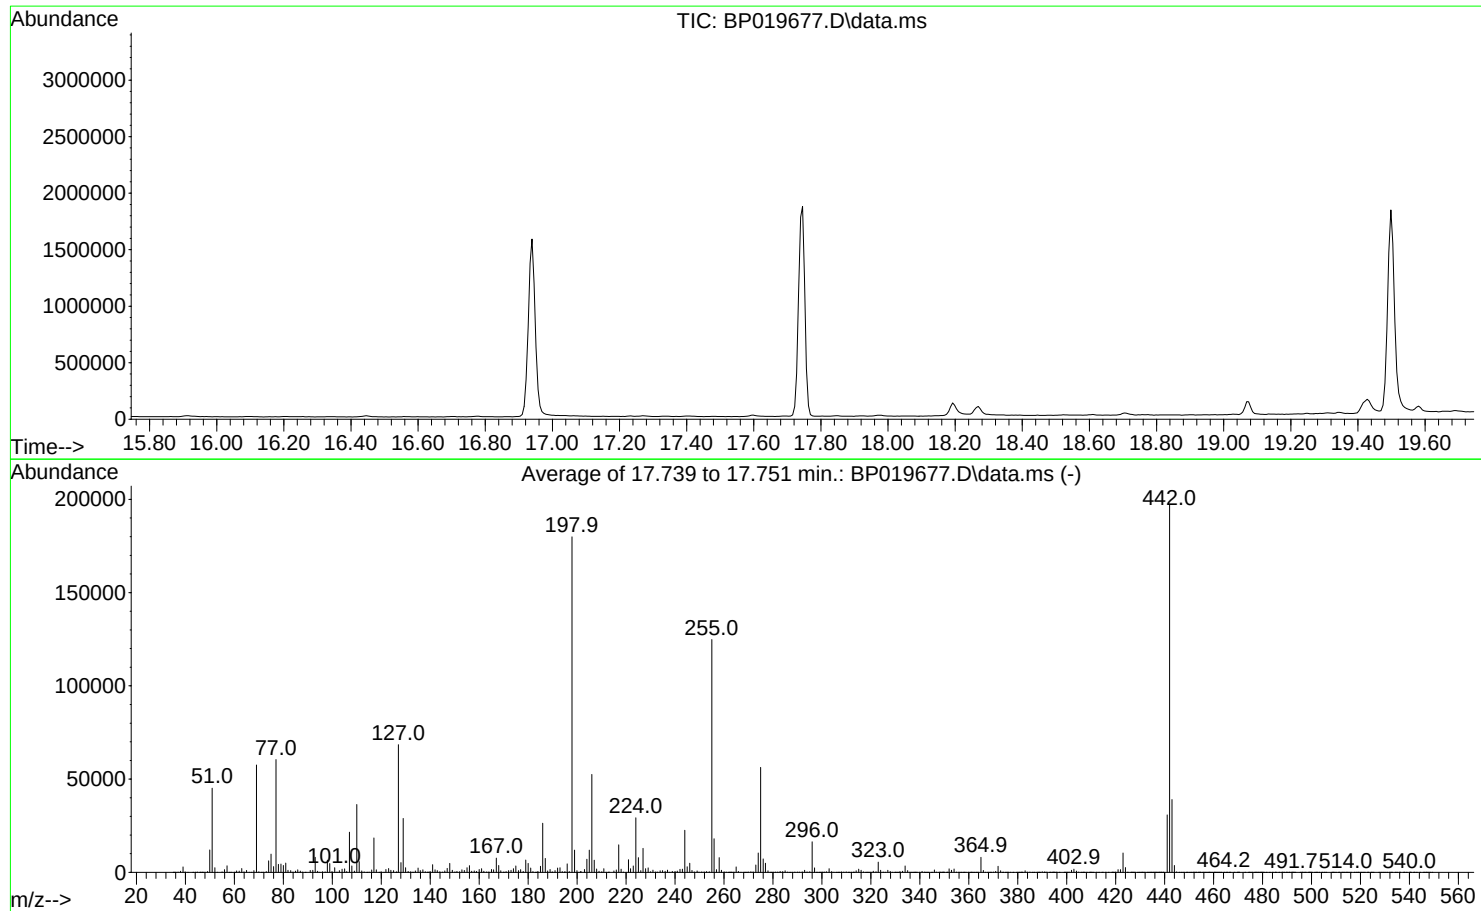




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	45152	PASS
68	69	0.00	2	1.7	962	PASS
69	198	0.00	100	32.0	57563	PASS
70	69	0.00	2	0.6	322	PASS
127	198	10	80	38.1	68501	PASS
197	198	0.00	2	0.2	434	PASS
198	198	100	100	100.0	179911	PASS
199	198	5	9	6.6	11942	PASS
275	198	10	60	31.3	56303	PASS
365	198	1	100	4.5	8103	PASS
441	198	0.01	100	17.1	30801	PASS
442	442	100	100	100.0	197244	PASS
443	442	15	24	19.8	39027	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021324\
Data File : BP019677.D
Acq On : 13 Feb 2024 10:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 14 00:20:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

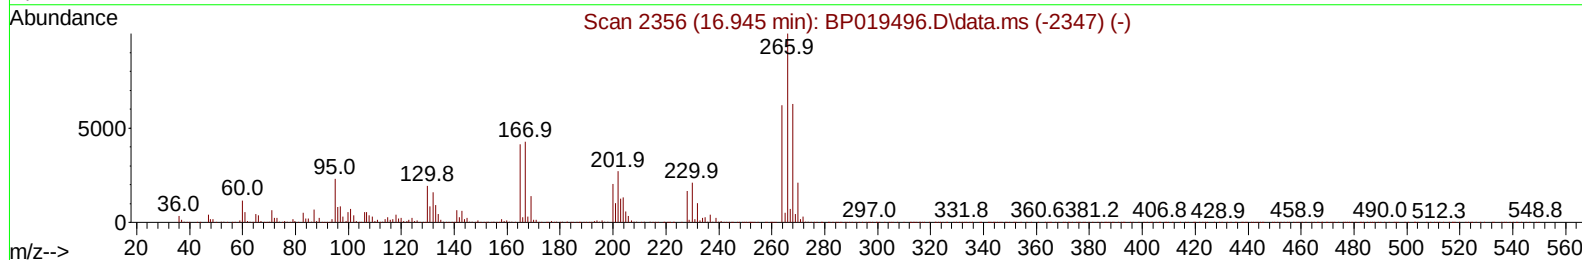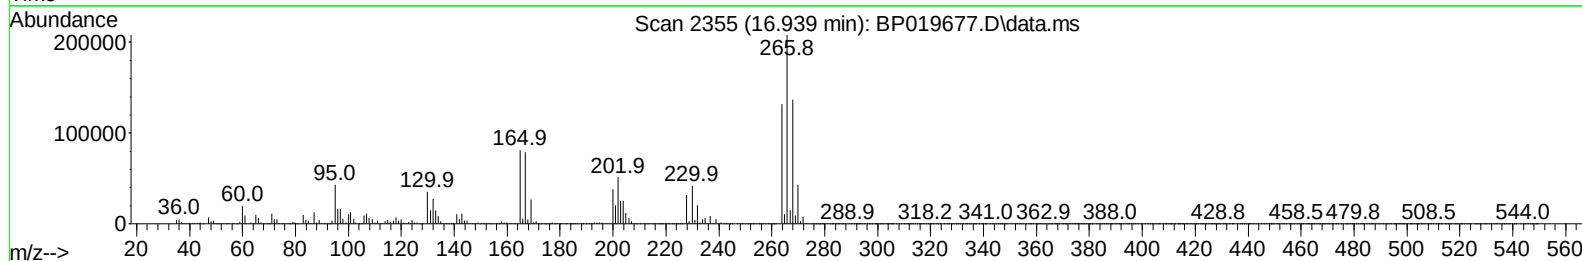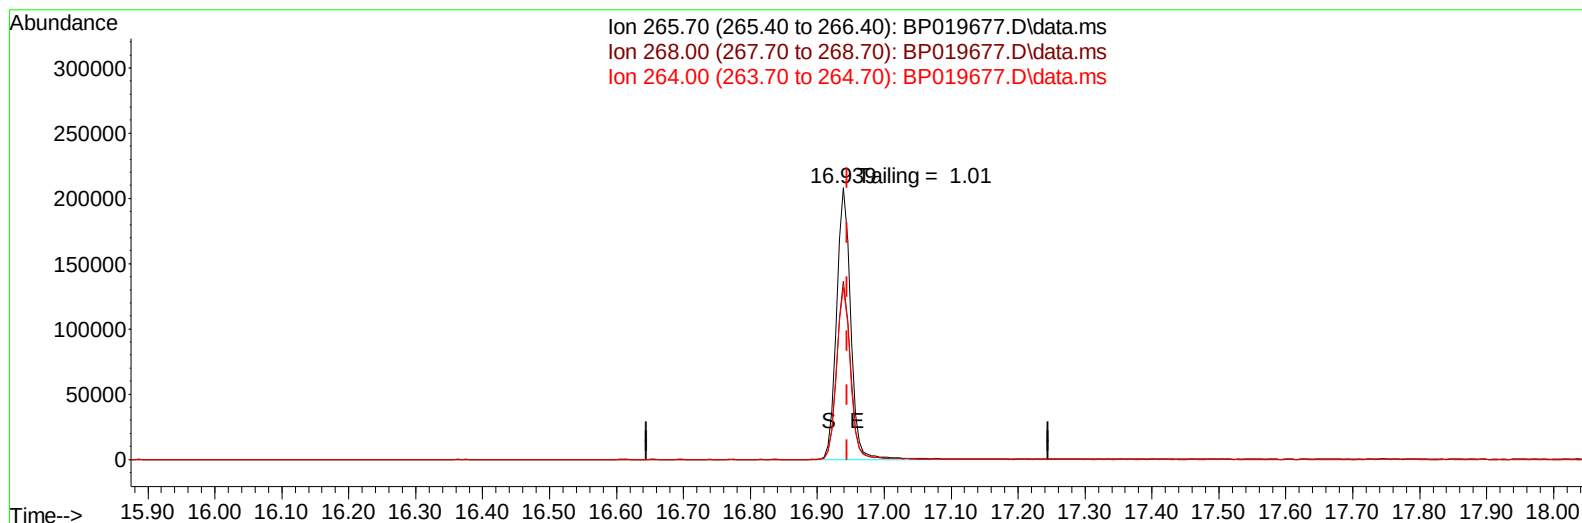

TIC: BP019677.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.006) 101485.82 ng




response 301699

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.76
264.00	62.10	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021324\
Data File : BP019677.D
Acq On : 13 Feb 2024 10:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 14 00:20:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

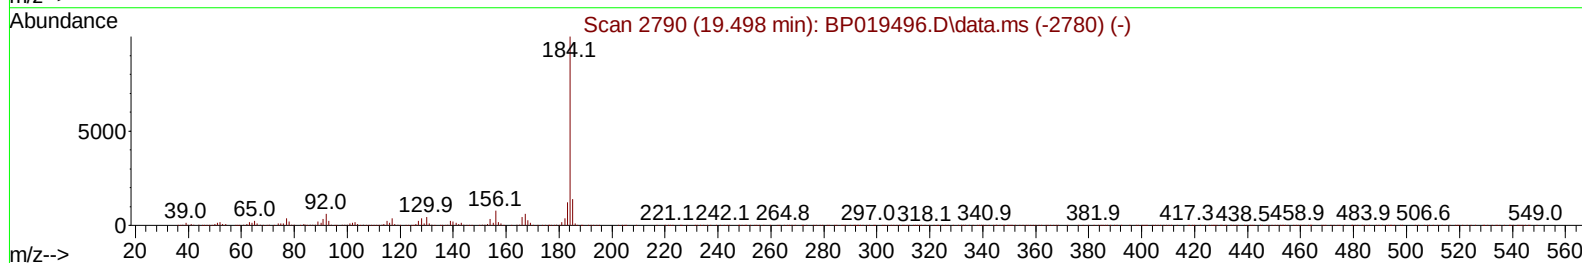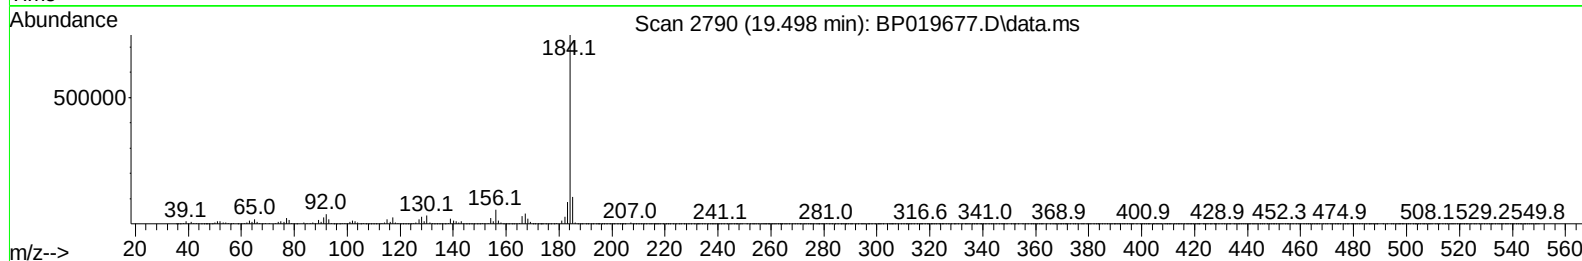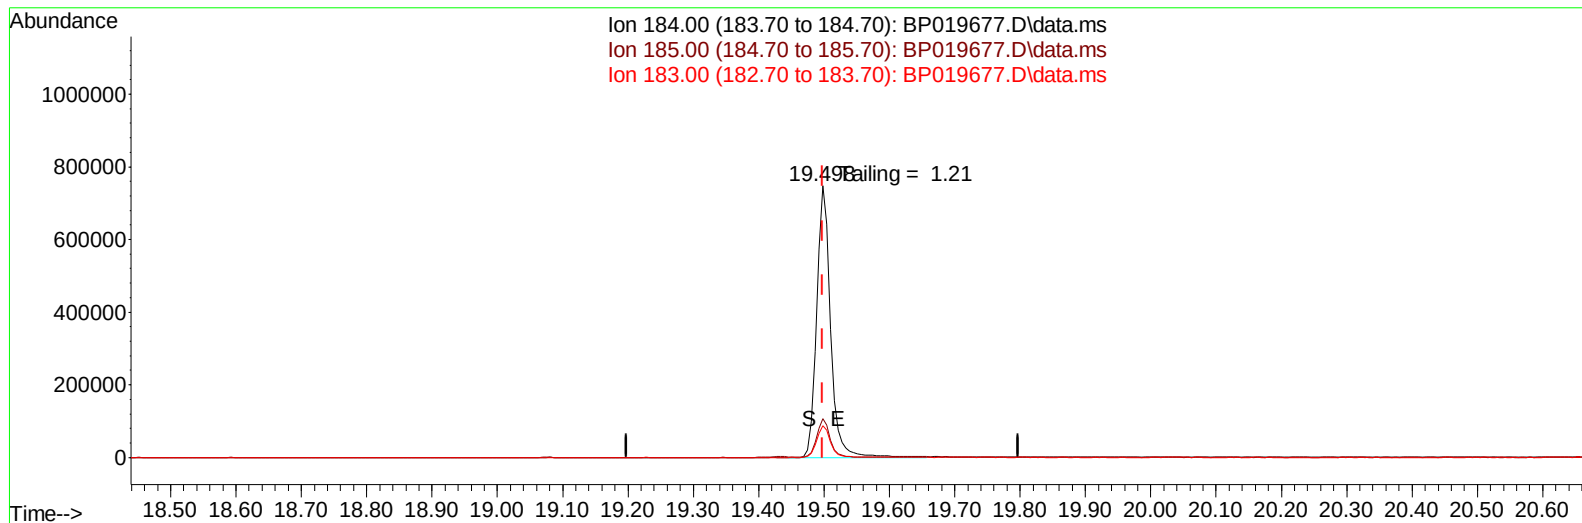

TIC: BP019677.D\data.ms

(77) Benzidine

19.498min (+ 0.000) 26702.79 ng

response 1109834

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.28
183.00	12.10	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/13/2024	BNA_P	<u>BP019677.D</u>
Compound Name	Response	Retention Time
DDT	779502	20.698
DDD	23796	20.269
DDE	2062	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25858	805360	3.21

Instrument :
BNA_P
ClientSampleId :
DFTPP