
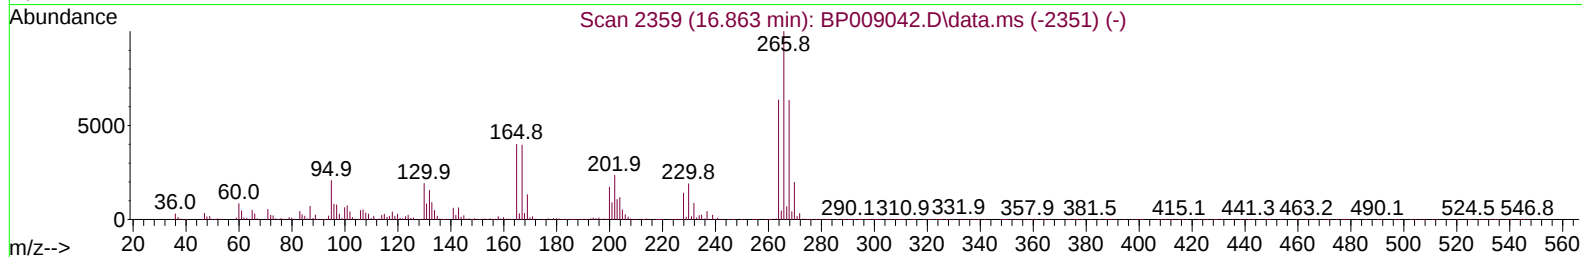
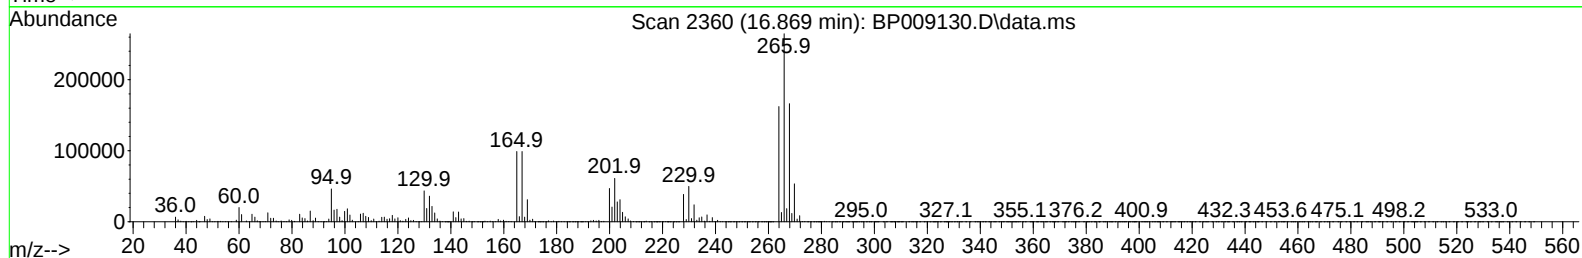


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP021422\  
 Data File : BP009130.D  
 Acq On : 14 Feb 2022 12:16  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 13:49:44 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020722.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Feb 07 15:13:17 2022  
 Response via : Initial Calibration

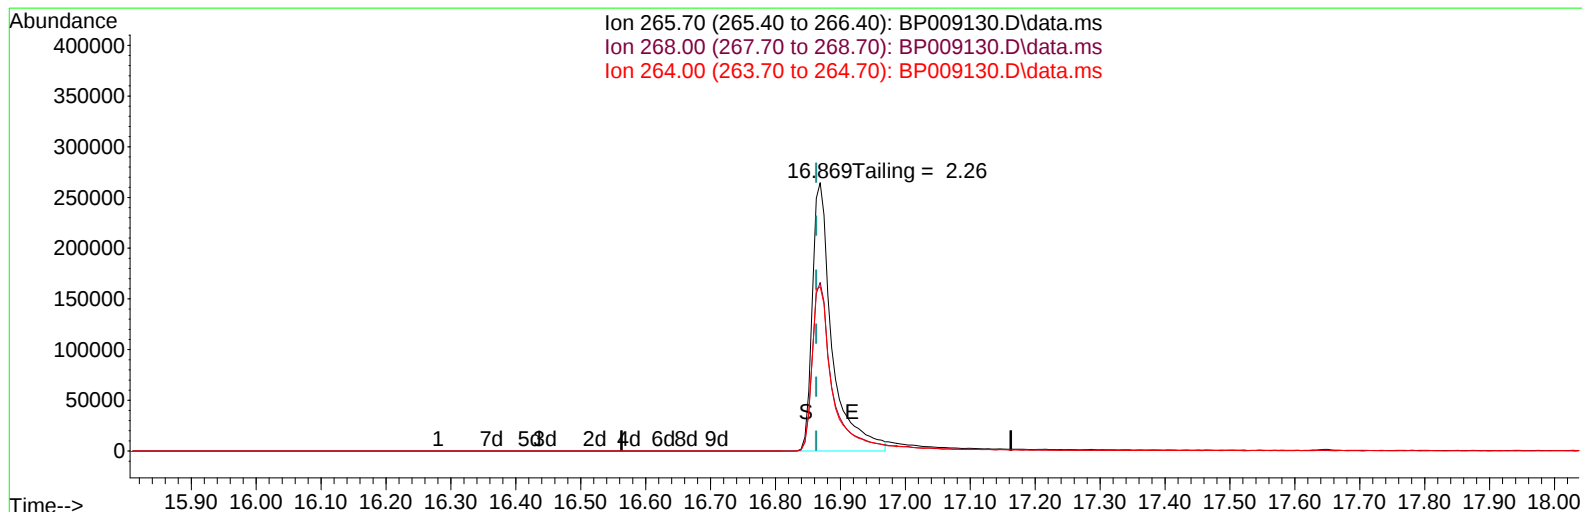

TIC: BP009130.D\data.ms

**(70) Pentachlorophenol (C)**




16.869min (+ 0.006) 731744.53 ng m

response 590165

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.60  | 62.78  |
| 264.00 | 62.90  | 61.26  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP021422\  
 Data File : BP009130.D  
 Acq On : 14 Feb 2022 12:16  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 13:49:44 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020722.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Feb 07 15:13:17 2022  
 Response via : Initial Calibration

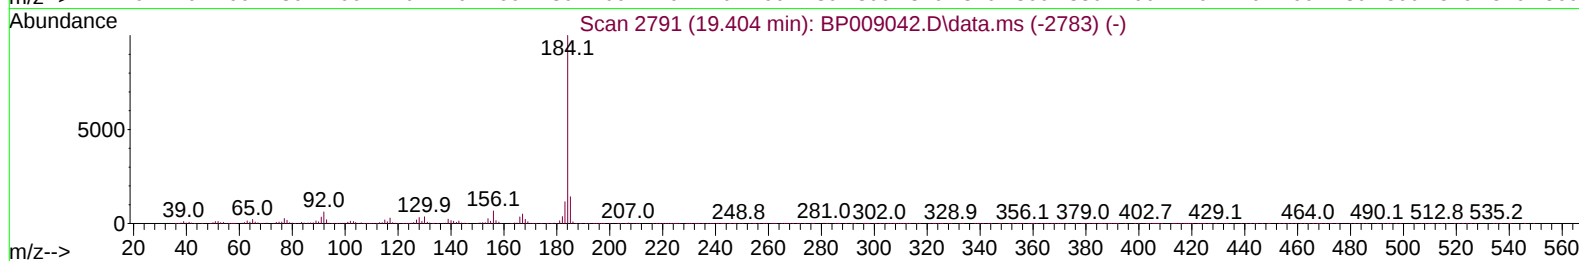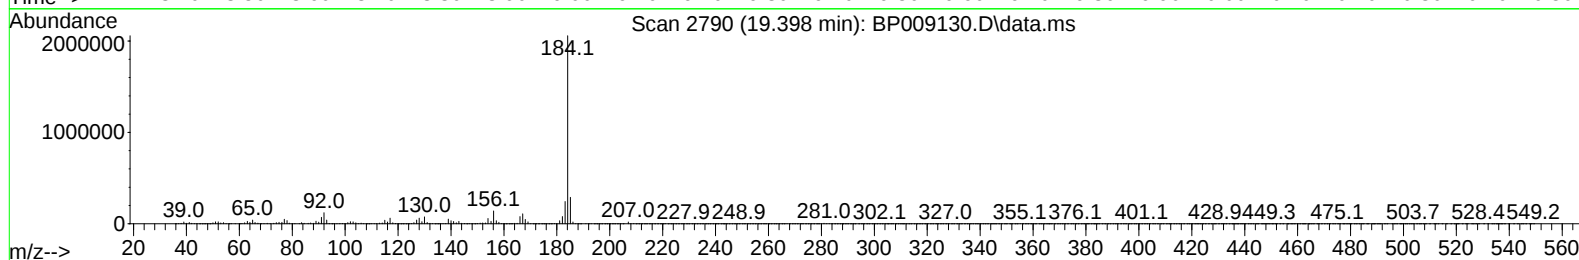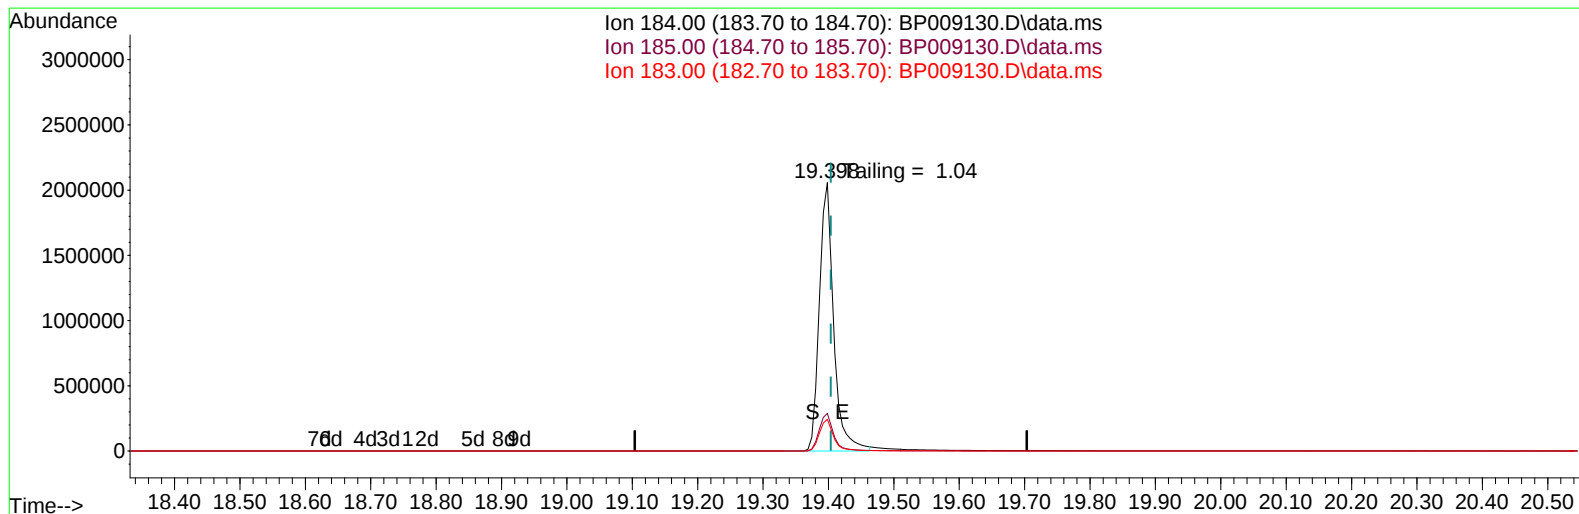

TIC: BP009130.D\data.ms

**(77) Benzidine****19.398min (-0.006) 6702.21 ng m****response 3191867**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.20  | 14.03  |
| 183.00 | 11.90  | 11.81  |
| 0.00   | 0.00   | 0.00   |