

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
Data File : BP009132.D
Acq On : 14 Feb 2022 13:34
Operator : CG/JU
Sample : PB142649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142649BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	402	409	434	rBV	3650981	5998634	37.73%	9.255%
2	6.993	673	681	702	rBV	3254383	6056412	38.09%	9.344%
3	7.793	810	817	835	rBV	726863	1213496	7.63%	1.872%
4	8.958	1006	1015	1048	rBV	2249614	4094815	25.76%	6.318%
5	10.593	1282	1293	1311	rBV	851553	1644041	10.34%	2.537%
6	13.057	1705	1712	1738	rBV	6484866	10786588	67.85%	16.642%
7	14.440	1939	1947	1967	rBV	1409090	2424489	15.25%	3.741%
8	15.940	2193	2202	2228	rBV	4714969	8530626	53.66%	13.162%
9	17.198	2409	2416	2431	rBV	1757778	2943602	18.52%	4.542%
10	19.763	2846	2852	2870	rBV	11985827	15898250	100.00%	24.529%
11	21.298	3108	3113	3122	rBV	2033147	2886756	18.16%	4.454%
12	23.698	3515	3521	3536	rVB	1035509	2336563	14.70%	3.605%




Sum of corrected areas: 64814272

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
Data File : BP009132.D
Acq On : 14 Feb 2022 13:34
Operator : CG/JU
Sample : PB142649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142649BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

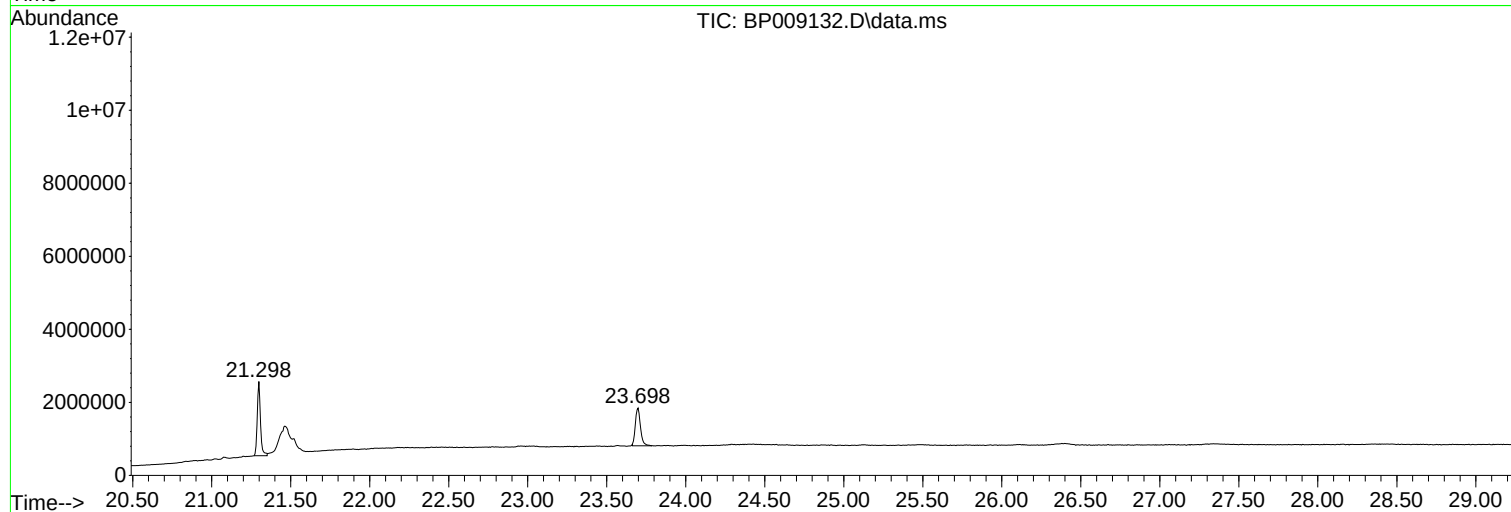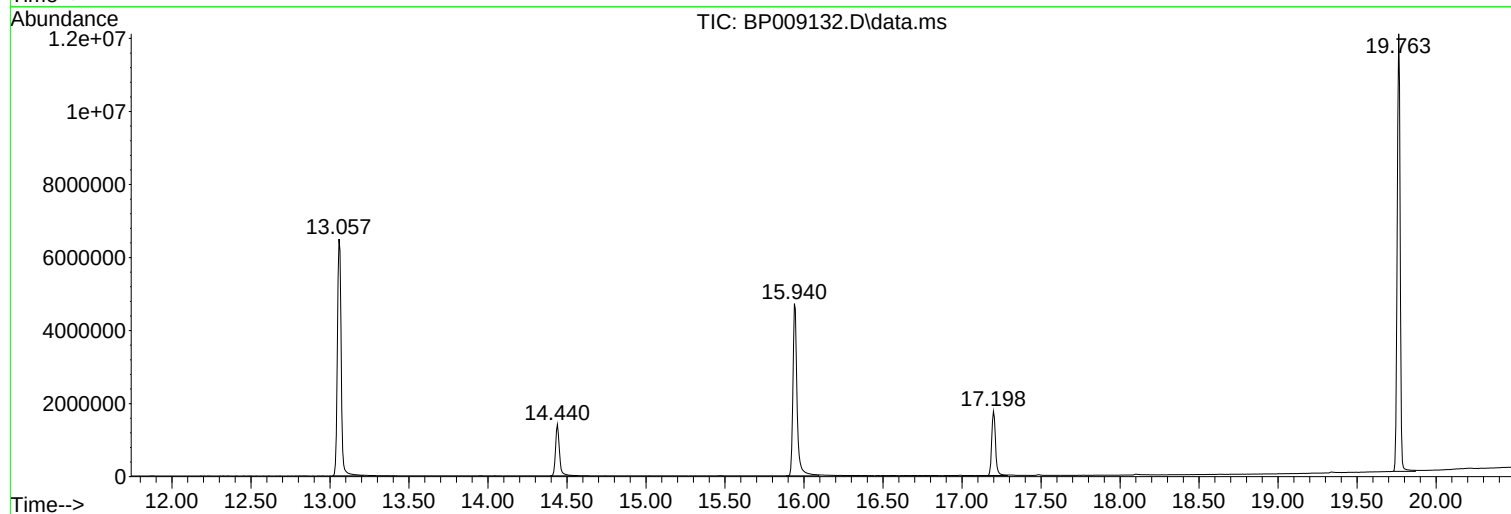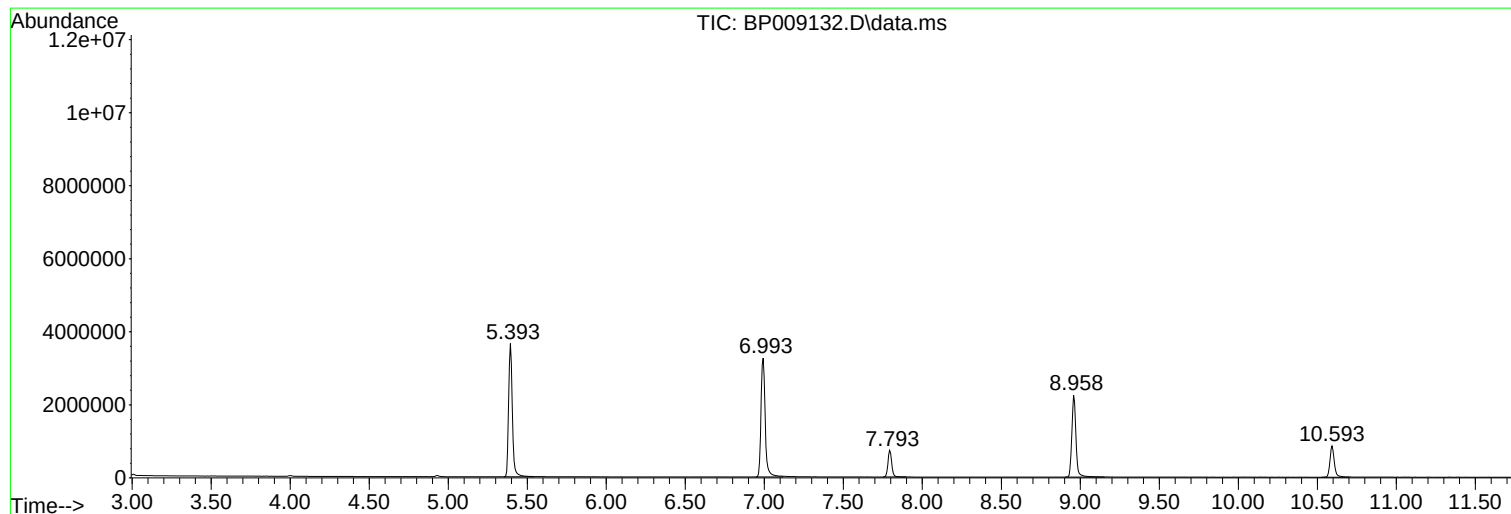

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
Data File : BP009132.D
Acq On : 14 Feb 2022 13:34
Operator : CG/JU
Sample : PB142649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142649BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
Data File : BP009132.D
Acq On : 14 Feb 2022 13:34
Operator : CG/JU
Sample : PB142649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142649BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------