

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
 Data File : BP009144.D
 Acq On : 14 Feb 2022 20:34
 Operator : CG/JU
 Sample : N1524-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	402	409	436	rBV	2233285	3953958	38.64%	8.378%
2	6.987	673	680	701	rBV	1972572	3853724	37.66%	8.165%
3	7.793	809	817	834	rBV	687943	1202195	11.75%	2.547%
4	8.958	1003	1015	1041	rBV	1299063	2634388	25.74%	5.582%
5	10.593	1283	1293	1309	rBV	786400	1578631	15.43%	3.345%
6	13.057	1704	1712	1744	rBV	4006823	6650185	64.99%	14.091%
7	14.434	1939	1946	1964	rVV	1222920	2100805	20.53%	4.451%
8	15.940	2194	2202	2221	rBV	2813033	5056090	49.41%	10.713%
9	17.192	2409	2415	2430	rBV	1560337	2584576	25.26%	5.476%
10	18.092	2564	2568	2583	rBV2	71692	145895	1.43%	0.309%
11	19.757	2845	2851	2861	rBV	8314528	10233127	100.00%	21.682%
12	20.992	3058	3061	3070	rBV	283815	393333	3.84%	0.833%
13	21.292	3107	3112	3126	rBV	2207641	3133264	30.62%	6.639%
14	21.404	3128	3131	3142	rVV	189242	343783	3.36%	0.728%
15	23.680	3512	3518	3533	rVB2	1515527	3331894	32.56%	7.060%




Sum of corrected areas: 47195848

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
Data File : BP009144.D
Acq On : 14 Feb 2022 20:34
Operator : CG/JU
Sample : N1524-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

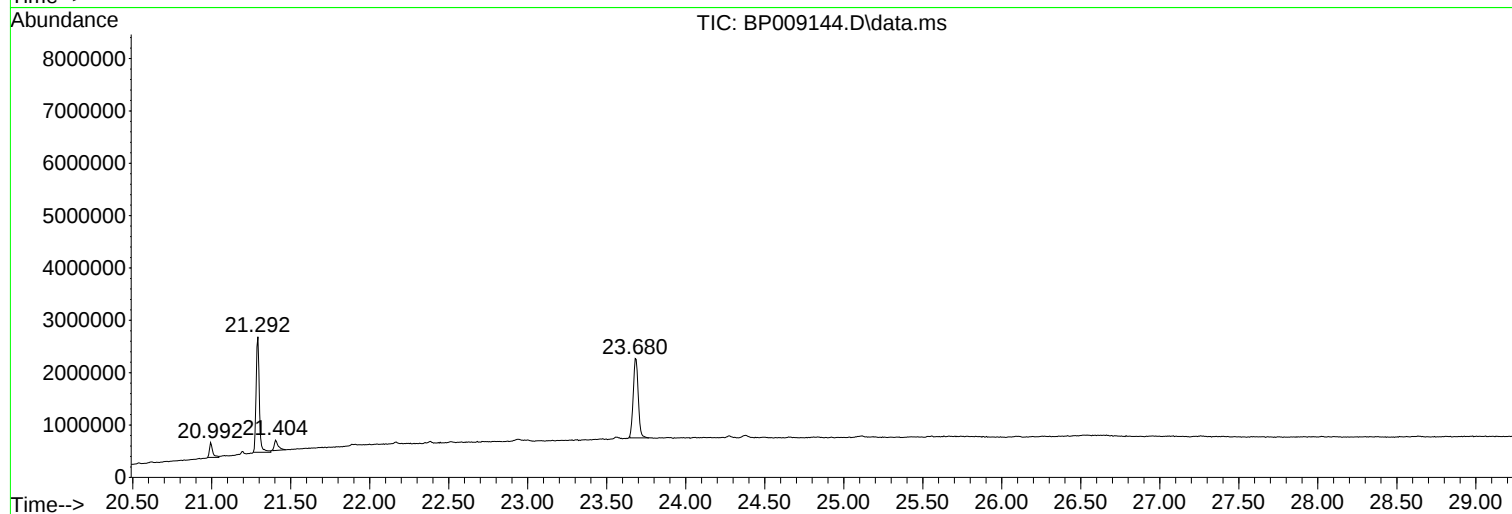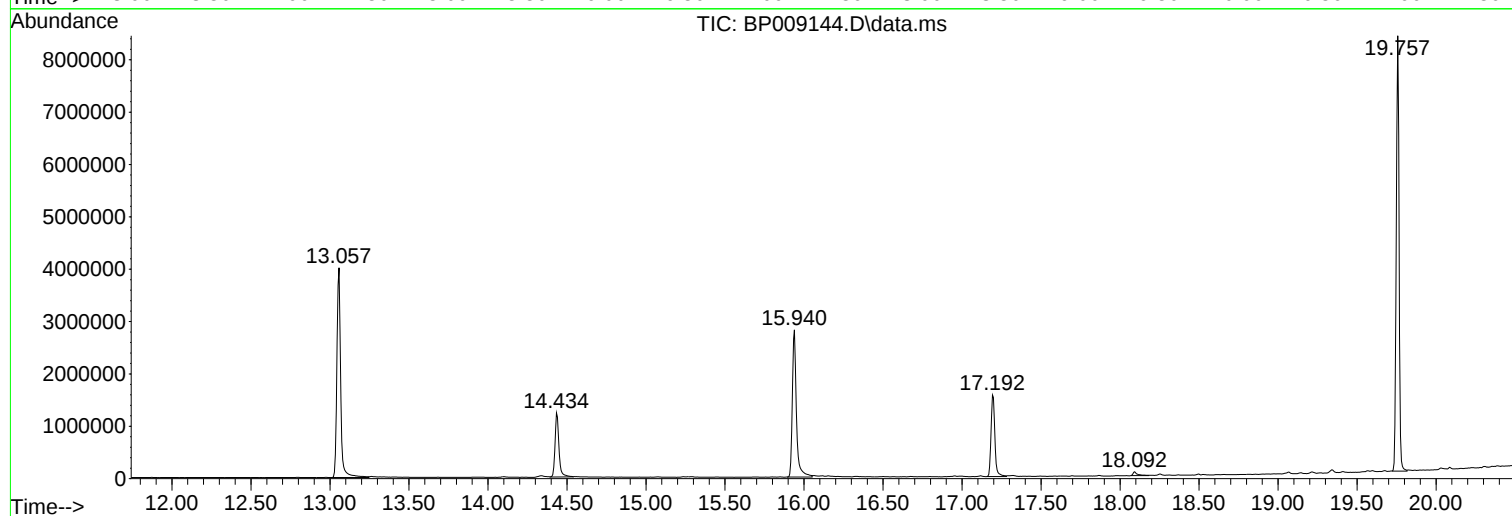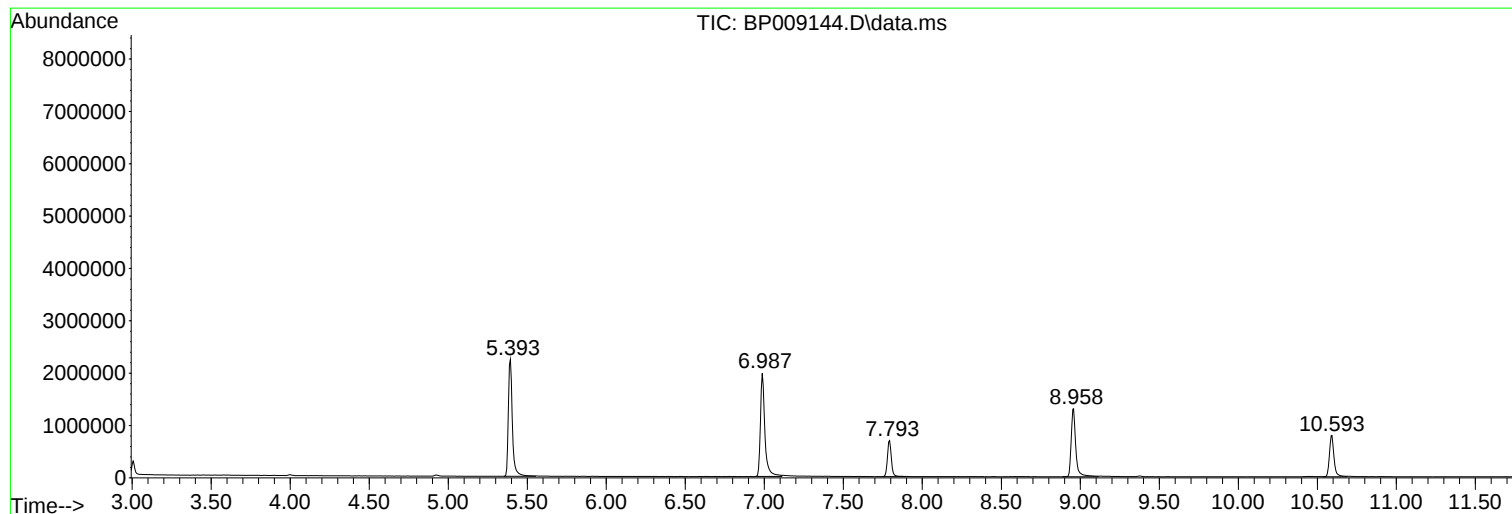

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
Data File : BP009144.D
Acq On : 14 Feb 2022 20:34
Operator : CG/JU
Sample : N1524-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 5-Eicosene, (E)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.992	2.51 ng	393333	Chrysene-d12	21.292

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		5-Eicosene, (E)-	280	C20H40	074685-30-6	98
2		E-15-Heptadecenal	252	C17H32O	1000130-97-9	97
3		1-Tetracosene	336	C24H48	010192-32-2	95
4		1-Hexacosene	364	C26H52	018835-33-1	95
5		Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94

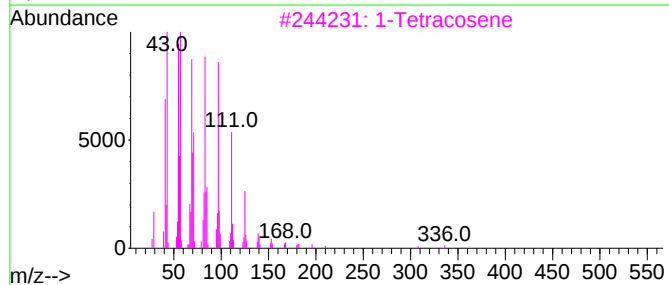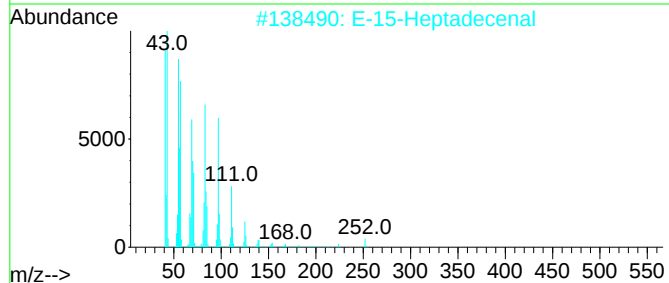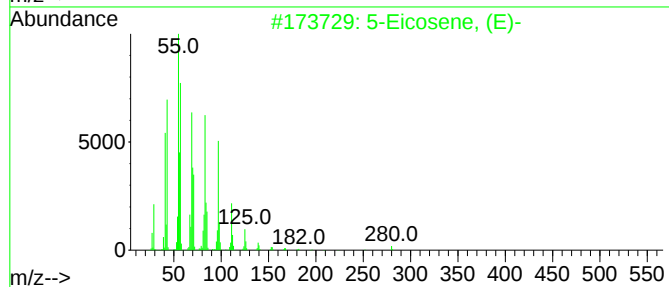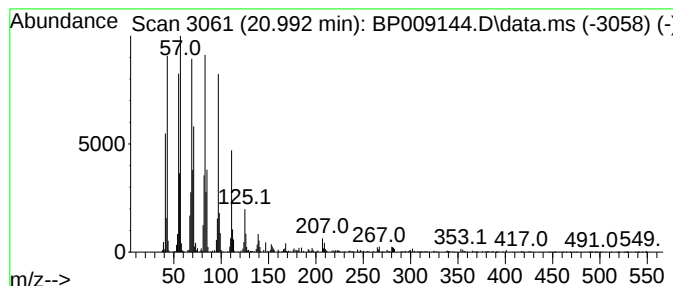

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
Data File : BP009144.D
Acq On : 14 Feb 2022 20:34
Operator : CG/JU
Sample : N1524-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.404	2.19 ng	343783	Chrysene-d12	21.292

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	90
2			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	42
3			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	40
4			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	37
5			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	35

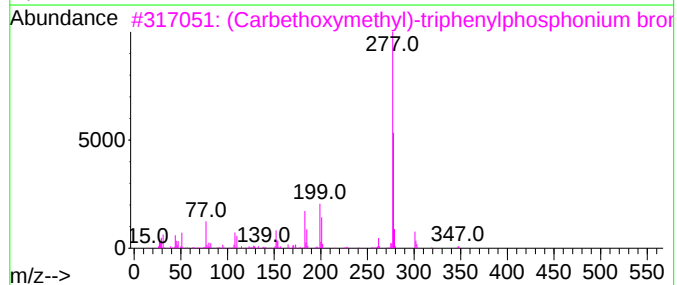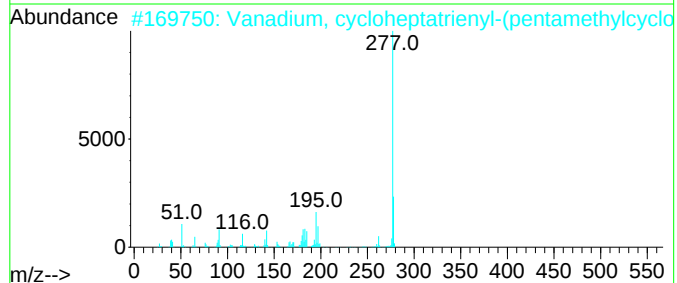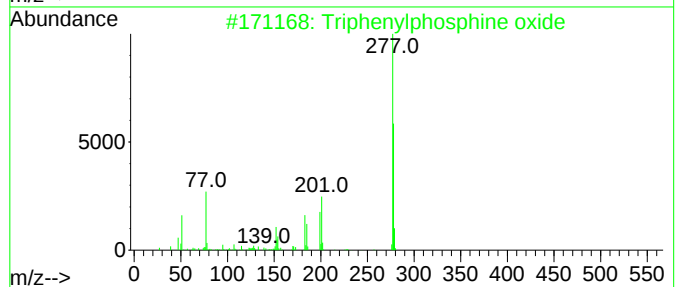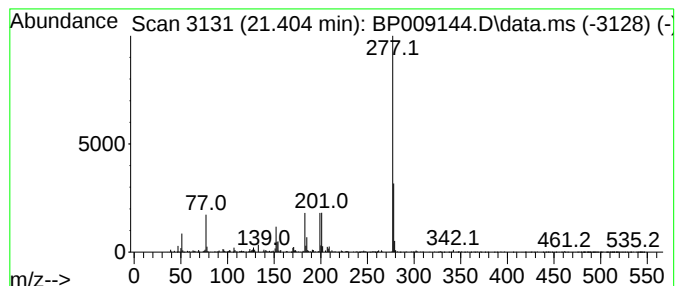

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
Data File : BP009144.D
Acq On : 14 Feb 2022 20:34
Operator : CG/JU
Sample : N1524-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
5-Eicosene, (E)-	20.992	2.5	ng	393333	5	21.292	3133260	20.0
Triphenylphosph...	21.404	2.2	ng	343783	5	21.292	3133260	20.0