
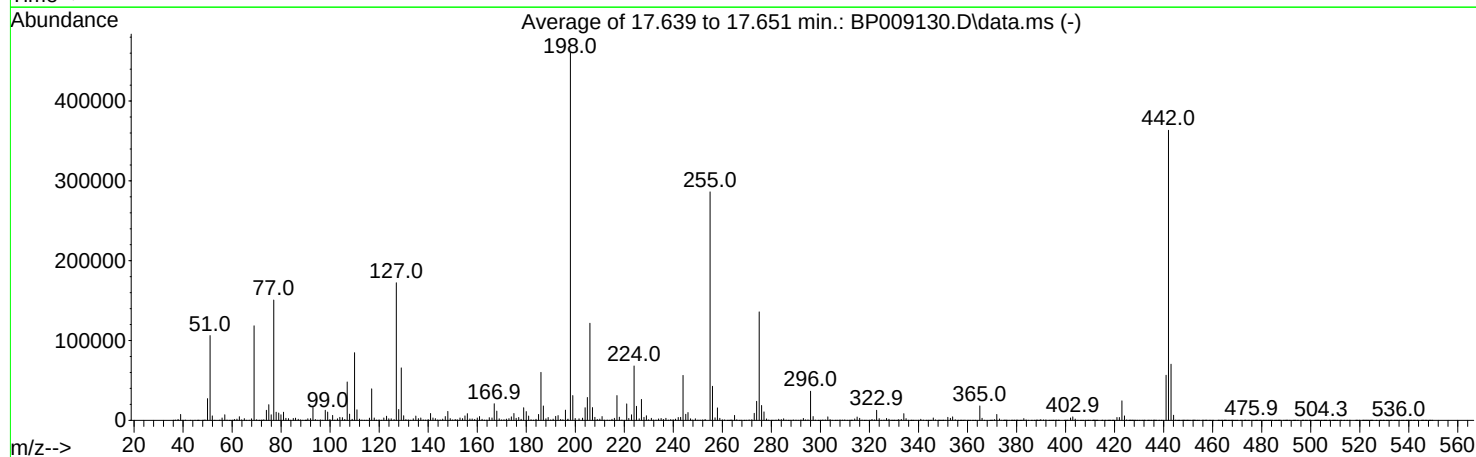


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
 Data File : BP009130.D
 Acq On : 14 Feb 2022 12:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 07 15:13:17 2022

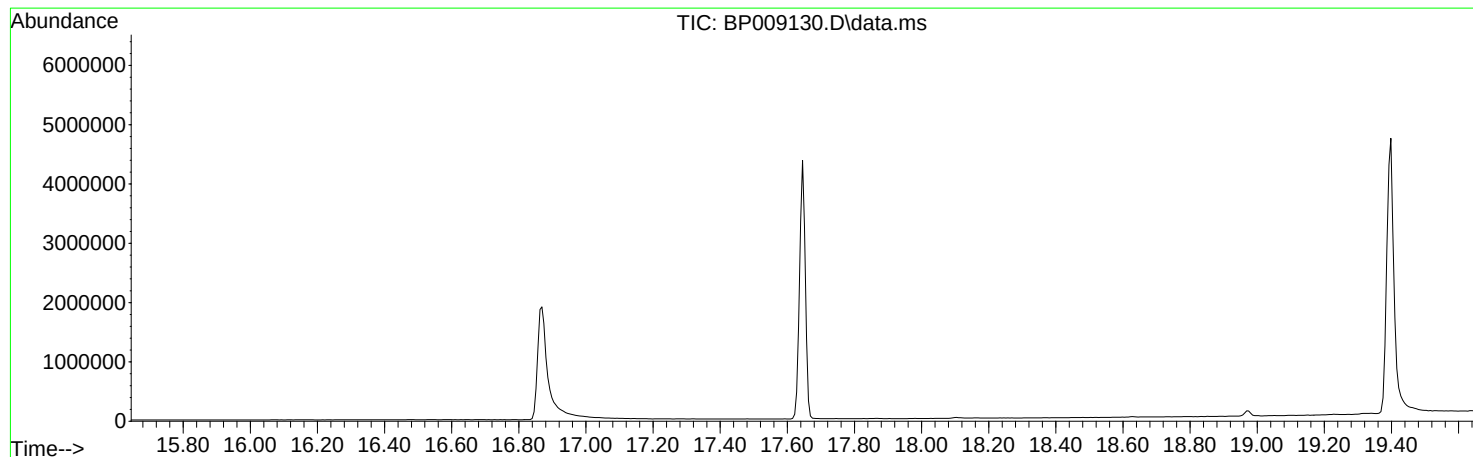




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.1	106223	PASS
68	69	0.00	2	1.6	1924	PASS
69	198	0.00	100	25.7	118504	PASS
70	69	0.00	2	0.6	727	PASS
127	198	10	80	37.4	172477	PASS
197	198	0.00	2	0.3	1577	PASS
198	198	100	100	100.0	460821	PASS
199	198	5	9	6.7	31072	PASS
275	198	10	60	29.5	135907	PASS
365	198	1	100	3.9	17978	PASS
441	198	0.01	100	12.3	56531	PASS
442	442	100	100	100.0	363435	PASS
443	442	15	24	19.4	70384	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
Data File : BP009130.D
Acq On : 14 Feb 2022 12:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 14 13:49:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 15:13:17 2022
Response via : Initial Calibration

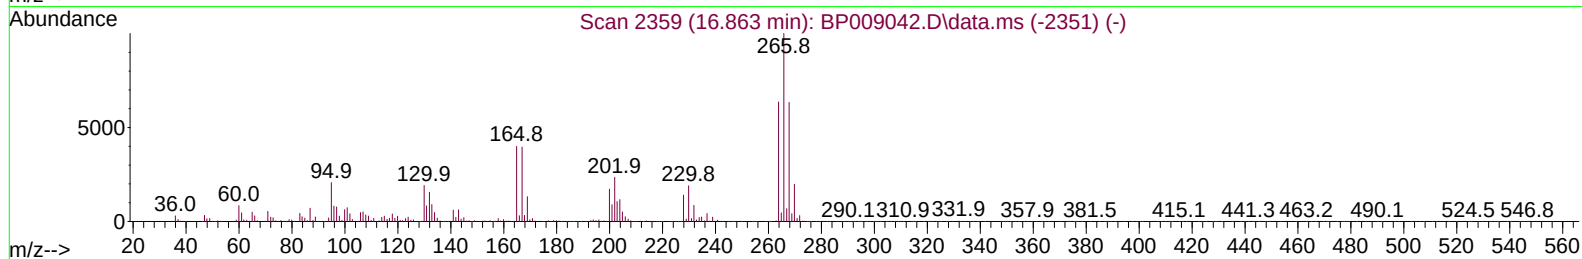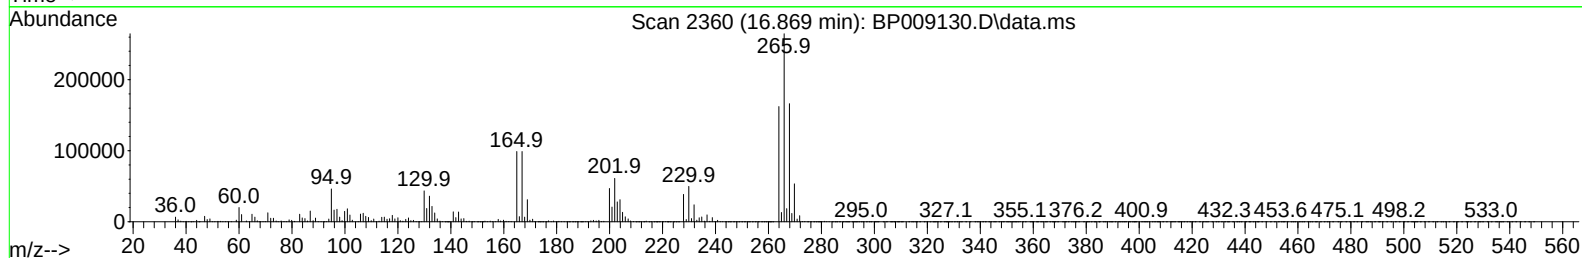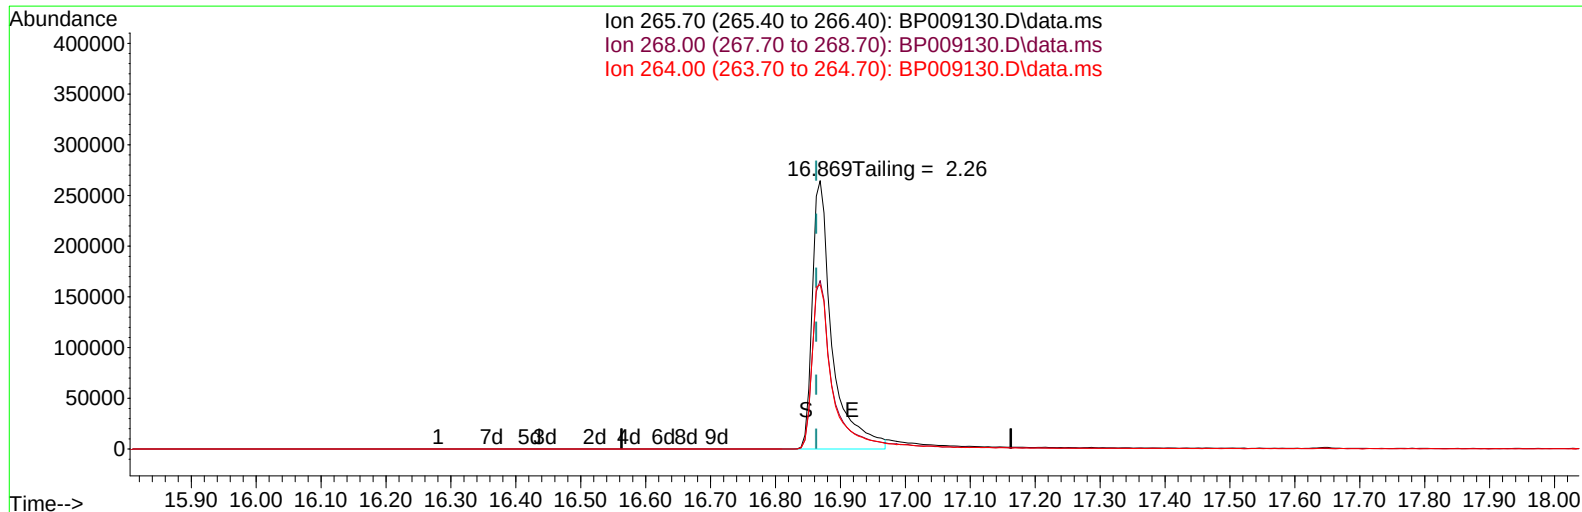

TIC: BP009130.D\data.ms

(70) Pentachlorophenol (C)

16.869min (+ 0.006) 731744.53 ng m




response 590165

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.78
264.00	62.90	61.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021422\
Data File : BP009130.D
Acq On : 14 Feb 2022 12:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 14 13:49:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 15:13:17 2022
Response via : Initial Calibration

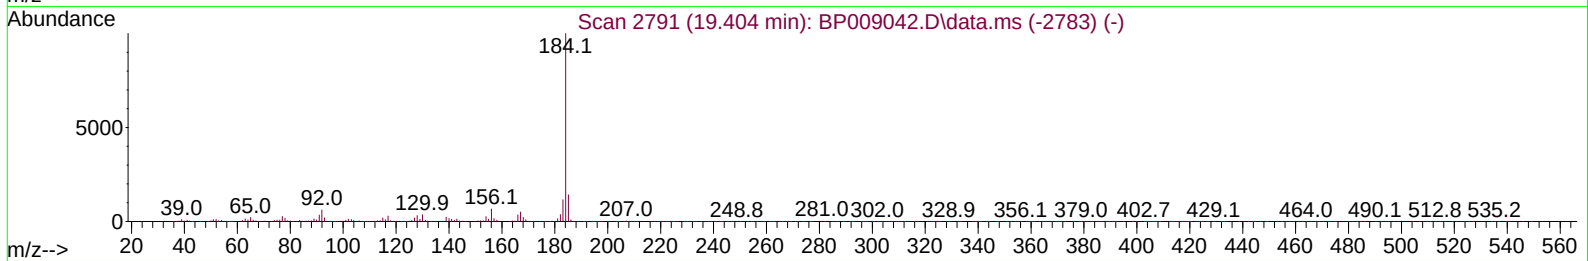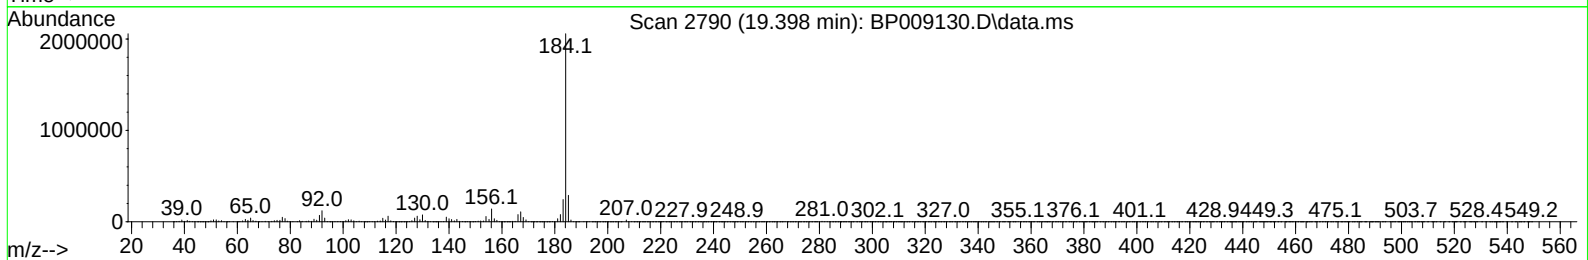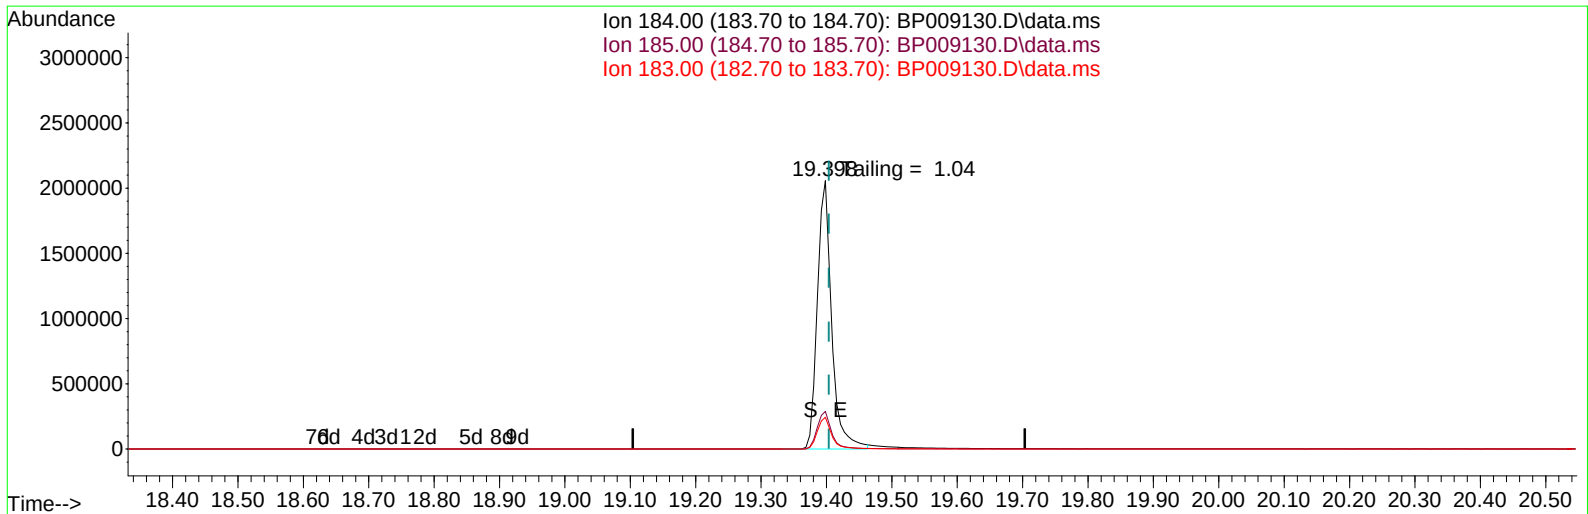

TIC: BP009130.D\data.ms

(77) Benzidine

19.398min (-0.006) 6702.21 ng m

response 3191867

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.03
183.00	11.90	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/14/2022	BNA_P	<u>BP009130.D</u>
Compound Name	Response	Retention Time
DDT	1588301	20.59
DDD	11862	20.17
DDE	3242	19.67
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15104	1603405	0.94

Instrument :
BNA_P
ClientSampleId :
DFTPP