

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021423\
 Data File : BP013814.D
 Acq On : 14 Feb 2023 10:03
 Operator : CG/JU
 Sample : PB150821BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK821

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.464	43	47	61	rVB	57725	77798	1.47%	0.154%
2	3.899	117	121	143	rBV	642294	1007771	19.09%	1.989%
3	4.234	173	178	186	rVB	12824	18623	0.35%	0.037%
4	4.717	254	260	266	rBV	2553	7286	0.14%	0.014%
5	7.264	684	693	713	rBV	734879	1225142	23.20%	2.418%
6	7.434	715	722	738	rVB	656883	1018036	19.28%	2.009%
7	7.640	748	757	772	rBV	791230	1272987	24.11%	2.512%
8	8.117	828	838	851	rBV	674630	1092255	20.69%	2.156%
9	8.816	946	957	979	rBV	927943	1577342	29.87%	3.113%
10	9.287	1028	1037	1056	rBV	705506	1161328	21.99%	2.292%
11	10.016	1153	1161	1171	rBV	591256	975943	18.48%	1.926%
12	10.558	1245	1253	1269	rBV	906625	1615615	30.60%	3.189%
13	10.940	1310	1318	1327	rBV	887973	1538520	29.14%	3.037%
14	11.075	1333	1341	1360	rBV	912484	1610394	30.50%	3.178%
15	12.522	1578	1587	1596	rBV2	15061	31608	0.60%	0.062%
16	13.634	1772	1776	1781	rBV7	3612	5674	0.11%	0.011%
17	14.151	1857	1864	1880	rBV	1905022	2693311	51.01%	5.316%
18	14.446	1905	1914	1928	rBV	2008156	2988811	56.61%	5.899%
19	14.751	1959	1966	1978	rBV	1462011	2160505	40.92%	4.264%
20	14.934	1990	1997	2019	rBV	720379	1095085	20.74%	2.161%
21	15.157	2033	2035	2041	rVB7	3808	5987	0.11%	0.012%
22	15.746	2126	2135	2146	rBV	2631593	3877783	73.44%	7.653%
23	15.851	2147	2153	2169	rVV	826375	1162202	22.01%	2.294%
24	15.981	2171	2175	2185	rVB5	13304	25170	0.48%	0.050%
25	17.181	2375	2379	2383	rBV7	4252	6769	0.13%	0.013%
26	17.292	2394	2398	2404	rBV3	3787	6420	0.12%	0.013%
27	17.504	2427	2434	2444	rBV	1887881	2798779	53.01%	5.524%
28	17.604	2445	2451	2469	rVB	3099177	4440850	84.11%	8.765%
29	18.363	2577	2580	2584	rBV5	5230	7888	0.15%	0.016%
30	19.404	2753	2757	2762	rVB2	44754	55373	1.05%	0.109%
31	19.469	2765	2768	2775	rVB	39247	56681	1.07%	0.112%
32	19.828	2823	2829	2839	rBV	3867564	5280088	100.00%	10.421%
33	21.586	3122	3128	3138	rBV	2016450	2887504	54.69%	5.699%
34	23.980	3528	3535	3551	rVB	2135392	4367420	82.71%	8.620%
35	24.151	3557	3564	3576	rVB2	1152587	2514186	47.62%	4.962%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021423\
Data File : BP013814.D
Acq On : 14 Feb 2023 10:03
Operator : CG/JU
Sample : PB150821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK821

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Title : SVOA CALIBRATION




Sum of corrected areas: 50667134

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021423\
Data File : BP013814.D
Acq On : 14 Feb 2023 10:03
Operator : CG/JU
Sample : PB150821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

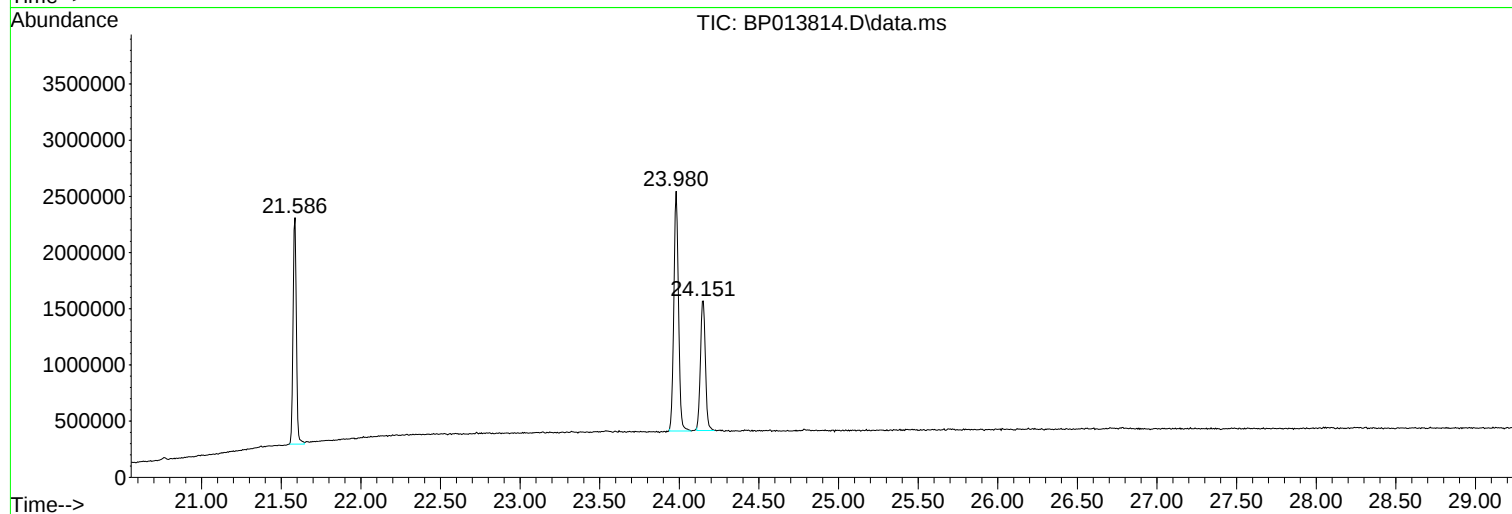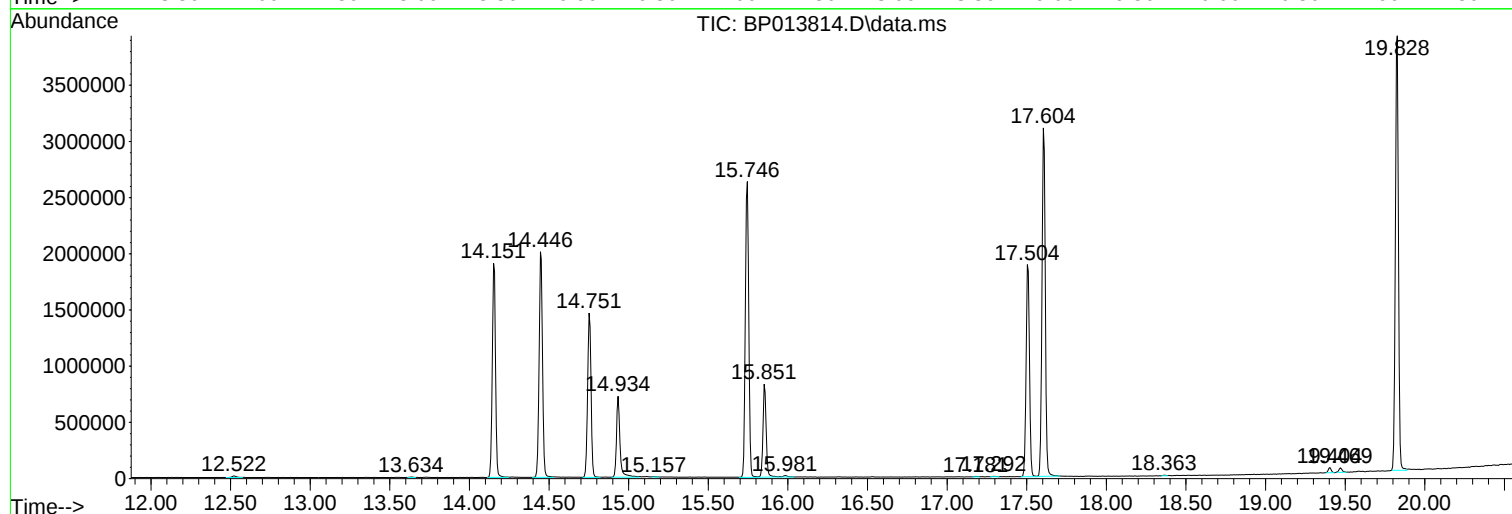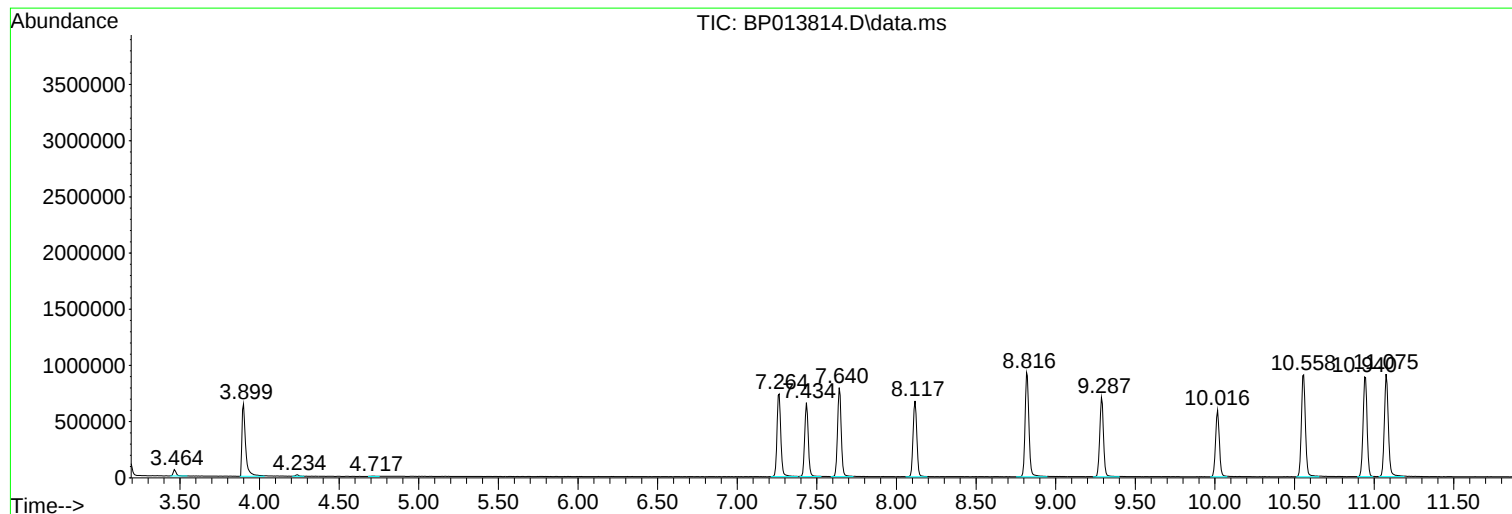

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021423\
Data File : BP013814.D
Acq On : 14 Feb 2023 10:03
Operator : CG/JU
Sample : PB150821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021423\
Data File : BP013814.D
Acq On : 14 Feb 2023 10:03
Operator : CG/JU
Sample : PB150821BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK821

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------