

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021423\
 Data File : BP013816.D
 Acq On : 14 Feb 2023 14:26
 Operator : CG/JU
 Sample : 01512-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	41	rVV7	5284	14828	0.32%	0.034%
2	3.470	44	48	57	rVB	44050	60402	1.30%	0.140%
3	3.911	120	123	141	rBV	115440	194364	4.18%	0.450%
4	4.140	157	162	167	rVB	18673	28086	0.60%	0.065%
5	4.240	174	179	185	rVB	19356	28461	0.61%	0.066%
6	4.346	192	197	205	rVB3	14183	21315	0.46%	0.049%
7	4.622	239	244	246	rBV6	3766	5052	0.11%	0.012%
8	5.193	331	341	348	rBV2	28874	53030	1.14%	0.123%
9	6.487	557	561	568	rVB	9947	15784	0.34%	0.037%
10	7.269	683	694	707	rBV	135739	241826	5.20%	0.560%
11	7.440	716	723	737	rBV	675770	1045019	22.46%	2.418%
12	7.652	752	759	770	rBV	583525	957120	20.57%	2.215%
13	8.122	832	839	853	rBV	715486	1165992	25.06%	2.698%
14	8.828	951	959	975	rBV	423848	703892	15.13%	1.629%
15	9.034	989	994	997	rVB3	5113	7672	0.16%	0.018%
16	9.299	1031	1039	1052	rBV	713157	1199092	25.77%	2.774%
17	9.393	1052	1055	1061	rVV7	4357	9015	0.19%	0.021%
18	9.452	1061	1065	1073	rVB6	8385	16205	0.35%	0.037%
19	9.693	1101	1106	1111	rVB2	8723	12380	0.27%	0.029%
20	10.022	1155	1162	1176	rBV	533370	890543	19.14%	2.060%
21	10.563	1245	1254	1274	rBV	860879	1456442	31.30%	3.370%
22	10.952	1308	1320	1330	rBV	952190	1597133	34.32%	3.695%
23	11.087	1335	1343	1355	rBV	594835	1081695	23.25%	2.503%
24	12.187	1525	1530	1538	rVB	27010	40747	0.88%	0.094%
25	12.463	1569	1577	1582	rBV9	4342	9144	0.20%	0.021%
26	12.528	1582	1588	1598	rVB	14121	29761	0.64%	0.069%
27	13.281	1710	1716	1720	rBV7	4116	7035	0.15%	0.016%
28	13.640	1773	1777	1784	rVB6	6538	9663	0.21%	0.022%
29	13.728	1790	1792	1798	rVB6	3034	4890	0.11%	0.011%
30	14.163	1856	1866	1878	rBV	1723977	2537510	54.53%	5.871%
31	14.457	1908	1916	1930	rBV	1919491	2940396	63.19%	6.803%
32	14.757	1960	1967	1978	rBV	1389640	2152361	46.25%	4.980%
33	14.945	1993	1999	2021	rBV2	45801	110360	2.37%	0.255%
34	15.163	2032	2036	2045	rVB2	5255	12130	0.26%	0.028%
35	15.428	2078	2081	2087	rBV6	3803	5623	0.12%	0.013%
36	15.751	2125	2136	2148	rBV	2608465	3790951	81.47%	8.771%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021423\
 Data File : BP013816.D
 Acq On : 14 Feb 2023 14:26
 Operator : CG/JU
 Sample : 01512-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

37	15.857	2148	2154	2167	rVV	545378	791706	17.01%	1.832%
38	15.992	2173	2177	2185	rVB2	14229	23806	0.51%	0.055%
39	16.316	2227	2232	2238	rBV10	3216	6077	0.13%	0.014%
40	16.534	2265	2269	2274	rBV7	3521	5819	0.13%	0.013%
41	17.192	2373	2381	2386	rBV10	4591	10569	0.23%	0.024%
42	17.516	2428	2436	2446	rBV	1758678	2585705	55.57%	5.983%
43	17.616	2446	2453	2470	rVV	2767287	4039090	86.80%	9.345%
44	18.369	2576	2581	2586	rBV4	19312	31040	0.67%	0.072%
45	19.410	2754	2758	2763	rBV3	35507	48205	1.04%	0.112%
46	19.475	2766	2769	2776	rVB	31498	45935	0.99%	0.106%
47	19.586	2786	2788	2793	rVB6	14116	15754	0.34%	0.036%
48	19.833	2824	2830	2839	rBV	3389583	4653350	100.00%	10.767%
49	21.592	3123	3129	3137	rBV2	1785667	2565459	55.13%	5.936%
50	23.992	3529	3537	3552	rBV	1793796	3712489	79.78%	8.590%
51	24.157	3559	3565	3577	rVB2	1042758	2229373	47.91%	5.158%




Sum of corrected areas: 43220296

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021423\
Data File : BP013816.D
Acq On : 14 Feb 2023 14:26
Operator : CG/JU
Sample : 01512-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

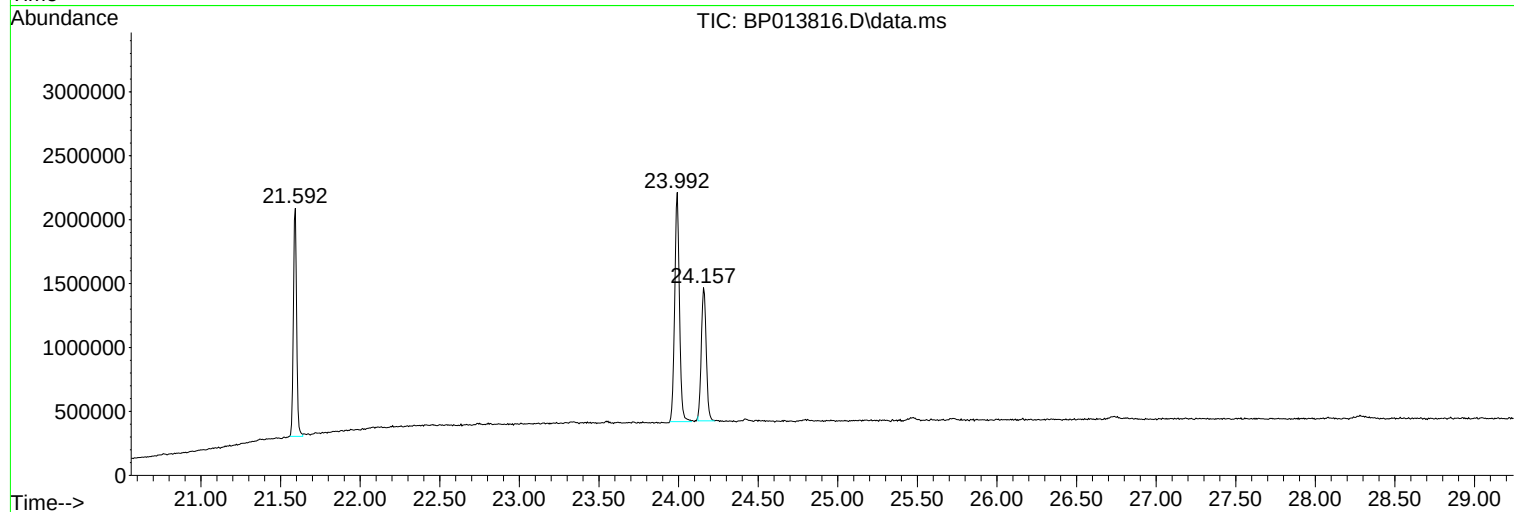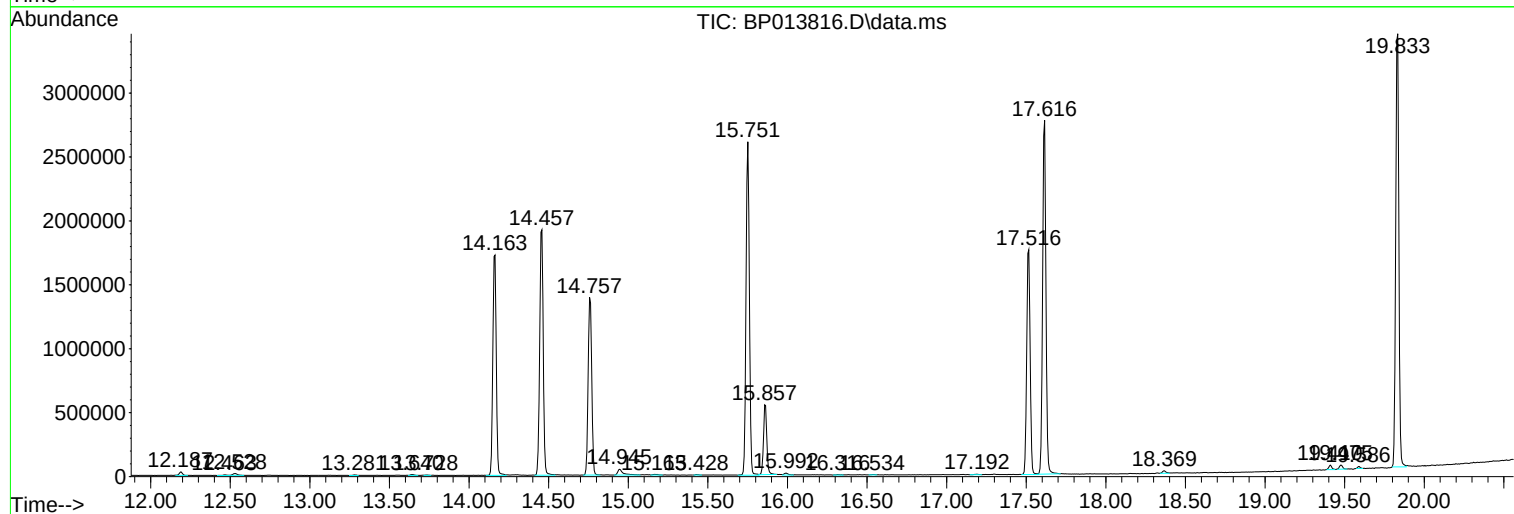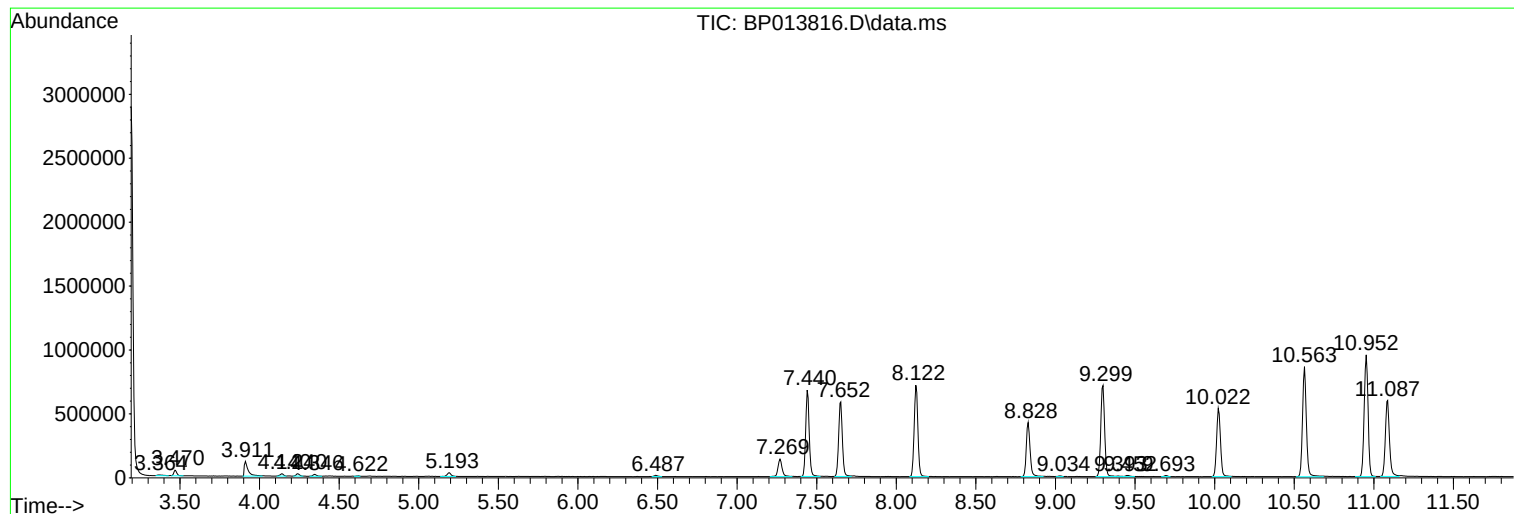

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021423\
Data File : BP013816.D
Acq On : 14 Feb 2023 14:26
Operator : CG/JU
Sample : 01512-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021423\
Data File : BP013816.D
Acq On : 14 Feb 2023 14:26
Operator : CG/JU
Sample : 01512-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc