
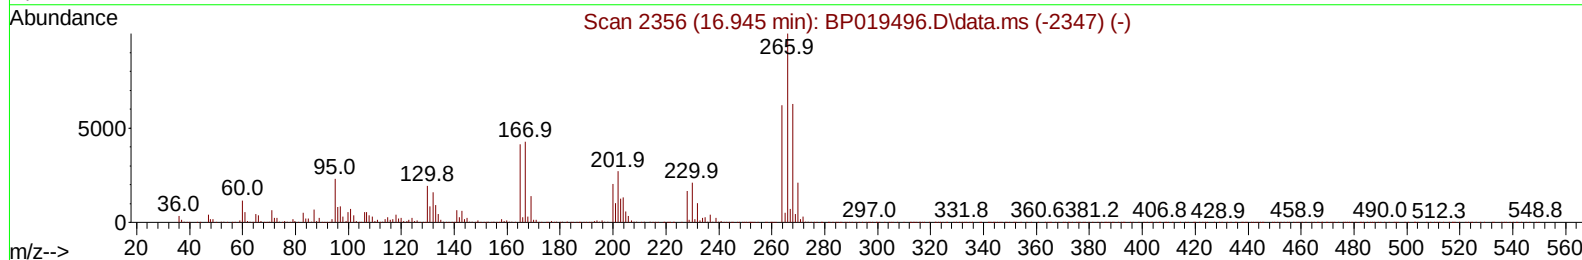
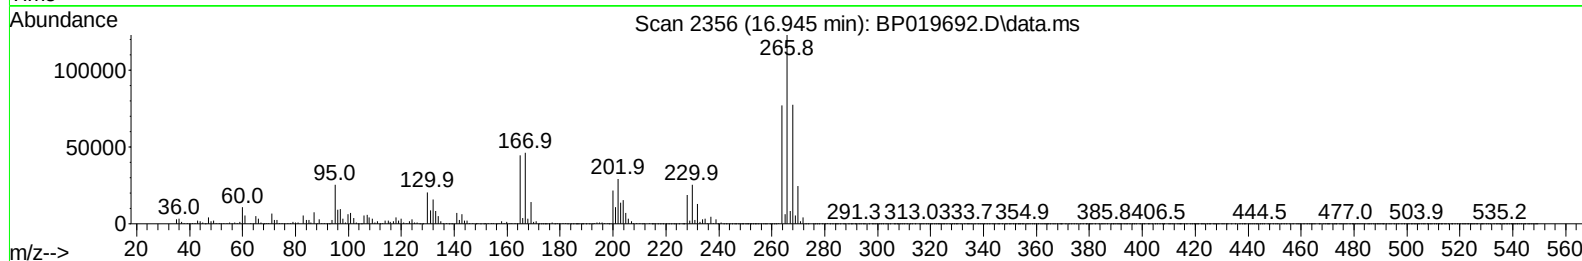


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021424\
Data File : BP019692.D
Acq On : 14 Feb 2024 09:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 00:54:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

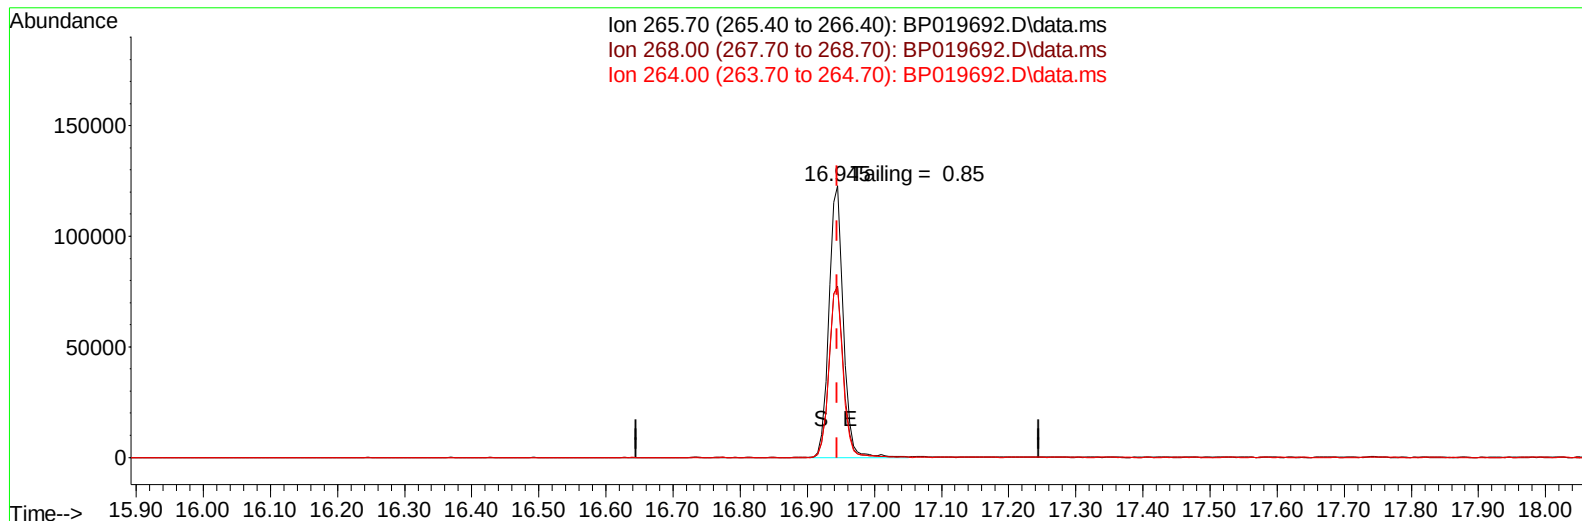

TIC: BP019692.D\data.ms

(70) Pentachlorophenol (C)




16.945min (+ 0.000) 84015.95 ng

response 184077

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.07
264.00	62.10	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021424\
Data File : BP019692.D
Acq On : 14 Feb 2024 09:44
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 00:54:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

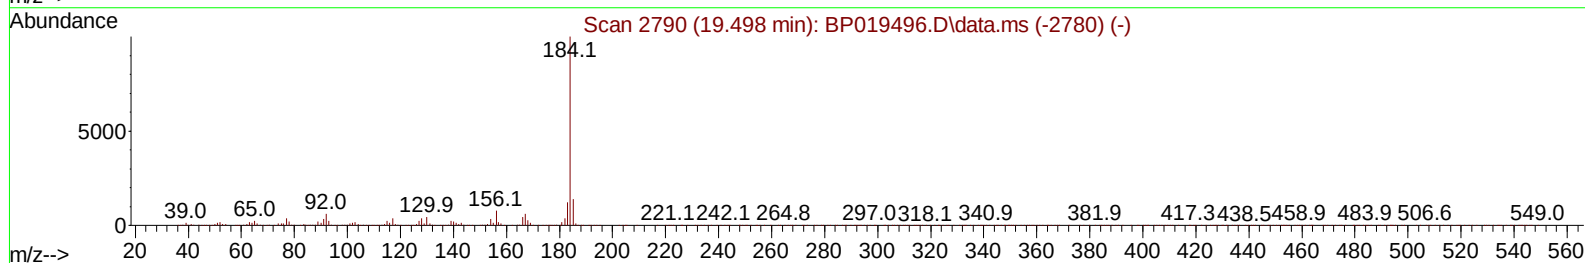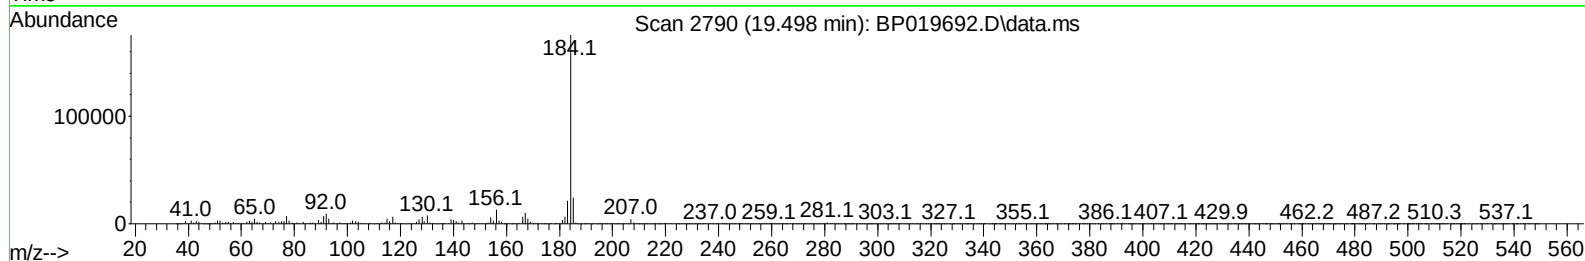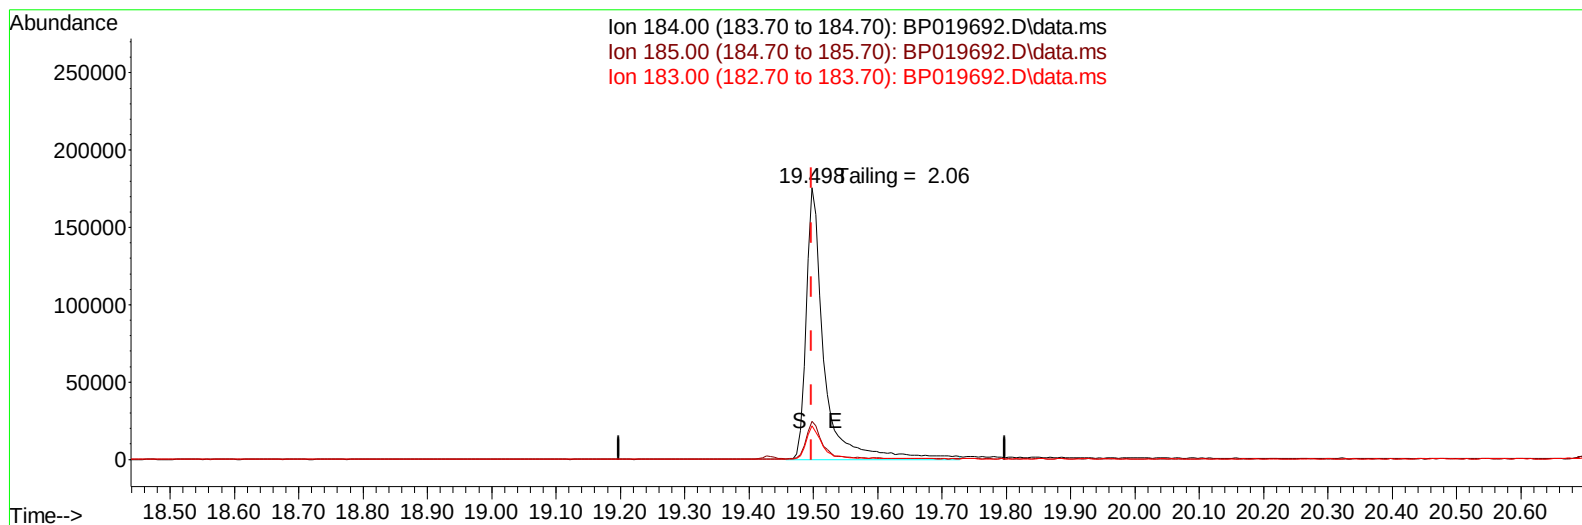

TIC: BP019692.D\data.ms

(77) Benzidine**19.498min (+ 0.000) 10382.98 ng****response 333425**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.04
183.00	12.10	12.37
0.00	0.00	0.00