


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021424\
Data File : BP019692.D
Acq On : 14 Feb 2024 09:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

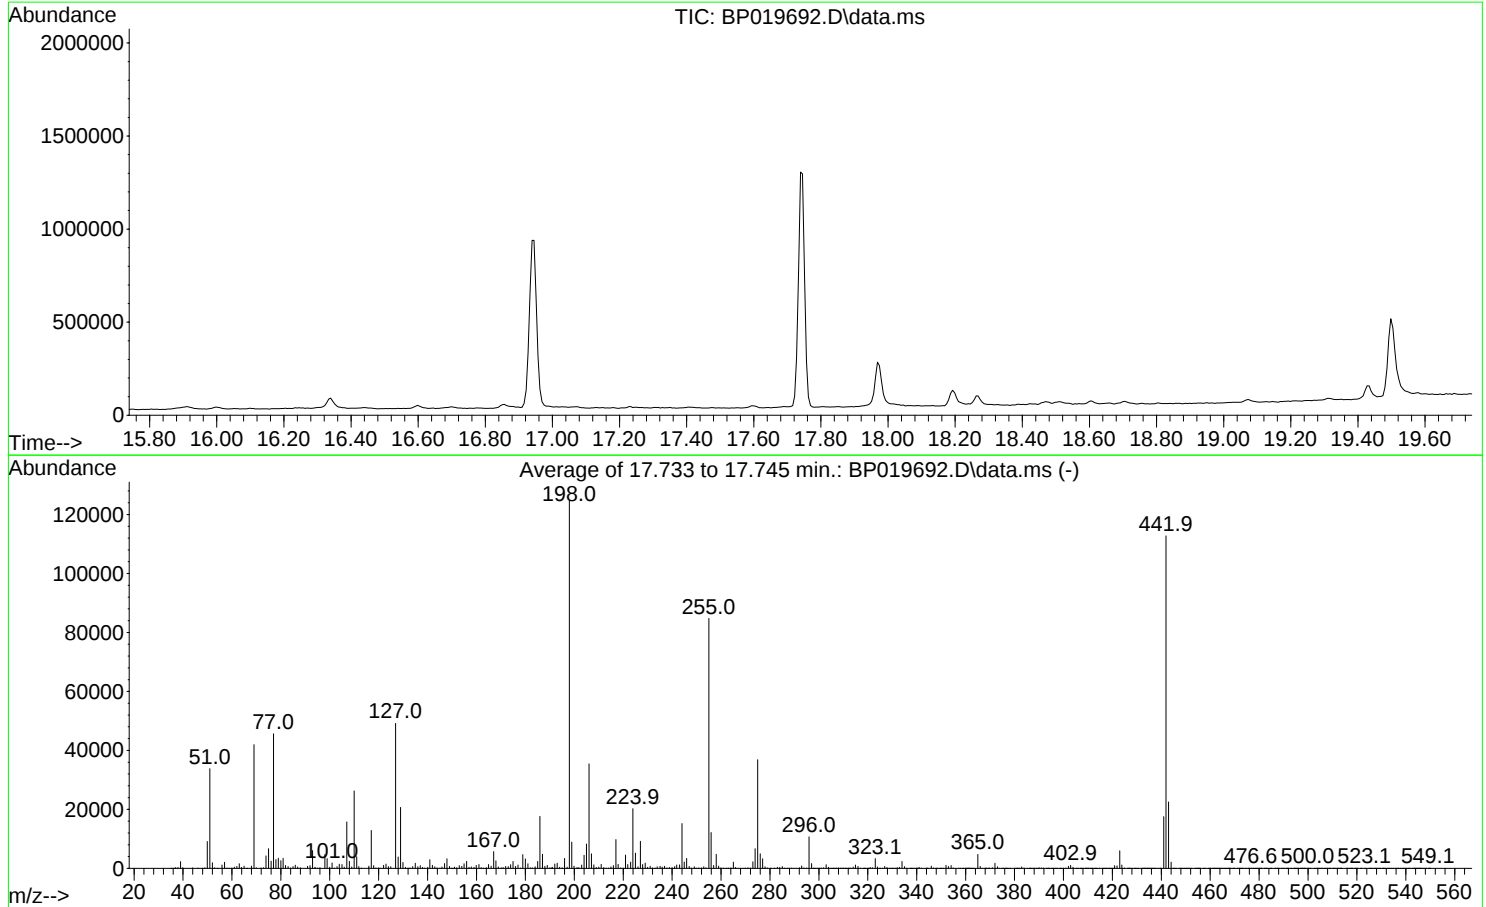




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	27.1	33799	PASS
68	69	0.00	2	1.8	737	PASS
69	198	0.00	100	33.6	41941	PASS
70	69	0.00	2	0.5	214	PASS
127	198	10	80	39.4	49184	PASS
197	198	0.00	2	0.4	444	PASS
198	198	100	100	100.0	124757	PASS
199	198	5	9	7.1	8887	PASS
275	198	10	60	29.5	36854	PASS
365	198	1	100	3.8	4737	PASS
441	198	0.01	100	14.1	17555	PASS
442	442	100	100	100.0	112767	PASS
443	442	15	24	20.0	22550	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021424\
Data File : BP019692.D
Acq On : 14 Feb 2024 09:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 15 00:54:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

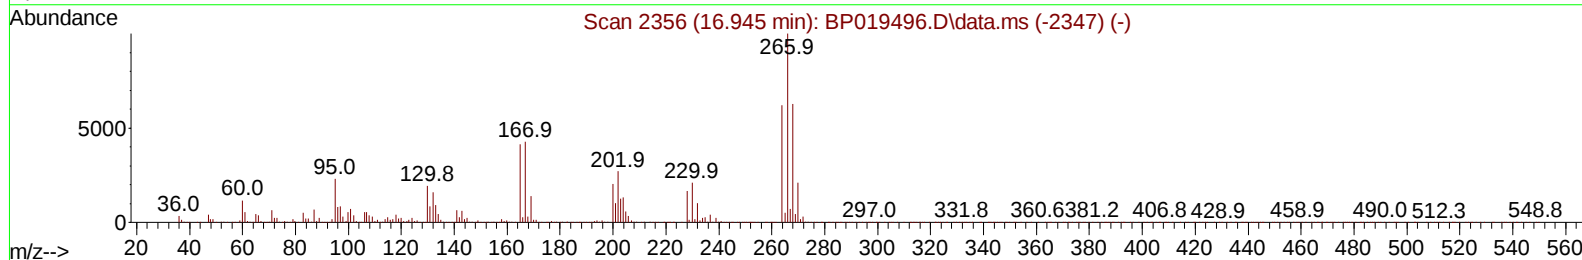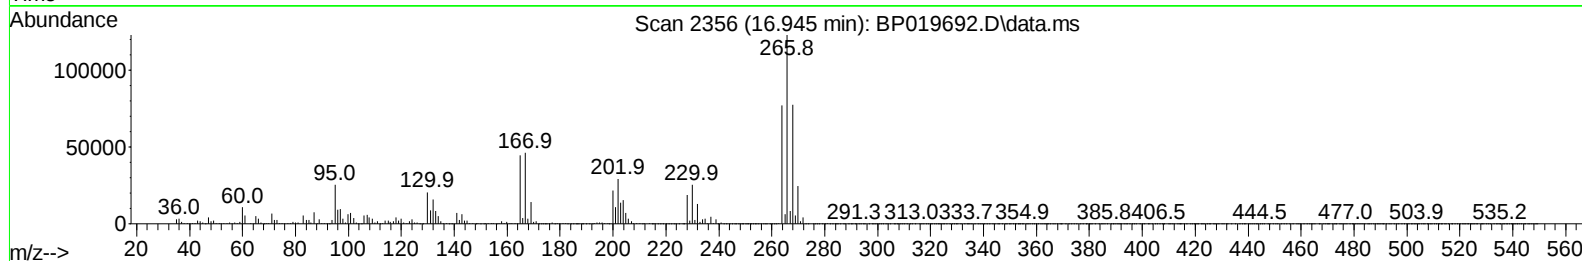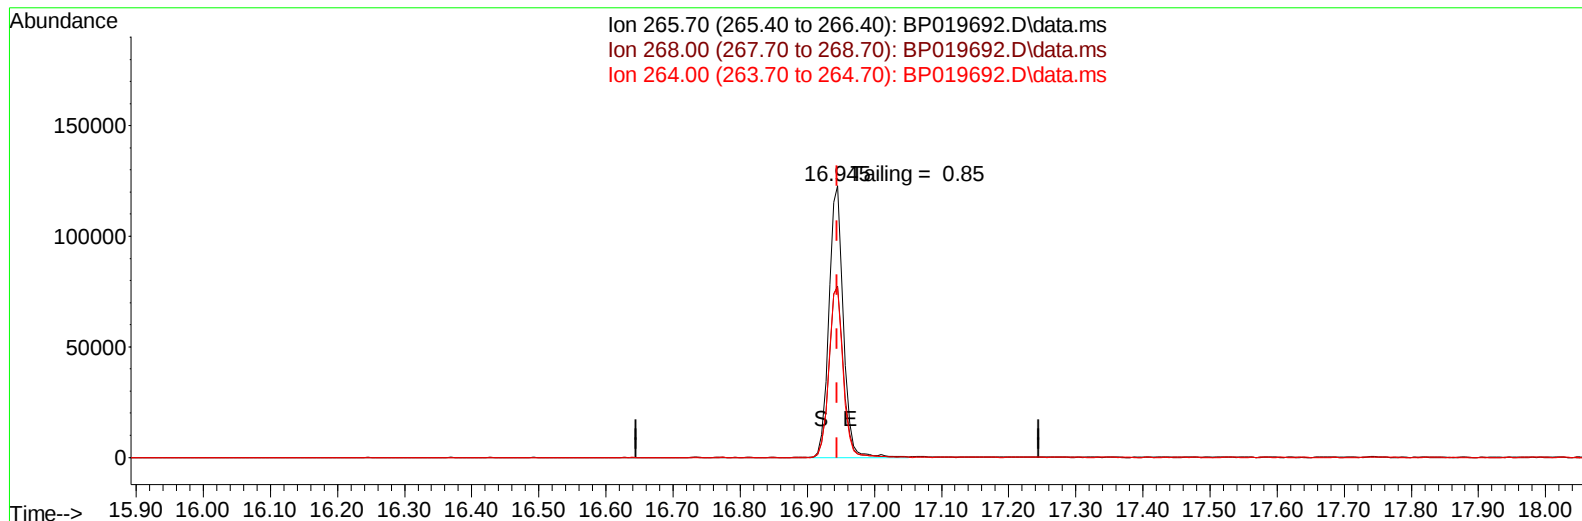

TIC: BP019692.D\data.ms

(70) Pentachlorophenol (C)

16.945min (+ 0.000) 84015.95 ng




response 184077

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.07
264.00	62.10	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021424\
Data File : BP019692.D
Acq On : 14 Feb 2024 09:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 15 00:54:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

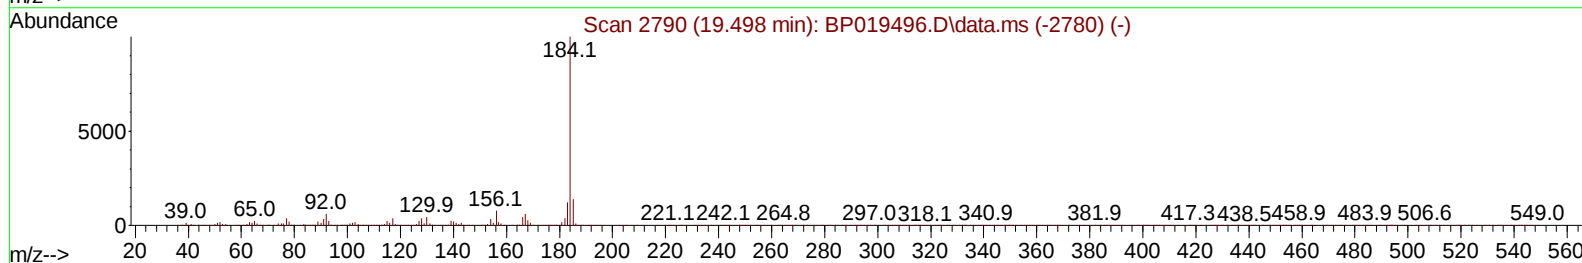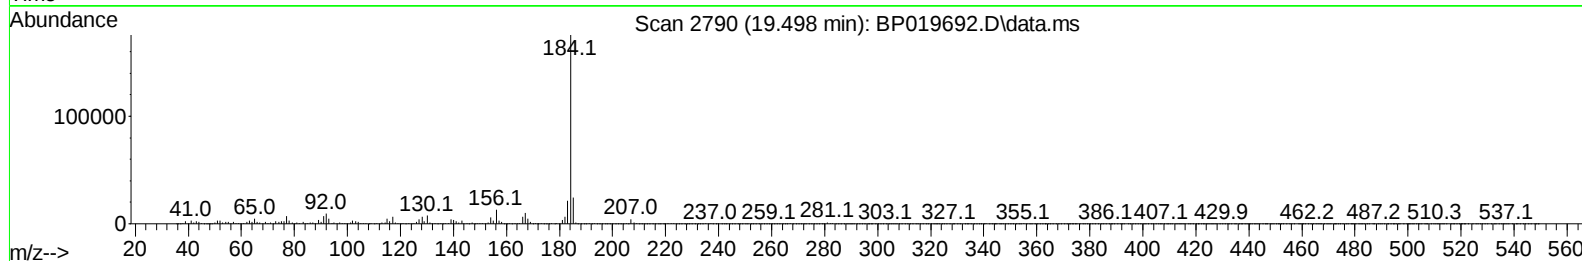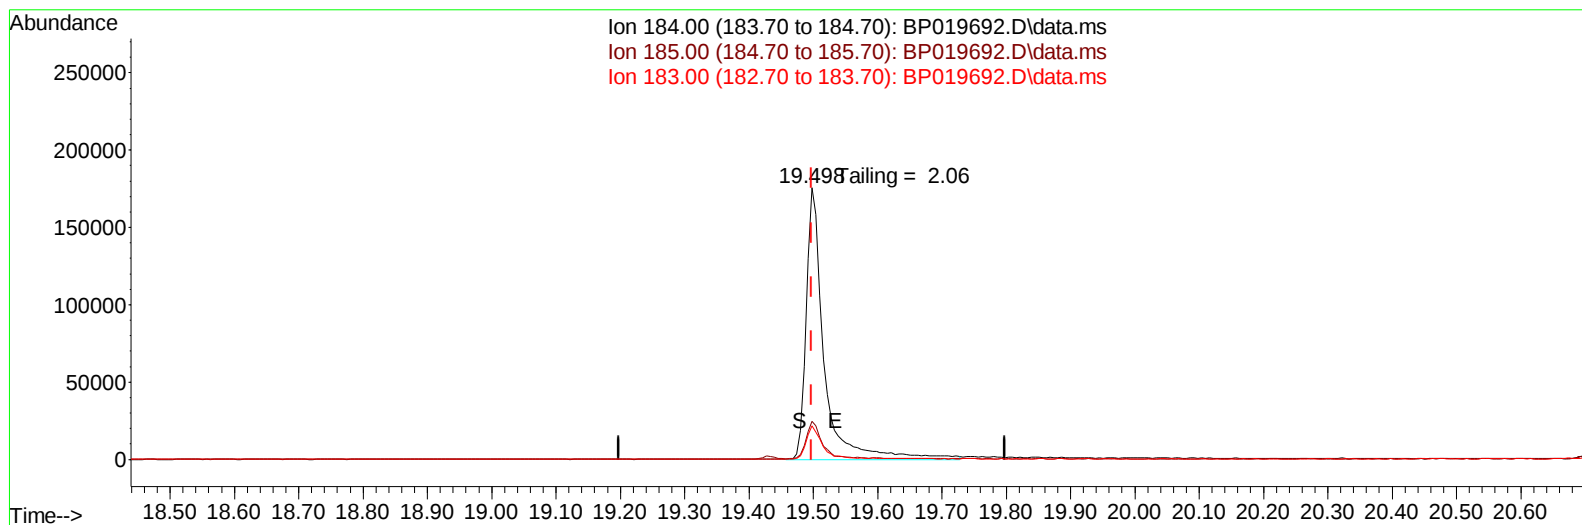

TIC: BP019692.D\data.ms

(77) Benzidine

19.498min (+ 0.000) 10382.98 ng

response 333425

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.04
183.00	12.10	12.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/14/2024	BNA_P	<u>BP019692.D</u>
Compound Name	Response	Retention Time
DDT	464597	20.698
DDD	12902	20.269
DDE	2018	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14920	479517	3.11

Instrument :
BNA_P
ClientSampleId :
DFTPP