

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021425\
 Data File : BP024064.D
 Acq On : 14 Feb 2025 16:45
 Operator : RC/JU
 Sample : Q1275-05DL2 1000X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZT2DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP024064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.017	155	158	164	rVB	16784	23059	0.24%	0.065%
2	6.922	647	652	661	rBV8	8179	19235	0.20%	0.054%
3	7.099	675	682	687	rBV	15210	26073	0.27%	0.074%
4	7.199	694	699	704	rVB2	22378	35390	0.37%	0.100%
5	7.305	710	717	724	rBV3	14246	26656	0.28%	0.075%
6	7.758	787	794	801	rBV	1273400	2002546	20.73%	5.670%
7	7.822	801	805	820	rVB	55407	102538	1.06%	0.290%
8	7.975	826	831	840	rBV	16835	25029	0.26%	0.071%
9	8.187	860	867	872	rBV	31867	54698	0.57%	0.155%
10	8.234	872	875	881	rVB3	11782	17355	0.18%	0.049%
11	8.469	910	915	921	rBV4	7462	14818	0.15%	0.042%
12	8.746	957	962	971	rVB4	7495	13000	0.13%	0.037%
13	8.905	985	989	996	rVB	14315	25113	0.26%	0.071%
14	9.028	1003	1010	1017	rBV6	9416	21332	0.22%	0.060%
15	9.334	1056	1062	1069	rVB6	13899	24367	0.25%	0.069%
16	9.610	1102	1109	1119	rVV7	12685	29165	0.30%	0.083%
17	9.781	1133	1138	1148	rBV7	4731	12672	0.13%	0.036%
18	10.169	1199	1204	1212	rBV6	10611	23002	0.24%	0.065%
19	10.534	1257	1266	1280	rVV	1920378	3169887	32.81%	8.975%
20	10.669	1280	1289	1301	rVB5	30130	75583	0.78%	0.214%
21	10.910	1325	1330	1337	rVB7	8026	13214	0.14%	0.037%
22	11.481	1422	1427	1431	rVB5	7878	11752	0.12%	0.033%
23	11.793	1477	1480	1489	rVB7	11637	20999	0.22%	0.059%
24	11.987	1509	1513	1520	rVB9	6543	10602	0.11%	0.030%
25	12.075	1523	1528	1533	rVV7	7607	13990	0.14%	0.040%
26	12.351	1570	1575	1582	rBV9	7275	15782	0.16%	0.045%
27	12.981	1677	1682	1686	rBV7	6098	10808	0.11%	0.031%
28	13.310	1730	1738	1745	rBV5	11090	26342	0.27%	0.075%
29	13.781	1813	1818	1826	rBV	33765	56828	0.59%	0.161%
30	14.063	1860	1866	1872	rBV	44286	61327	0.63%	0.174%
31	14.369	1911	1918	1938	rBV	2609150	4143240	42.88%	11.731%
32	14.675	1964	1970	1977	rVB	5127	12438	0.13%	0.035%
33	14.928	2007	2013	2017	rBV5	18486	30155	0.31%	0.085%
34	15.004	2017	2026	2048	rBV	1415734	1936532	20.04%	5.483%
35	15.369	2084	2088	2099	rVB	62363	99174	1.03%	0.281%
36	15.487	2104	2108	2112	rBV7	8786	14999	0.16%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021425\
Data File : BP024064.D
Acq On : 14 Feb 2025 16:45
Operator : RC/JU
Sample : Q1275-05DL2 1000X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZT2DL2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	16.639	2300	2304	2307	rBV6	7573	9830	0.10%	0.028%
38	16.810	2326	2333	2351	rBV	5991482	9662235	100.00%	27.358%
39	17.163	2387	2393	2405	rBV	3518467	4742361	49.08%	13.428%
40	17.263	2405	2410	2422	rVB2	65185	128904	1.33%	0.365%
41	17.534	2452	2456	2463	rBV	25015	37176	0.38%	0.105%
42	19.633	2809	2813	2821	rBV2	76377	129037	1.34%	0.365%
43	21.598	3141	3147	3159	rBV2	2550628	4390634	45.44%	12.432%
44	24.945	3708	3716	3736	rVB	1397405	3997504	41.37%	11.319%




Sum of corrected areas: 35317381

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021425\
Data File : BP024064.D
Acq On : 14 Feb 2025 16:45
Operator : RC/JU
Sample : Q1275-05DL2 1000X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZT2DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

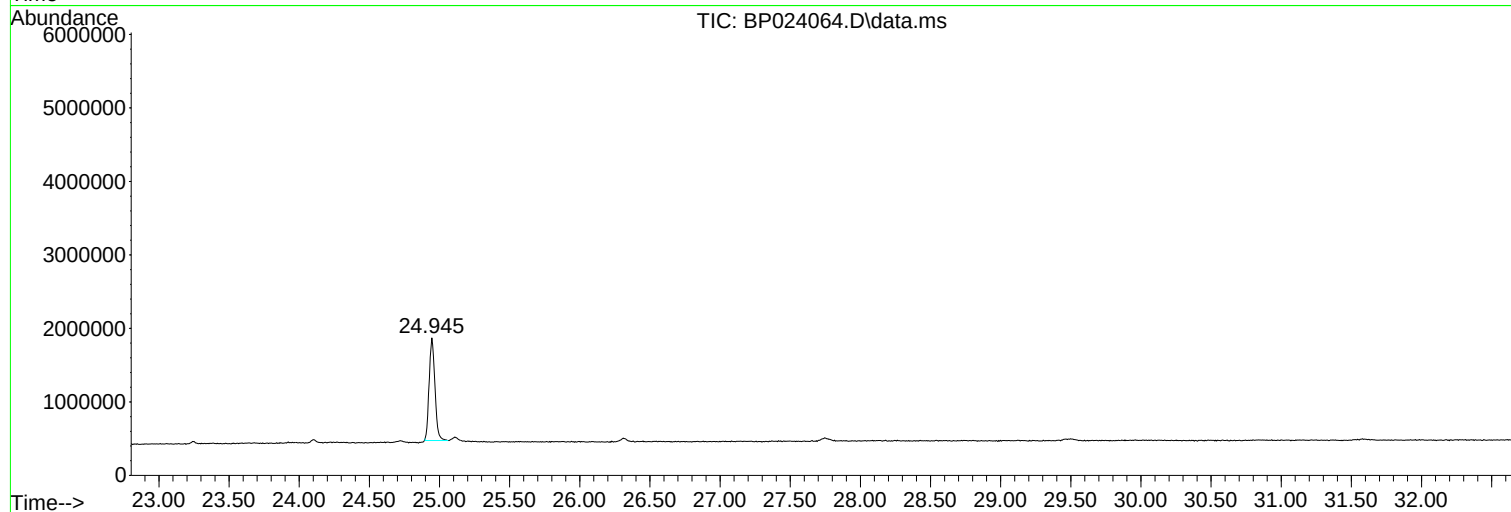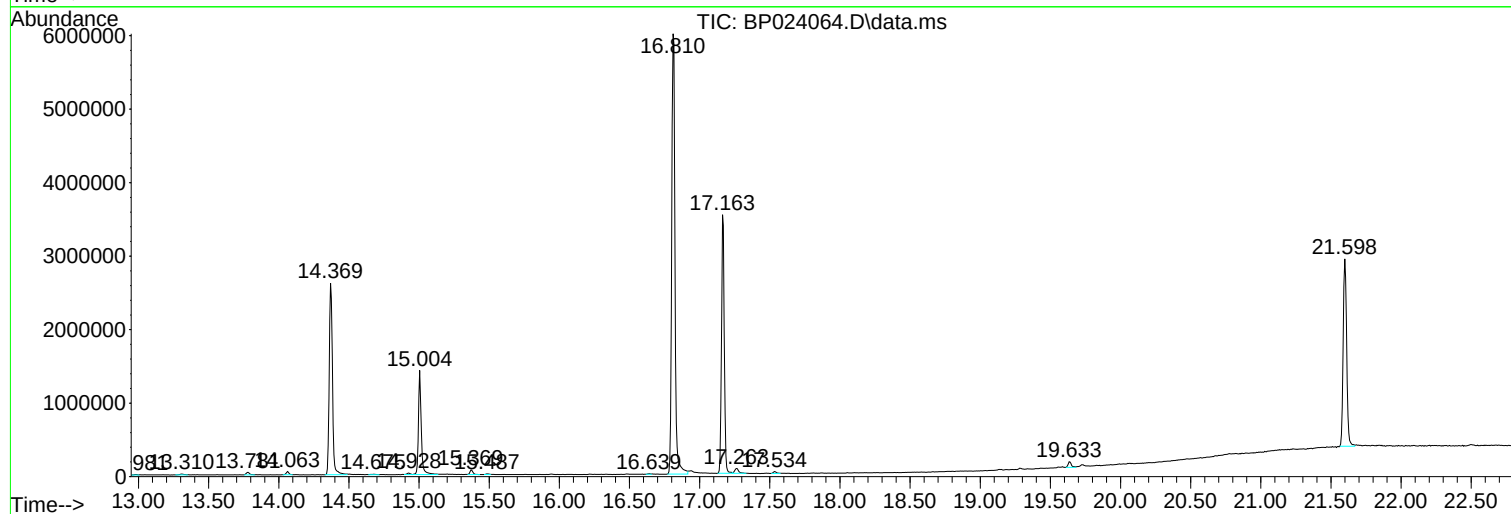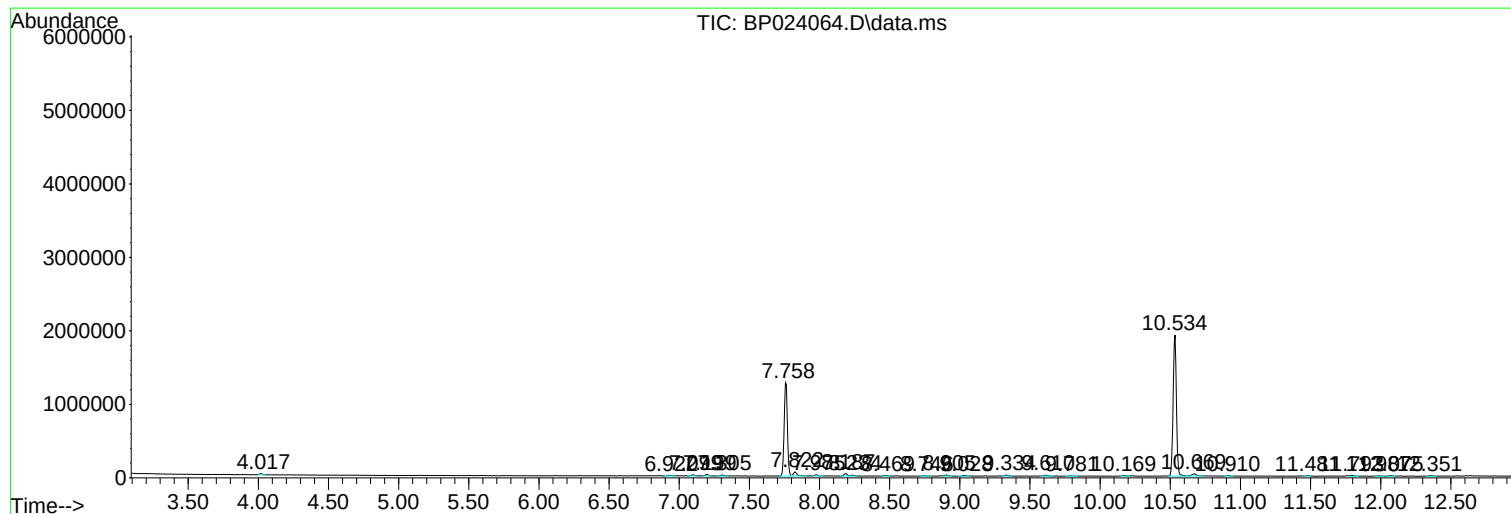

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021425\
Data File : BP024064.D
Acq On : 14 Feb 2025 16:45
Operator : RC/JU
Sample : Q1275-05DL2 1000X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZT2DL2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Phenol, 2,3,4,6--tetrachloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.004	9.35 ng/ul	1936530	Acenaphthene-d10	14.369

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenol, 2,3,4,6-tetrachloro-	230	C6H2Cl4O	000058-90-2	99
2			Phenol, 2,3,4,6-tetrachloro-	230	C6H2Cl4O	000058-90-2	99
3			Phenol, 2,3,4,6-tetrachloro-	230	C6H2Cl4O	000058-90-2	99
4			Phenol, 2,3,4,5-tetrachloro-	230	C6H2Cl4O	004901-51-3	98
5			Phenol, 2,3,5,6-tetrachloro-	230	C6H2Cl4O	000935-95-5	98

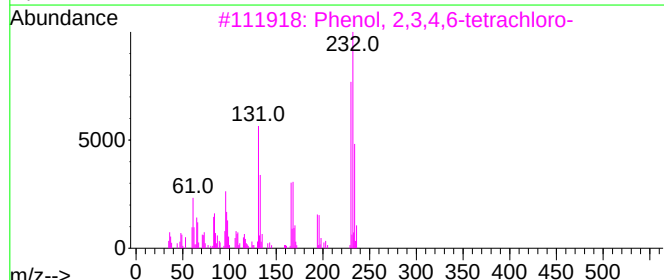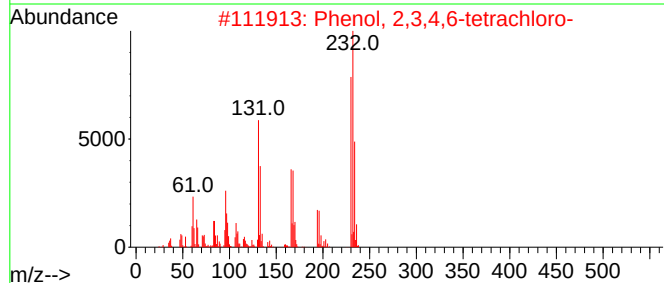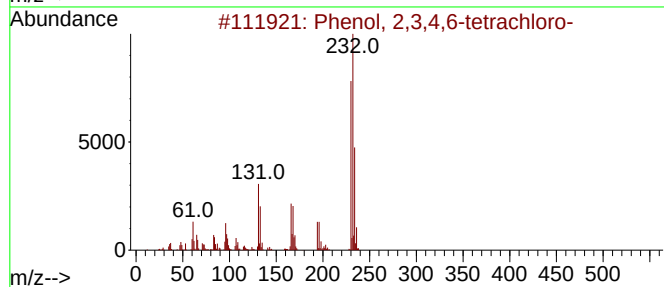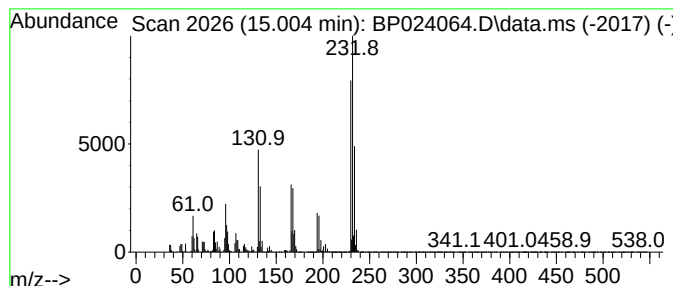

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021425\
Data File : BP024064.D
Acq On : 14 Feb 2025 16:45
Operator : RC/JU
Sample : Q1275-05DL2 1000X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZT2DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phenol, 2,3,4,6...	15.004	9.3	ng/ul	1936530	3	14.369	4143240	20.0