

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021425\
 Data File : BP024066.D
 Acq On : 14 Feb 2025 18:06
 Operator : RC/JU
 Sample : Q1275-01DL2 500X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCZT0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP024066.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.893	134	137	146	rVB5	12532	21094	0.17%	0.058%
2	4.017	155	158	161	rVB	15838	15503	0.13%	0.042%
3	5.581	420	424	430	rVB2	8143	13888	0.11%	0.038%
4	6.946	648	656	659	rBV4	8213	14729	0.12%	0.040%
5	7.099	677	682	694	rBV	29038	52539	0.42%	0.143%
6	7.305	709	717	723	rBV2	26828	48630	0.39%	0.133%
7	7.757	786	794	801	rBV	1225531	1846766	14.93%	5.035%
8	7.822	801	805	816	rVB	85092	143453	1.16%	0.391%
9	7.975	826	831	839	rVB	14958	23498	0.19%	0.064%
10	8.469	906	915	923	rBV	19760	42122	0.34%	0.115%
11	8.904	983	989	996	rBV	28069	47871	0.39%	0.131%
12	9.034	1000	1011	1025	rBV	53012	111815	0.90%	0.305%
13	9.281	1047	1053	1057	rBV6	8612	15483	0.13%	0.042%
14	9.622	1104	1111	1118	rBV4	16074	34926	0.28%	0.095%
15	10.169	1198	1204	1212	rBV2	24158	52057	0.42%	0.142%
16	10.528	1258	1265	1281	rBV	1654696	2793264	22.59%	7.616%
17	10.675	1282	1290	1301	rVB	28964	68427	0.55%	0.187%
18	10.910	1324	1330	1338	rVB	35075	58912	0.48%	0.161%
19	11.793	1476	1480	1487	rVB	36877	55181	0.45%	0.150%
20	11.993	1509	1514	1520	rVB	30546	43060	0.35%	0.117%
21	12.140	1535	1539	1545	rVB5	15371	23968	0.19%	0.065%
22	12.222	1545	1553	1560	rBV10	9243	17399	0.14%	0.047%
23	12.610	1614	1619	1620	rBV4	17998	24792	0.20%	0.068%
24	12.640	1620	1624	1628	rVB4	14647	28474	0.23%	0.078%
25	12.987	1677	1683	1687	rVB6	8896	14134	0.11%	0.039%
26	13.304	1730	1737	1743	rBV8	10377	22906	0.19%	0.062%
27	13.781	1813	1818	1829	rVV	71958	117441	0.95%	0.320%
28	14.069	1860	1867	1874	rBV2	79768	139063	1.12%	0.379%
29	14.381	1912	1920	1935	rBV	2344352	3806285	30.78%	10.378%
30	14.687	1965	1972	1978	rVV5	18607	38452	0.31%	0.105%
31	14.745	1979	1982	1988	rVB7	7485	13143	0.11%	0.036%
32	14.934	2007	2014	2018	rVB6	21039	34573	0.28%	0.094%
33	15.010	2018	2027	2044	rVV	815334	1342733	10.86%	3.661%
34	15.381	2083	2090	2097	rBV	123268	184502	1.49%	0.503%
35	15.492	2104	2109	2120	rVB4	28976	61913	0.50%	0.169%
36	15.745	2143	2152	2157	rBV4	4909	14265	0.12%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021425\
Data File : BP024066.D
Acq On : 14 Feb 2025 18:06
Operator : RC/JU
Sample : Q1275-01DL2 500X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZT0DL2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	16.075	2201	2208	2212	rBV10	6771	14921	0.12%	0.041%
38	16.222	2227	2233	2238	rVB8	11527	18234	0.15%	0.050%
39	16.481	2271	2277	2281	rBV	48590	70845	0.57%	0.193%
40	16.645	2300	2305	2312	rBV	8845	20599	0.17%	0.056%
41	16.810	2323	2333	2354	rBV	7635905	12367540	100.00%	33.719%
42	17.163	2385	2393	2405	rBV2	2742926	4348126	35.16%	11.855%
43	17.263	2405	2410	2428	rVB	126889	224869	1.82%	0.613%
44	17.528	2450	2455	2465	rVB	87134	142095	1.15%	0.387%
45	19.127	2722	2727	2733	rBV4	39675	59620	0.48%	0.163%
46	19.627	2808	2812	2819	rBV	126581	205798	1.66%	0.561%
47	21.592	3140	3146	3162	rBV2	2326560	4123828	33.34%	11.243%
48	24.945	3707	3716	3734	rVB2	1160534	3694452	29.87%	10.073%




Sum of corrected areas: 36678188

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021425\
Data File : BP024066.D
Acq On : 14 Feb 2025 18:06
Operator : RC/JU
Sample : Q1275-01DL2 500X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZT0DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

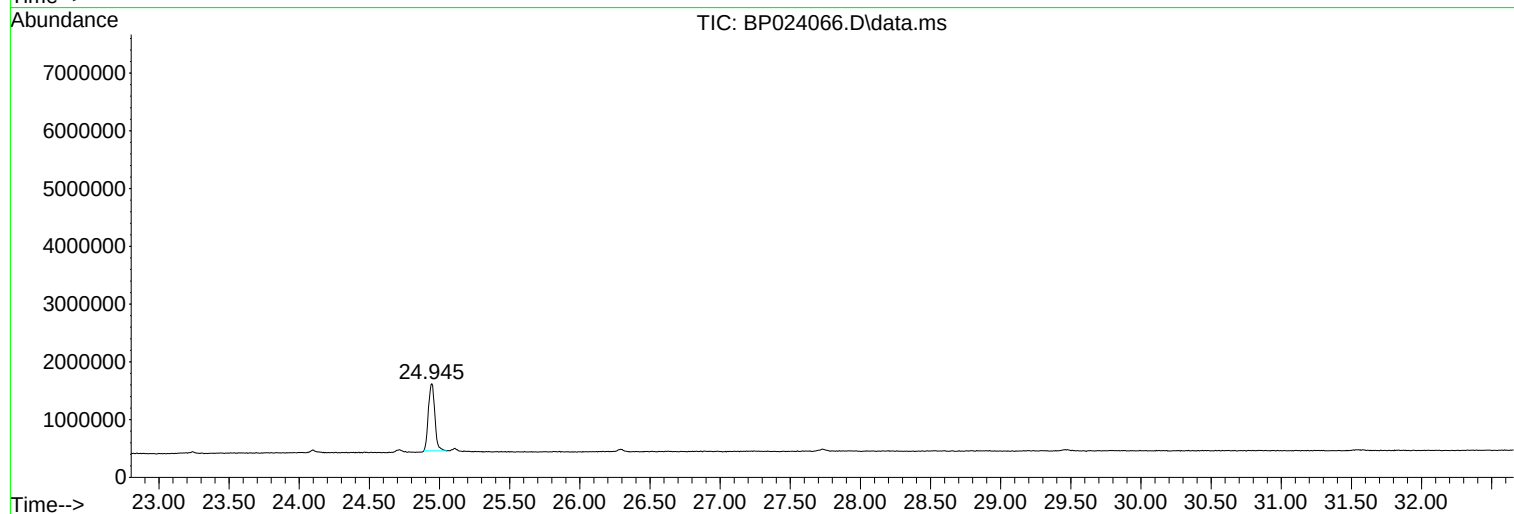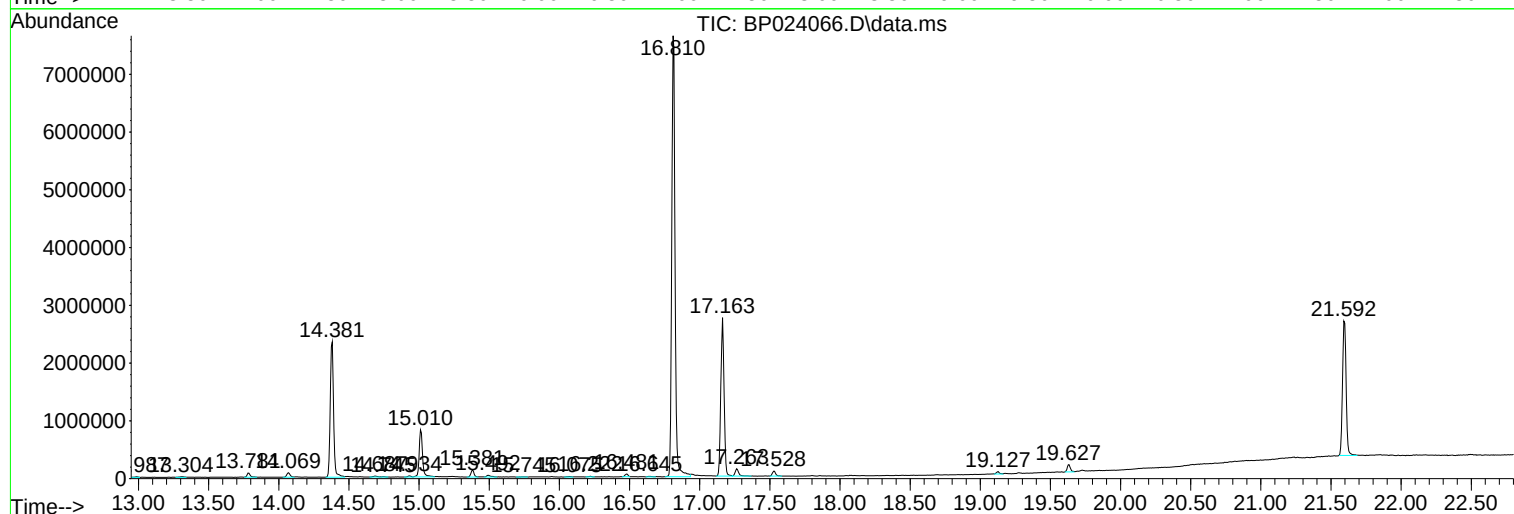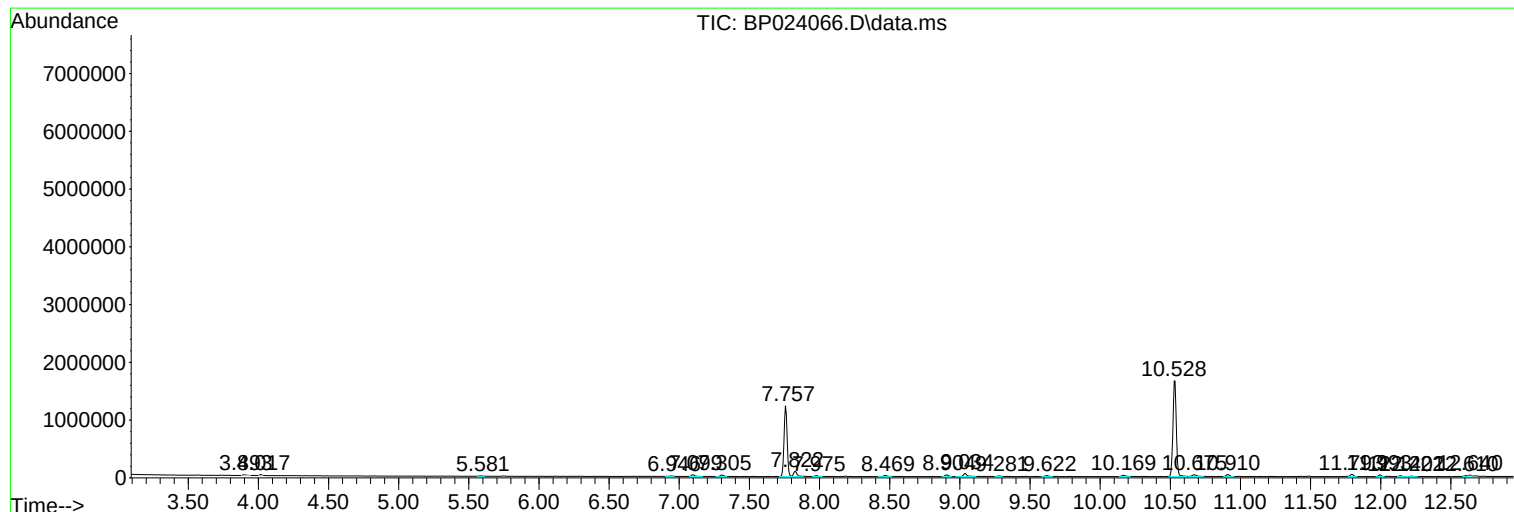

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021425\
Data File : BP024066.D
Acq On : 14 Feb 2025 18:06
Operator : RC/JU
Sample : Q1275-01DL2 500X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZT0DL2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Phenol, 2,3,4,6--tetrachloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.010	7.06 ng/ul	1342730	Acenaphthene-d10	14.381

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenol, 2,3,4,6-tetrachloro-	230	C6H2Cl4O	000058-90-2	99
2			Phenol, 2,3,4,6-tetrachloro-	230	C6H2Cl4O	000058-90-2	99
3			Phenol, 2,3,5,6-tetrachloro-	230	C6H2Cl4O	000935-95-5	99
4			Phenol, 2,3,4,6-tetrachloro-	230	C6H2Cl4O	000058-90-2	99
5			Phenol, 2,3,5,6-tetrachloro-	230	C6H2Cl4O	000935-95-5	98

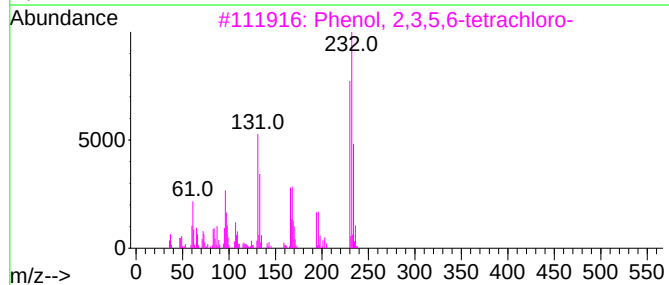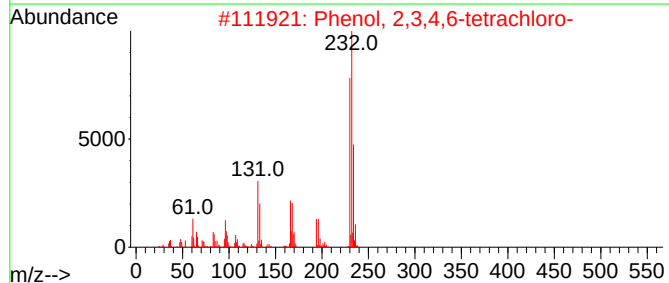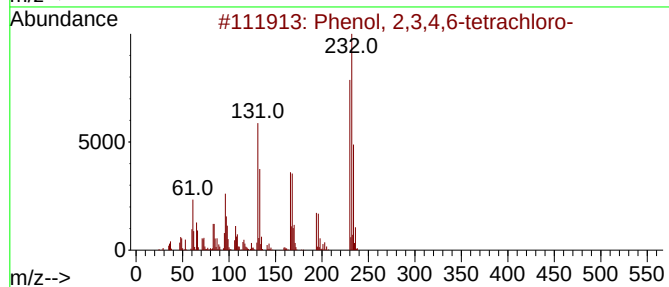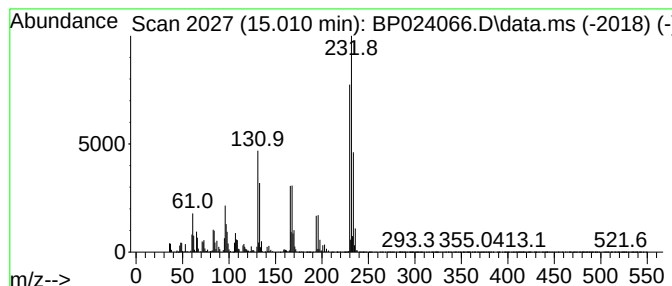

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021425\
Data File : BP024066.D
Acq On : 14 Feb 2025 18:06
Operator : RC/JU
Sample : Q1275-01DL2 500X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCZT0DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phenol, 2,3,4,6...	15.010	7.1	ng/ul	1342730	3	14.381	3806290	20.0