

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021521\
 Data File : BP004750.D
 Acq On : 15 Feb 2021 17:17
 Operator : CG/JU
 Sample : M1349-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Feb 16 00:05:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 15 12:16:19 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	46942	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	172374	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.42	164	99227	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.17	188	209428	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	241182	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	249842	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	5460	4.50	ng/uL	0.00
5) Phenol-d5	6.93	99	24458	6.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	51809	26.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	67796	23.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.48	113	42290	14.27	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	36452	30.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	42209	32.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	67208	25.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	4219	1.44	ng/ul	0.00
44) Dimethylphthalate-d6	13.82	166	243297	33.78	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	277926	31.72	ng/ul	0.00
52) 4-Nitrophenol-d4	14.62	143	8585	6.82	ng/ul	0.01
58) Fluorene-d10	15.41	176	209900	34.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.53	200	45668	36.08	ng/ul	0.00
71) Anthracene-d10	17.27	188	372021	40.28	ng/ul	0.00
79) Pyrene-d10	19.50	212	451652	40.00	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	526551	41.66	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.87	163	11729	1.579	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021521\
Data File : BP004750.D
Acq On : 15 Feb 2021 17:17
Operator : CG/JU
Sample : M1349-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Feb 16 00:05:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 15 12:16:19 2021
Response via : Initial Calibration

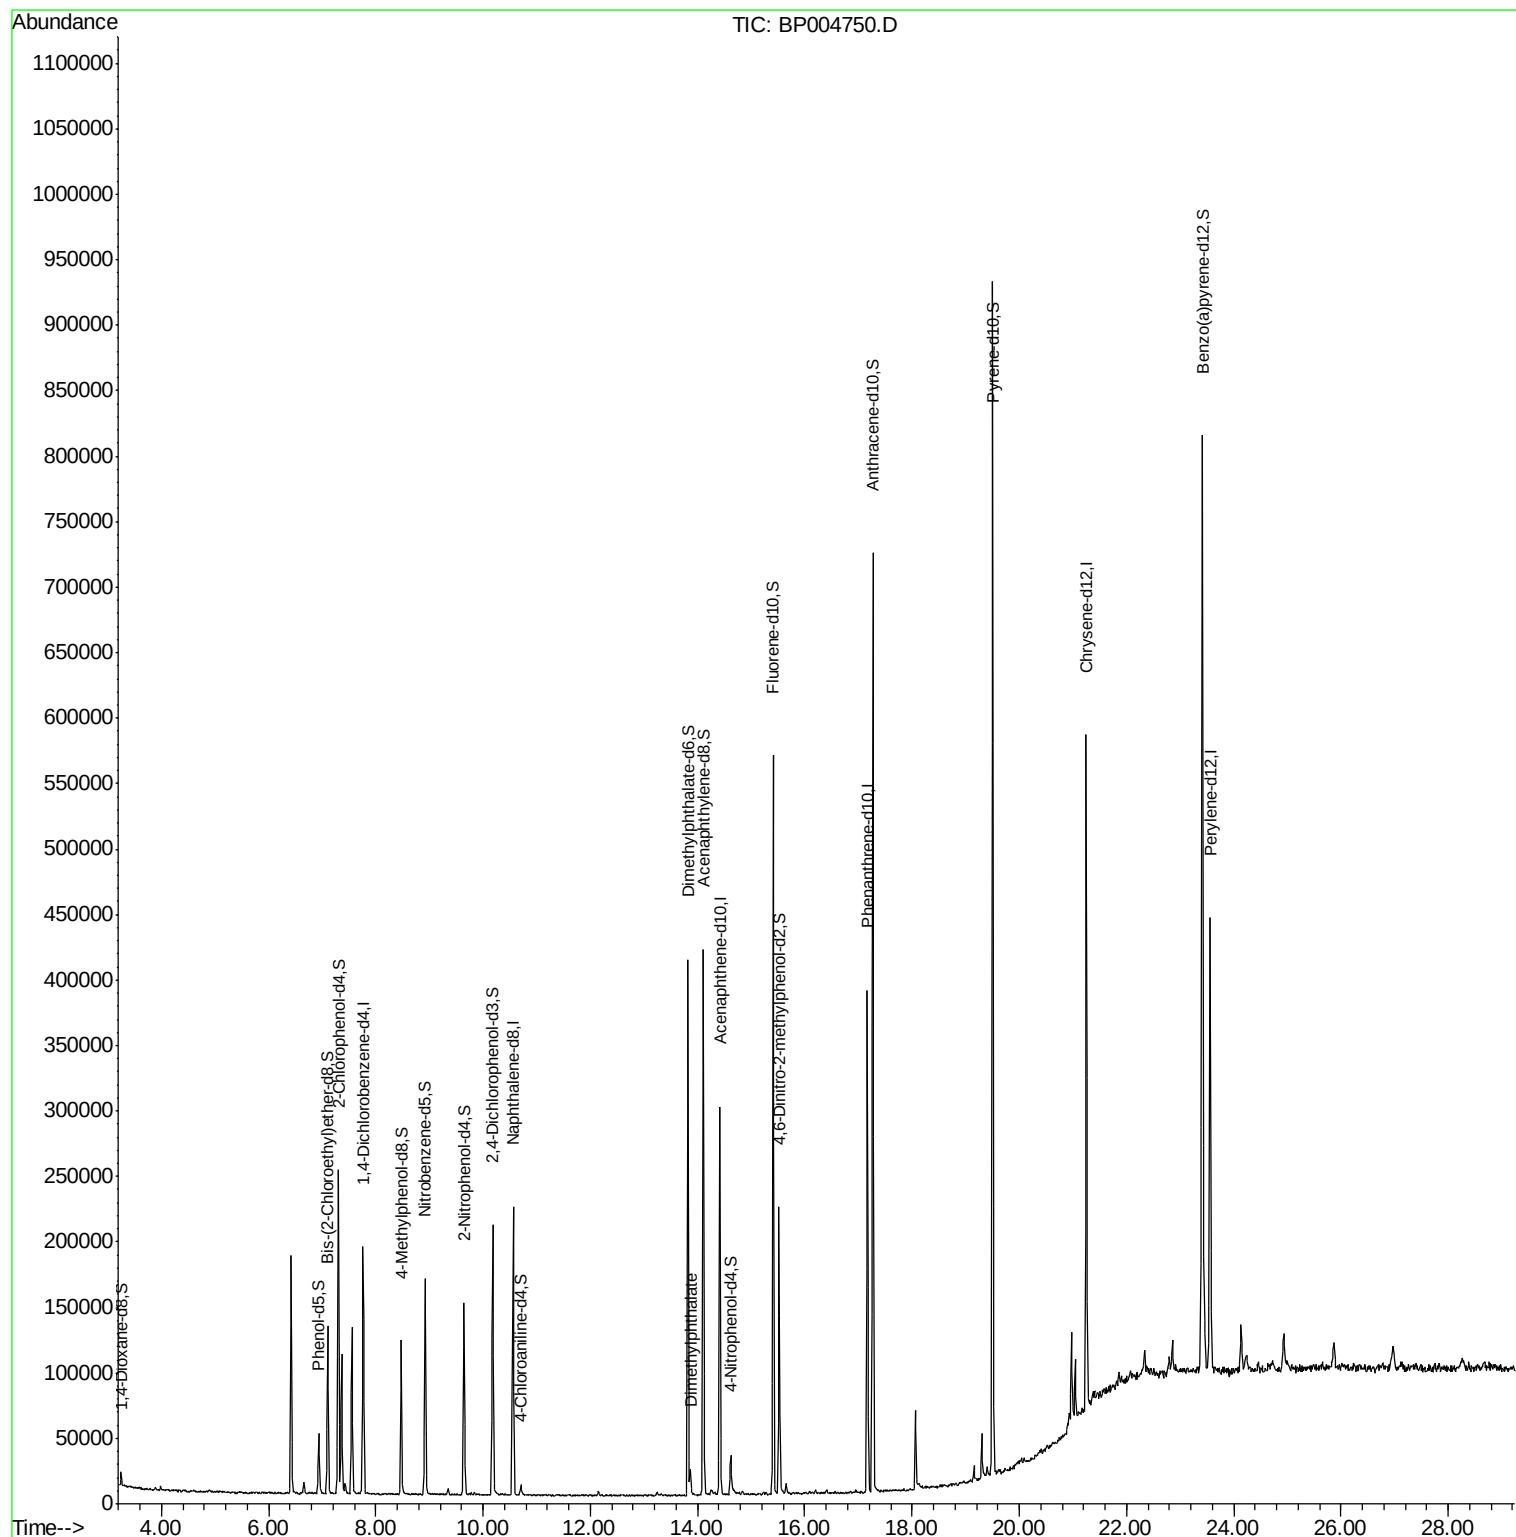

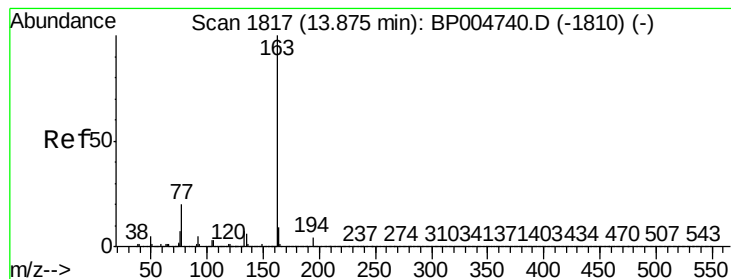

#45

Dimethylphthalate

Concen: 1.579 ng/ul

RT: 13.87 min Scan# 1817

Delta R.T. -0.00 min

Lab File: BP004750.D

Acq: 15 Feb 2021 17:17

Instrument :

BNA_P

ClientSampleId :


Tot Ion:163 Resp: 11729

Ion Ratio Lower Upper

163 100

194 4.1 3.8 5.6

164 8.3 8.0 12.0

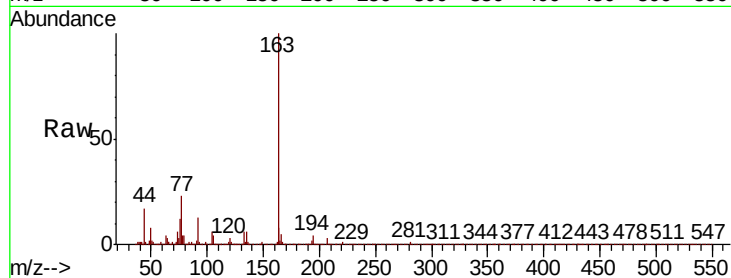

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

