

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021521\
 Data File : BP004753.D
 Acq On : 15 Feb 2021 18:58
 Operator : CG/JU
 Sample : M1349-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Feb 16 00:05:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 15 12:16:19 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	46391	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	178472	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.41	164	103662	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.17	188	217525	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	245751	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	252313	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	5718	4.76	ng/uL	0.00
5) Phenol-d5	6.93	99	24948	6.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	56154	29.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	71734	25.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.48	113	43876	14.98	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	38750	31.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	44661	33.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	73610	27.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	4098	1.35	ng/ul	0.00
44) Dimethylphthalate-d6	13.82	166	236999	31.50	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	290569	31.74	ng/ul	0.00
52) 4-Nitrophenol-d4	14.62	143	6561	4.99	ng/ul	0.00
58) Fluorene-d10	15.41	176	208078	32.27	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	38615	29.37	ng/ul	0.00
71) Anthracene-d10	17.26	188	340075	35.45	ng/ul	0.00
79) Pyrene-d10	19.50	212	408500	35.51	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.41	264	464623	36.40	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.87	163	12122	1.562	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021521\
Data File : BP004753.D
Acq On : 15 Feb 2021 18:58
Operator : CG/JU
Sample : M1349-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Feb 16 00:05:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 15 12:16:19 2021
Response via : Initial Calibration

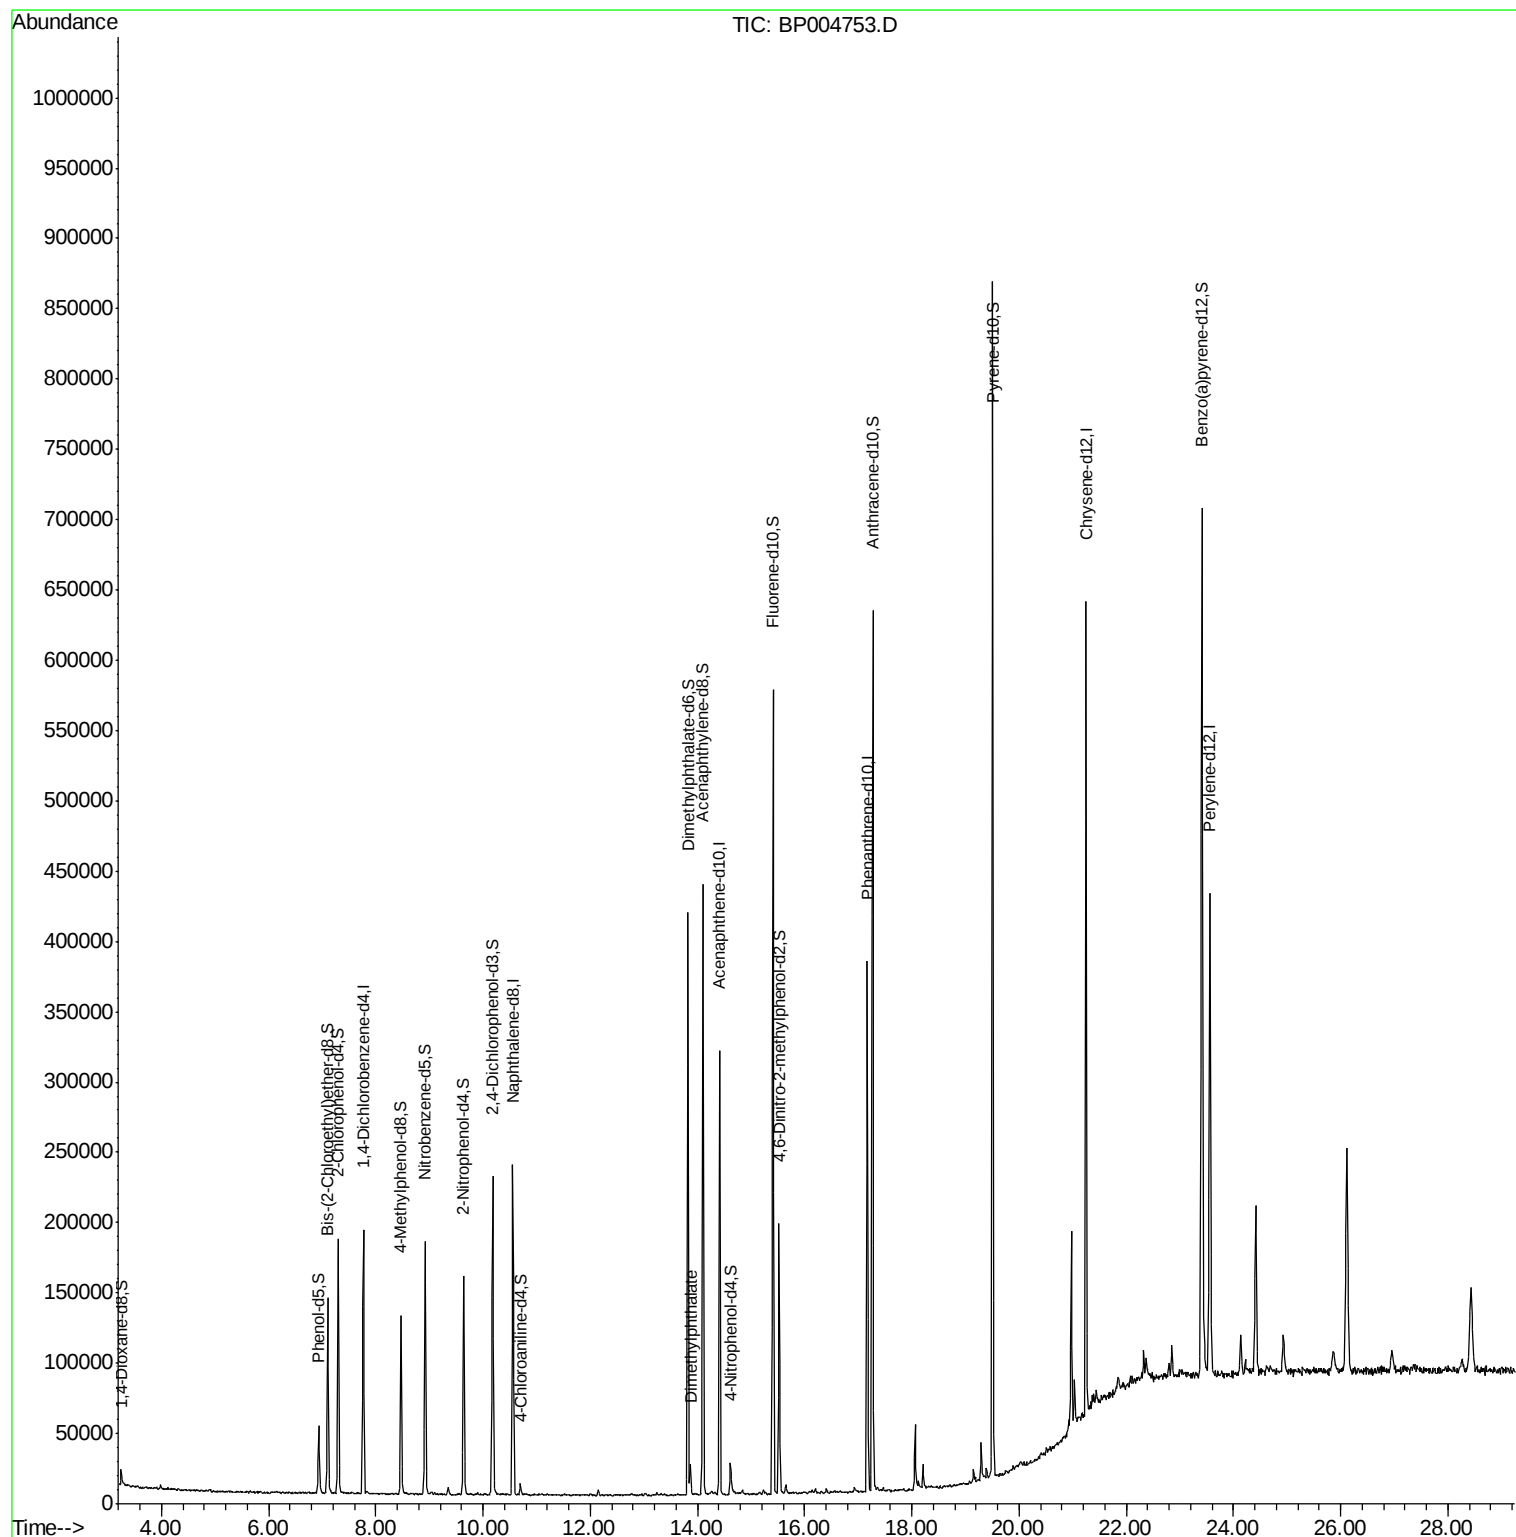

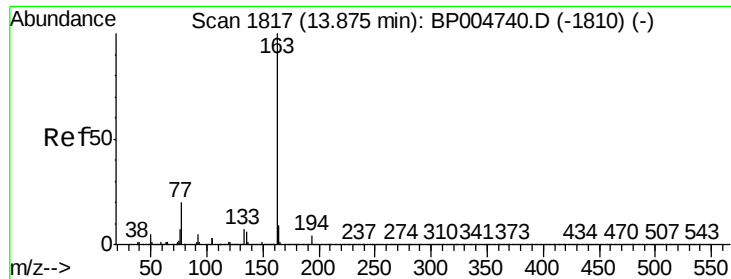

#45

Dimethylphthalate

Concen: 1.562 ng/ul

RT: 13.87 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BP004753.D

Acq: 15 Feb 2021 18:58

Instrument :

BNA_P

ClientSampleId :


Tot Ion:163 Resp: 12122

Ion Ratio Lower Upper

163 100

194 5.8 3.8 5.6#

164 9.7 8.0 12.0

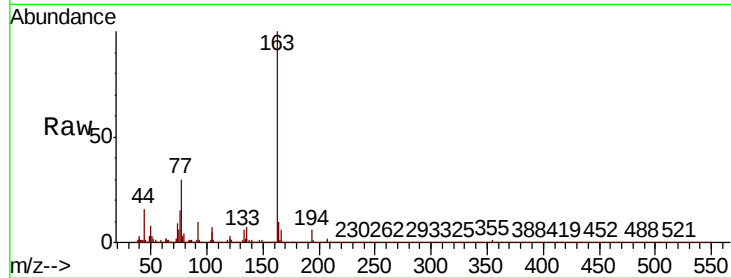

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

