

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021521\
 Data File : BP004743.D
 Acq On : 15 Feb 2021 13:21
 Operator : CG/JU
 Sample : M1349-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGQ1

Quant Time: Feb 15 13:59:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 15 12:16:19 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	45864	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	170152	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.42	164	97307	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.17	188	201397	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	220534	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	223448	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	5763	4.86	ng/uL	0.00
5) Phenol-d5	6.93	99	28339	7.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	64187	33.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	81695	29.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	48690	16.81	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	43450	36.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	50615	39.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	84100	32.41	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	4770	1.65	ng/ul	0.00
44) Dimethylphthalate-d6	13.83	166	272783	38.62	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	329395	38.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.62	143	7954	6.44	ng/ul	0.00
58) Fluorene-d10	15.41	176	223417	36.91	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.53	200	45279	37.19	ng/ul	0.00
71) Anthracene-d10	17.27	188	360095	40.54	ng/ul	0.00
79) Pyrene-d10	19.51	212	426685	41.33	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	484445	42.86	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.87	163	19218	2.638	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021521\
Data File : BP004743.D
Acq On : 15 Feb 2021 13:21
Operator : CG/JU
Sample : M1349-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGQ1

Quant Time: Feb 15 13:59:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 15 12:16:19 2021
Response via : Initial Calibration

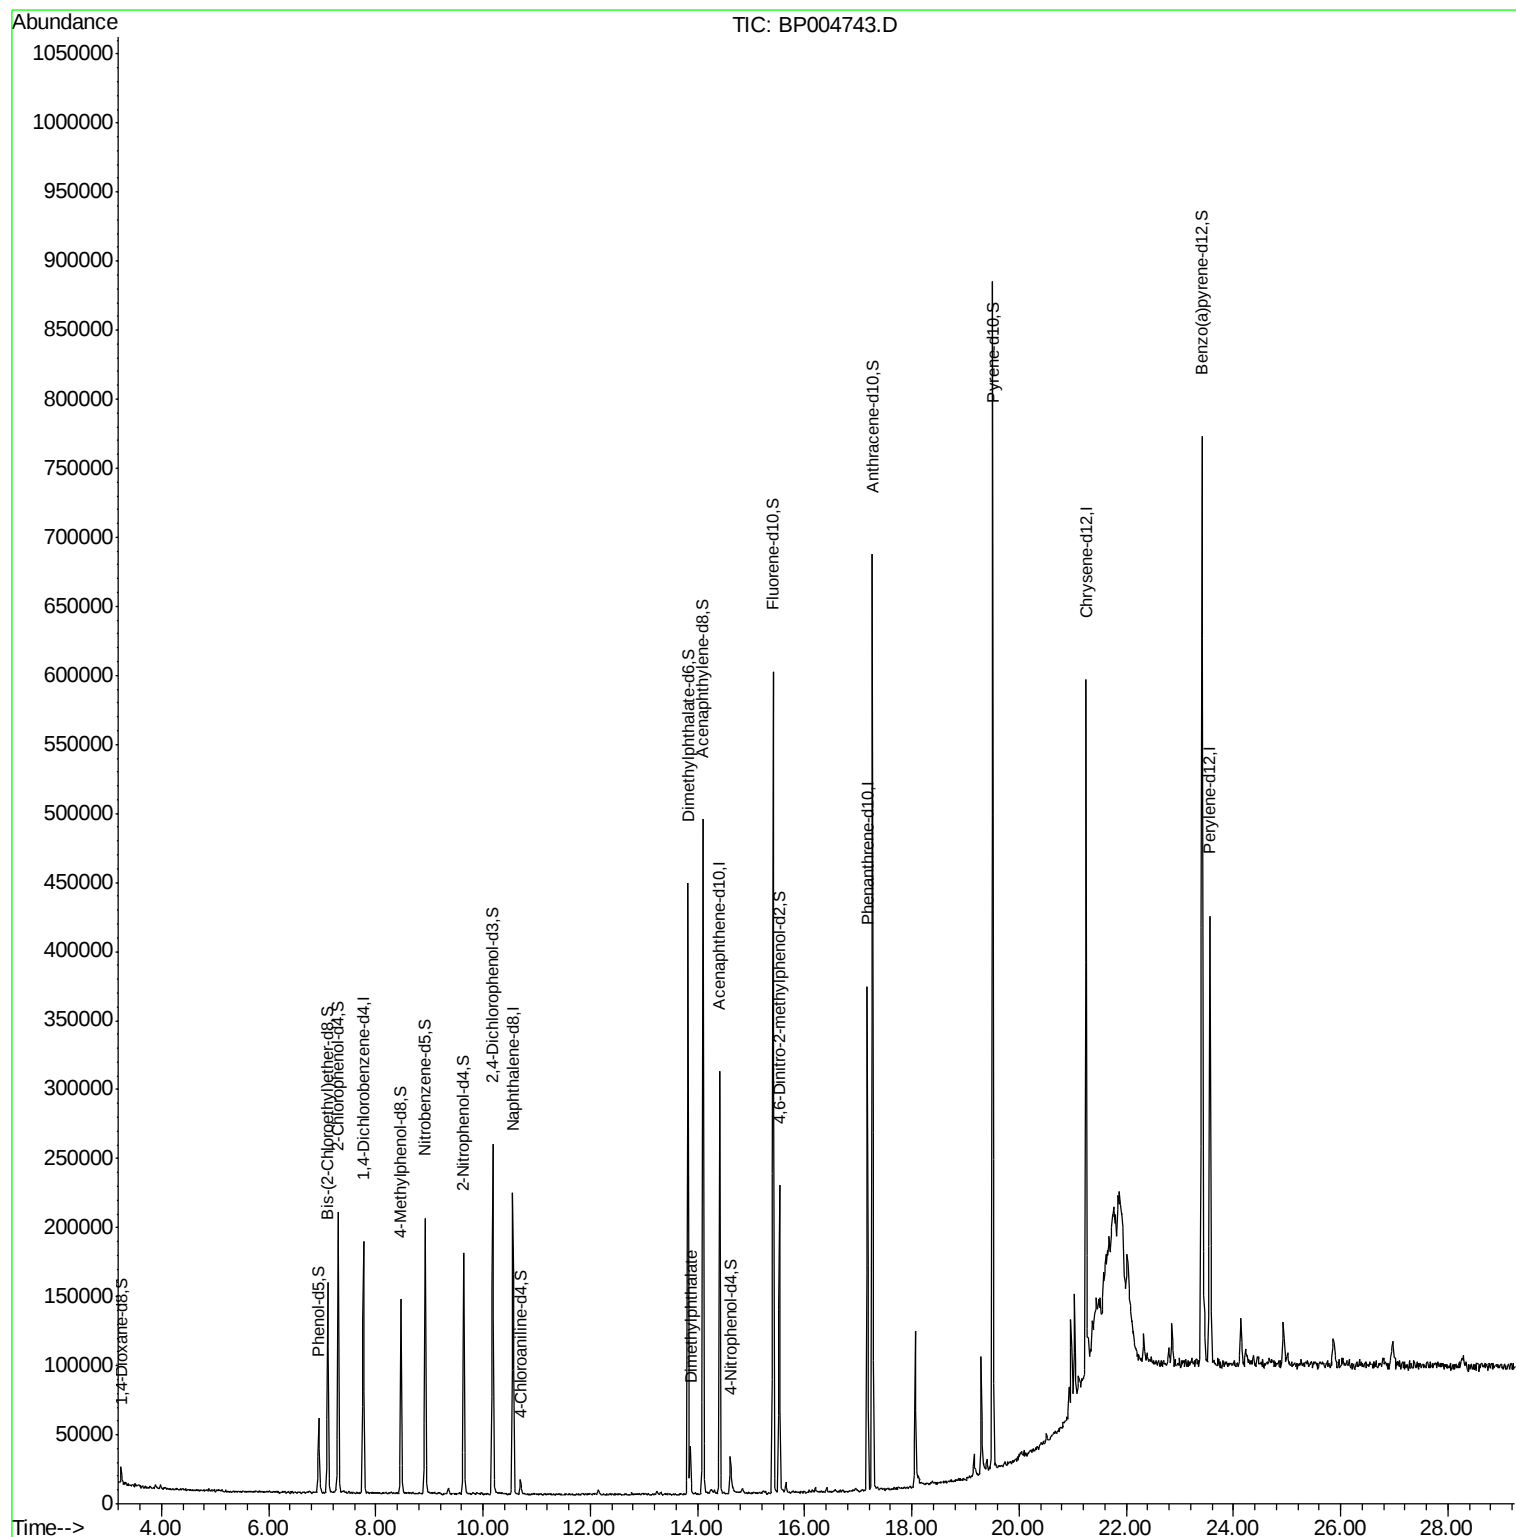

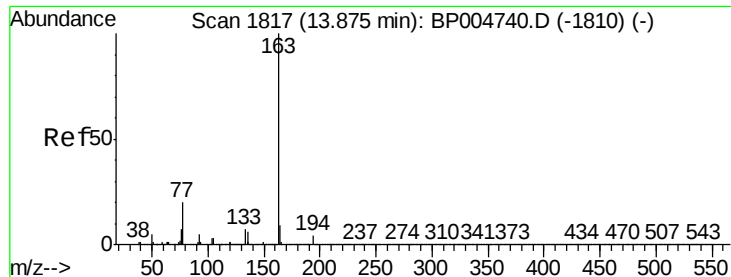

#45

Dimethylphthalate

Concen: 2.638 ng/ul

RT: 13.87 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BP004743.D

Acq: 15 Feb 2021 13:21

Instrument :

BNA_P

ClientSampleId :

DBGQ1


Tot Ion:163 Resp: 19218

Ion Ratio Lower Upper

163 100

194 3.3 3.8 5.6#

164 11.2 8.0 12.0

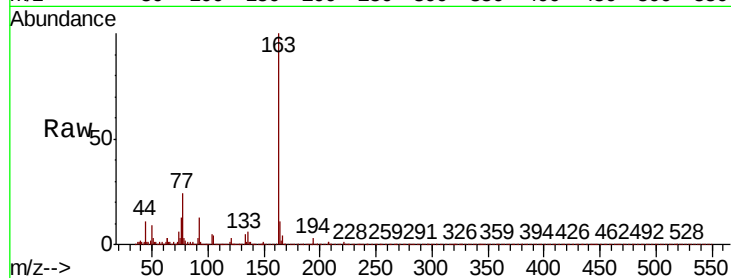

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

