

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021521\
 Data File : BP004752.D
 Acq On : 15 Feb 2021 18:24
 Operator : CG/JU
 Sample : M1349-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBG2

Manual Integrations
 APPROVED

mohammad
 2/16/2021 10:45:41 AM

Quant Time: Feb 16 00:26:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 15 12:16:19 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	48045	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	180605	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.41	164	108636	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.17	188	229249	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	258091	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	264612	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	6559	5.28	ng/uL	0.00
5) Phenol-d5	6.93	99	26250	6.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	53911	26.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	70503	24.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	45182	14.89	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	36813	29.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	42678	31.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	71617	26.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	4268	1.39	ng/ul	0.00
44) Dimethylphthalate-d6	13.82	166	243151	30.83	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	294854	30.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.62	143	8152m	5.91	ng/ul	0.00
58) Fluorene-d10	15.41	176	218310	32.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	45575	32.89	ng/ul	0.00
71) Anthracene-d10	17.27	188	385889	38.17	ng/ul	0.00
79) Pyrene-d10	19.50	212	460099	38.08	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.41	264	532399	39.77	ng/ul	0.00

Target Compounds				Ovalue	
45) Dimethylphthalate	13.87	163	12355	1.519	ng/ul# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021521\
Data File : BP004752.D
Acq On : 15 Feb 2021 18:24
Operator : CG/JU
Sample : M1349-15
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
DBGT2

Quant Time: Feb 16 00:26:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 15 12:16:19 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
2/16/2021 10:45:41 AM

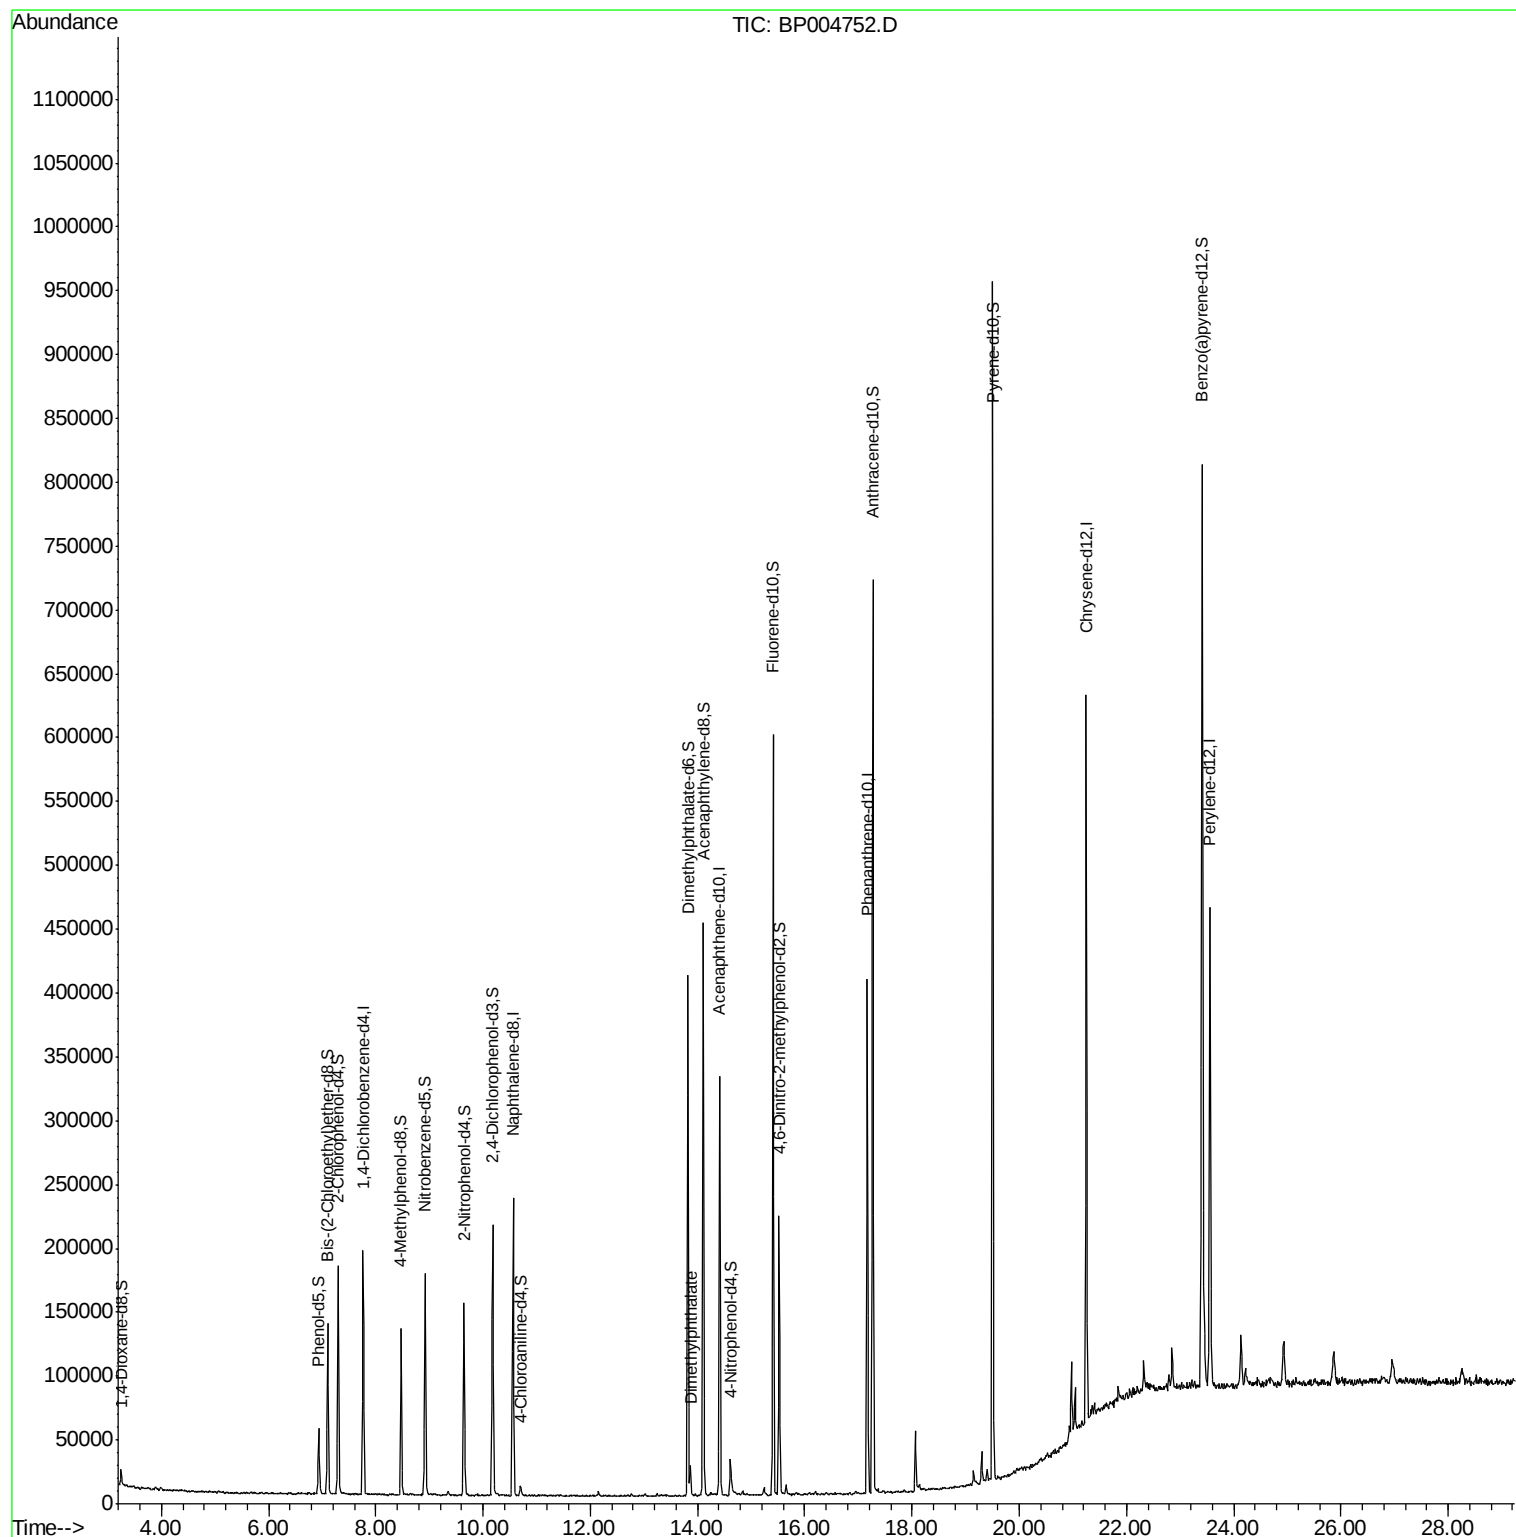

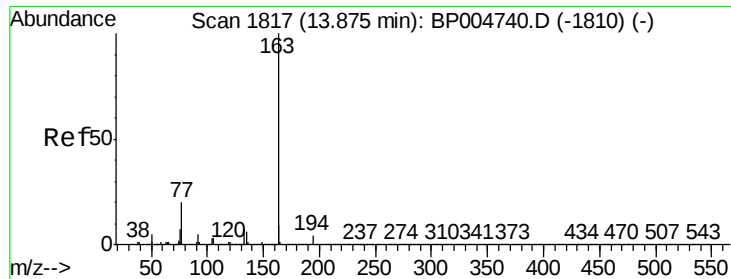

#45
 Dimethylphthalate
 Concen: 1.519 ng/ul
 RT: 13.87 min Scan# 1816
 Delta R.T. -0.01 min
 Lab File: BP004752.D
 Acq: 15 Feb 2021 18:24

Instrument :
 BNA_P
 ClientSampleId :
 DBG2

Tot Ion:	163	Resp:	12355
Ion Ratio	Lower	Upper	
163	100		
194	2.7	3.8	5.6#
164	11.0	8.0	12.0

Manual Integrations
 APPROVED

mohammad
 2/16/2021 10:45:41 AM

