

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021521\
 Data File : BP004754.D
 Acq On : 15 Feb 2021 19:32
 Operator : CG/JU
 Sample : M1349-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGS5

Manual Integrations
 APPROVED

mohammad
 2/16/2021 10:45:43 AM

Quant Time: Feb 16 00:44:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 15 12:16:19 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	48940	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	177638	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.41	164	95239	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.17	188	186475m	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	183689	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	196081	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	5772	4.56	ng/uL	0.00
5) Phenol-d5	6.93	99	24491	6.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	60144	29.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	75783	25.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	44443	14.38	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	41880	34.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	47368	35.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	75977	28.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	3802	1.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.82	166	244033	35.30	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	301135	35.80	ng/ul	0.00
52) 4-Nitrophenol-d4	14.62	143	5722m	4.74	ng/ul	0.00
58) Fluorene-d10	15.41	176	209422	35.35	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	39152	34.73	ng/ul	0.00
71) Anthracene-d10	17.27	188	332420	40.42	ng/ul	0.00
79) Pyrene-d10	19.50	212	370889	43.13	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.41	264	422608	42.60	ng/ul	0.00

Target Compounds				Ovalue	
45) Dimethylphthalate	13.87	163	9232	1.295	ng/ul# 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021521\
Data File : BP004754.D
Acq On : 15 Feb 2021 19:32
Operator : CG/JU
Sample : M1349-16
Misc :
ALS Vial : 16 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
DBG55

Quant Time: Feb 16 00:44:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 15 12:16:19 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
2/16/2021 10:45:43 AM

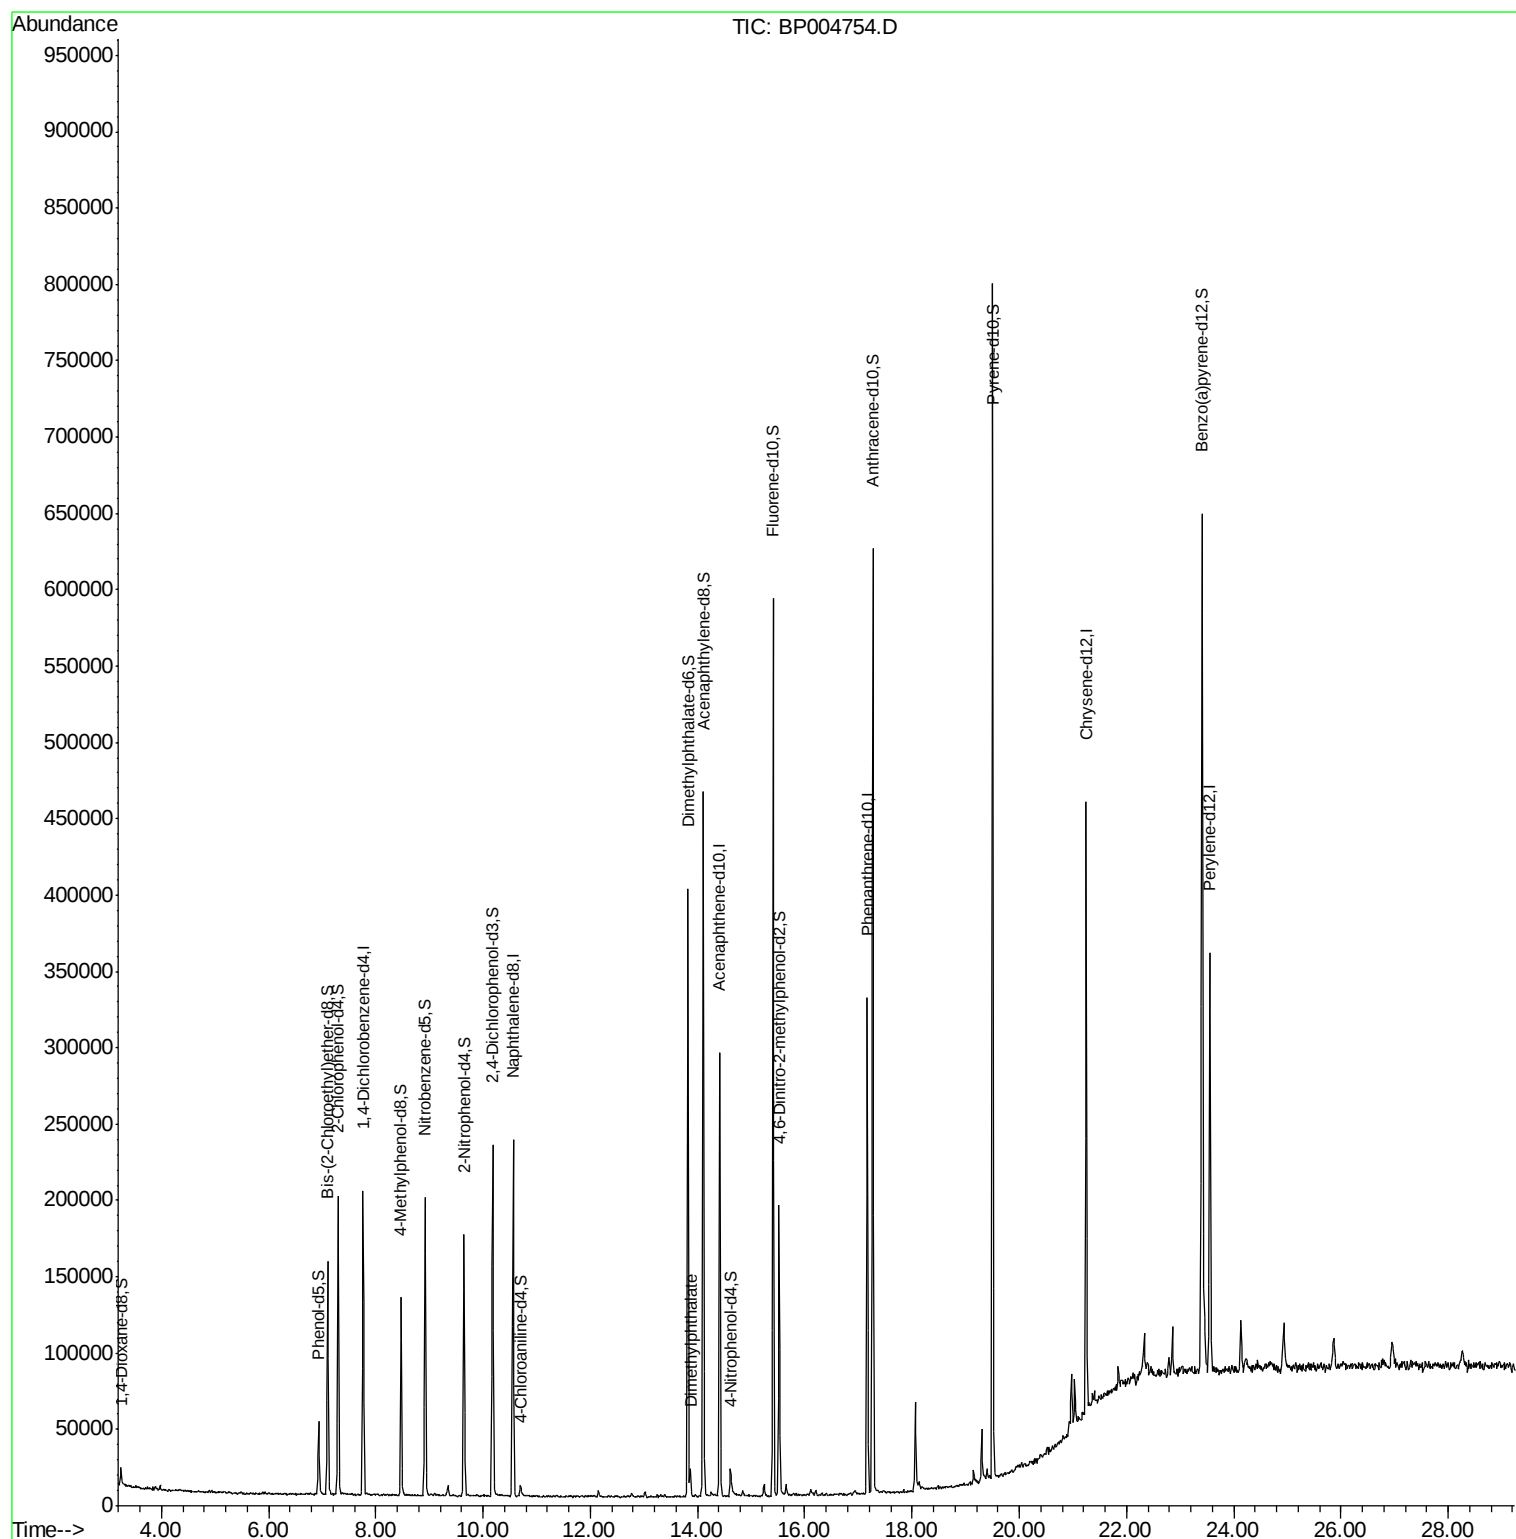

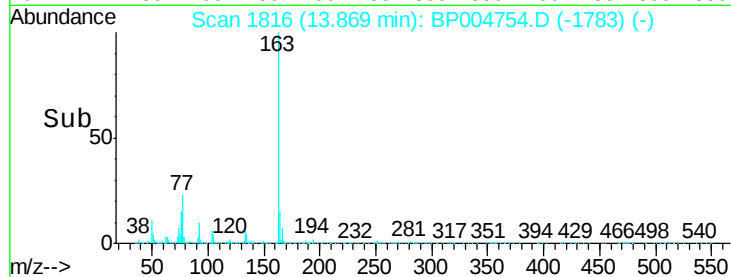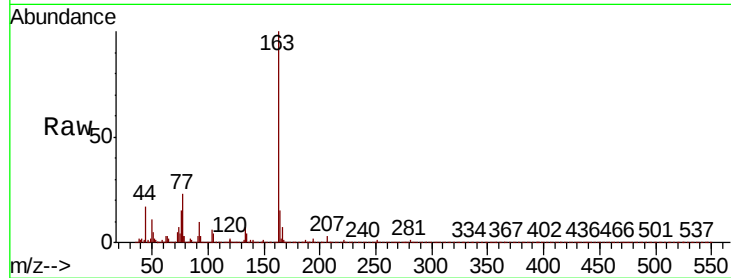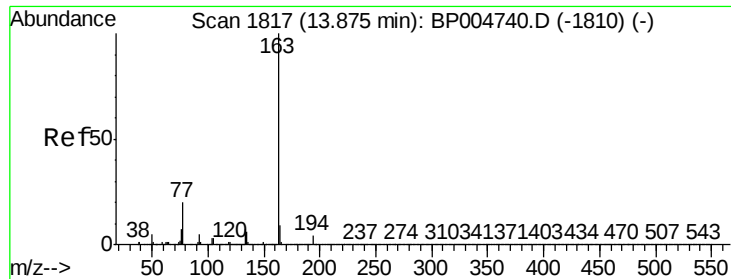

#45
 Dimethylphthalate
 Concen: 1.295 ng/ul
 RT: 13.87 min Scan# 1816
 Delta R.T. -0.01 min
 Lab File: BP004754.D
 Acq: 15 Feb 2021 19:32

Instrument :
 BNA_P
 ClientSampleId :
 DBGS5

Tot Ion	Ratio	Lower	Upper
163	100		
194	2.4	3.8	5.6#
164	15.4	8.0	12.0#

Manual Integrations
 APPROVED

mohammad
 2/16/2021 10:45:43 AM

