

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
Data File : BP009152.D
Acq On : 15 Feb 2022 13:49
Operator : CG/JU
Sample : PB142569BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142569BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.387	401	408	435	rBV	3655708	5915250	43.91%	9.710%
2	6.987	672	680	701	rBV	3218187	5917065	43.93%	9.713%
3	7.787	809	816	838	rBV	773250	1342133	9.96%	2.203%
4	8.958	1007	1015	1049	rBV	2157507	4124626	30.62%	6.771%
5	10.587	1284	1292	1318	rBV	844365	1788916	13.28%	2.936%
6	13.057	1703	1712	1729	rBV	6627102	10531353	78.18%	17.287%
7	14.440	1938	1947	1970	rBV	1451948	2467255	18.32%	4.050%
8	15.940	2193	2202	2235	rBV	4379639	7740650	57.47%	12.706%
9	17.198	2409	2416	2432	rBV	1664648	2731897	20.28%	4.484%
10	19.757	2845	2851	2863	rBV	10175019	13470024	100.00%	22.111%
11	21.292	3107	3112	3124	rBV	1740373	2596053	19.27%	4.261%
12	23.686	3513	3519	3530	rVB2	1062657	2295300	17.04%	3.768%




Sum of corrected areas: 60920522

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
Data File : BP009152.D
Acq On : 15 Feb 2022 13:49
Operator : CG/JU
Sample : PB142569BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142569BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

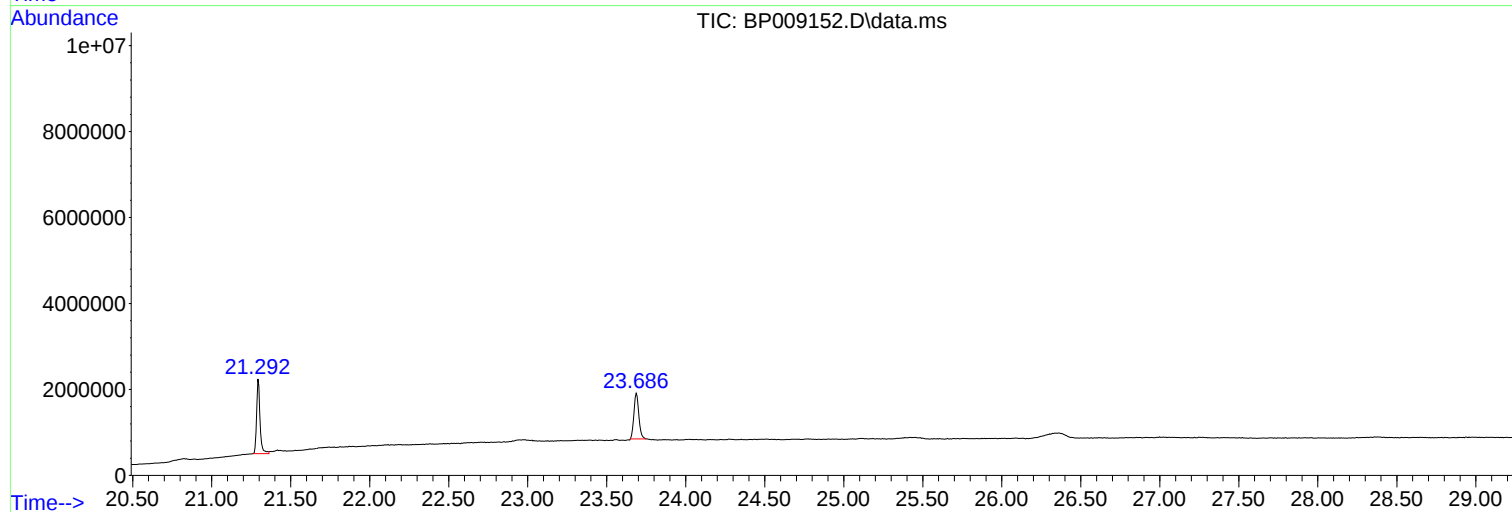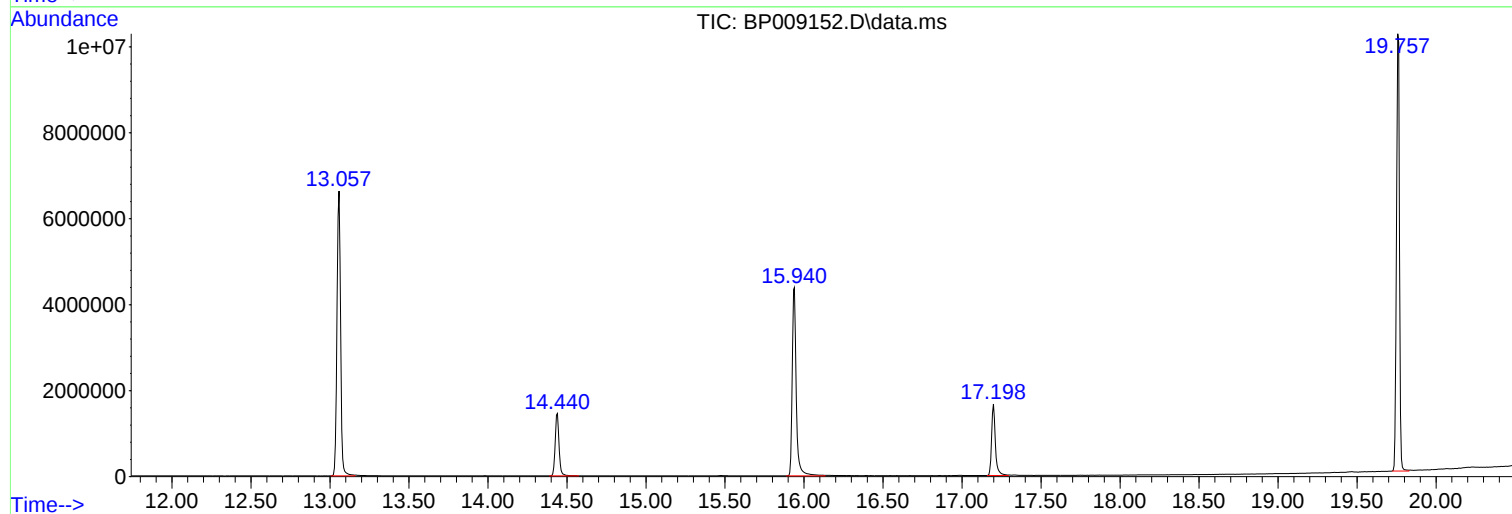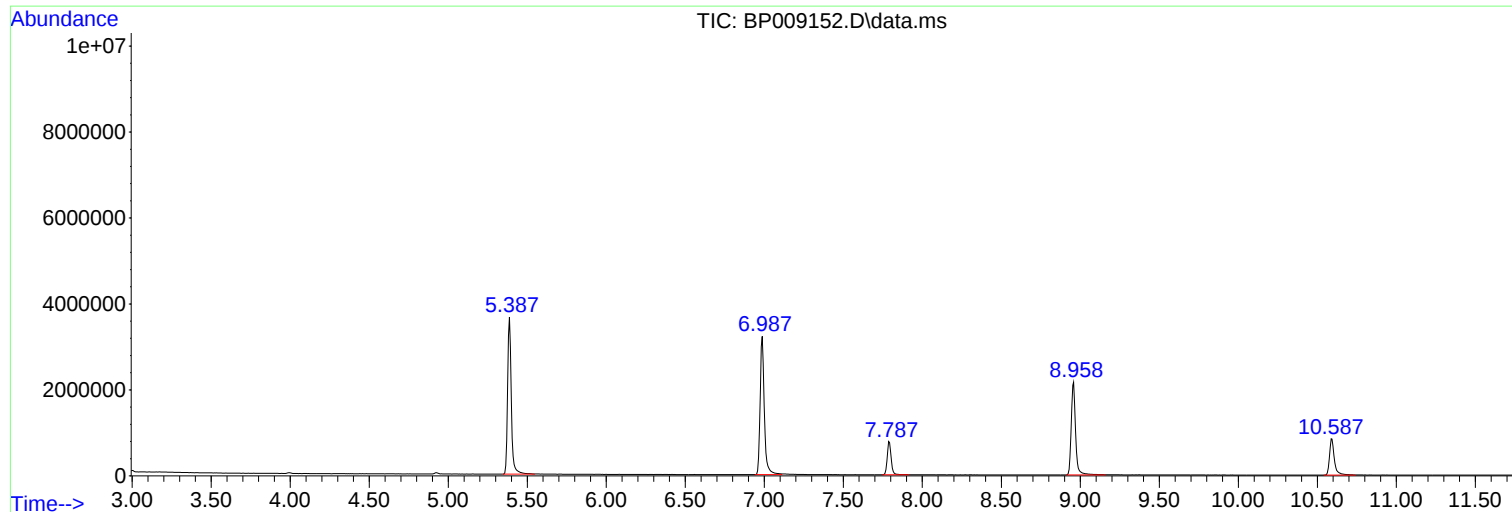

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
Data File : BP009152.D
Acq On : 15 Feb 2022 13:49
Operator : CG/JU
Sample : PB142569BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142569BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
Data File : BP009152.D
Acq On : 15 Feb 2022 13:49
Operator : CG/JU
Sample : PB142569BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142569BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------