

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
 Data File : BP009165.D
 Acq On : 15 Feb 2022 21:17
 Operator : CG/JU
 Sample : N1521-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP3-A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	401	407	431	rBV	1842385	3202610	46.23%	9.138%
2	6.981	672	679	713	rBV	1501545	3218831	46.46%	9.184%
3	7.781	808	815	836	rBV	550227	1000466	14.44%	2.855%
4	8.946	1006	1013	1041	rBV	972061	2116599	30.55%	6.039%
5	10.587	1284	1292	1316	rBV	570712	1249120	18.03%	3.564%
6	13.051	1703	1711	1733	rBV	2944279	5011251	72.34%	14.299%
7	14.428	1938	1945	1965	rBV	905417	1590490	22.96%	4.538%
8	15.933	2194	2201	2220	rBV	1937868	3570003	51.53%	10.186%
9	17.192	2408	2415	2431	rBV	1049173	1848208	26.68%	5.273%
10	18.086	2563	2567	2576	rBV2	71854	150576	2.17%	0.430%
11	19.327	2774	2778	2787	rBV5	41022	94276	1.36%	0.269%
12	19.751	2844	2850	2863	rBV	5525850	6927591	100.00%	19.766%
13	20.992	3057	3061	3066	rBV2	182668	263881	3.81%	0.753%
14	21.286	3106	3111	3120	rBV	1556170	2287831	33.02%	6.528%
15	23.674	3511	3517	3529	rVB2	1067497	2515490	36.31%	7.177%




Sum of corrected areas: 35047223

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
Data File : BP009165.D
Acq On : 15 Feb 2022 21:17
Operator : CG/JU
Sample : N1521-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP3-A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

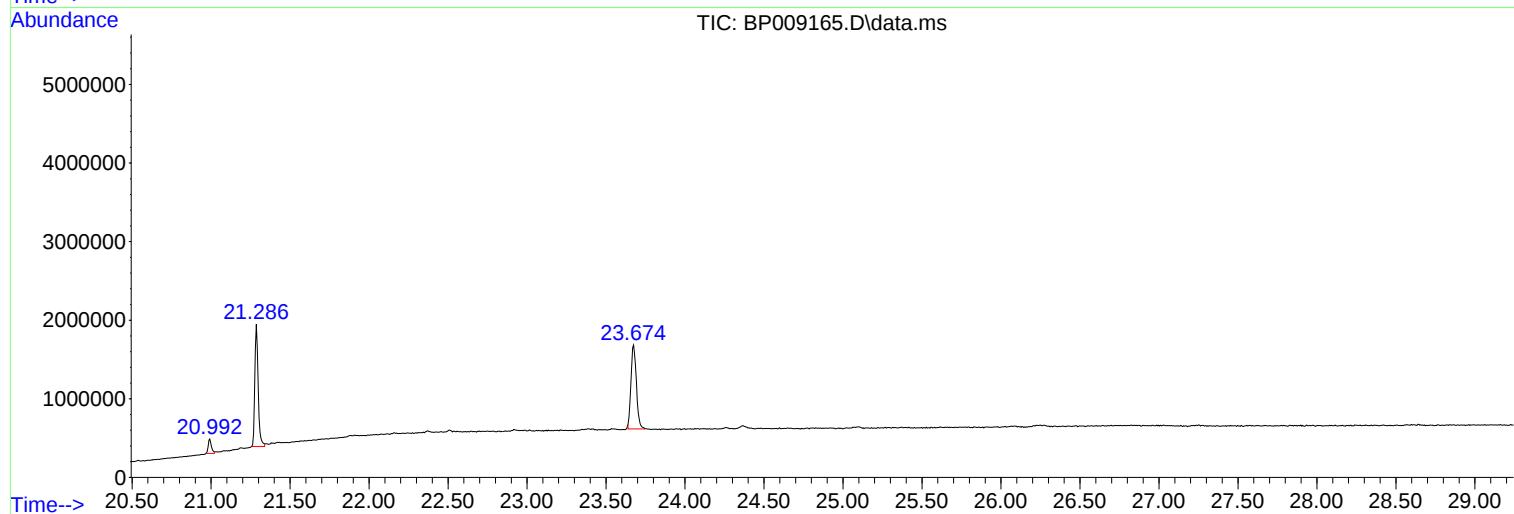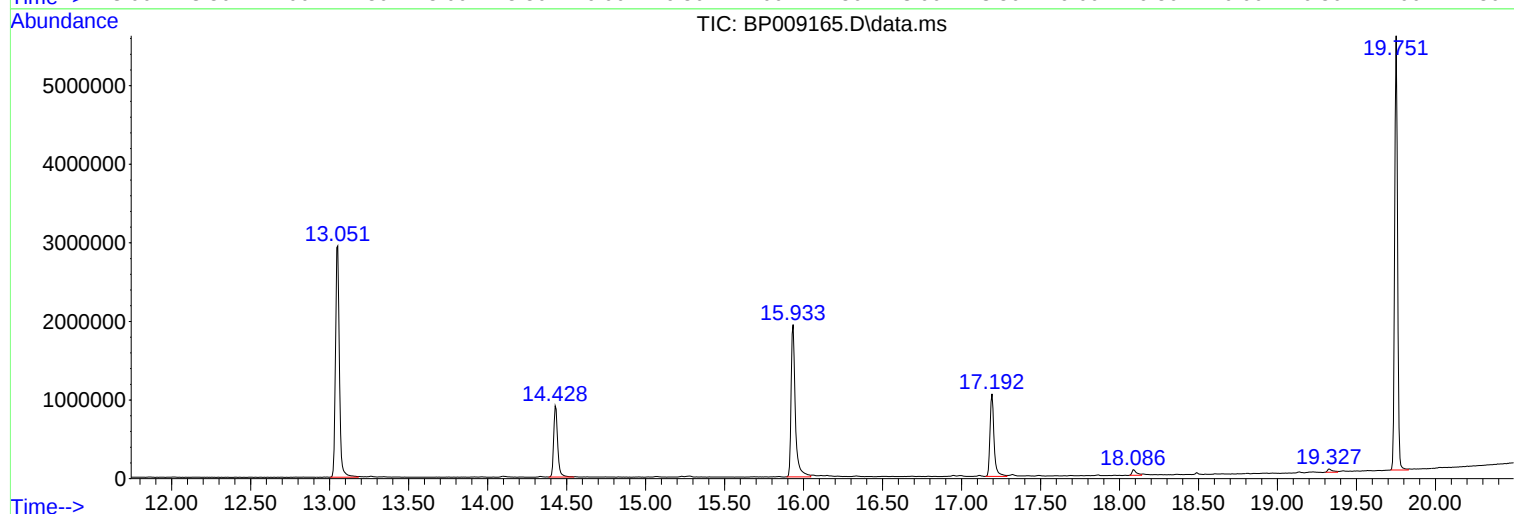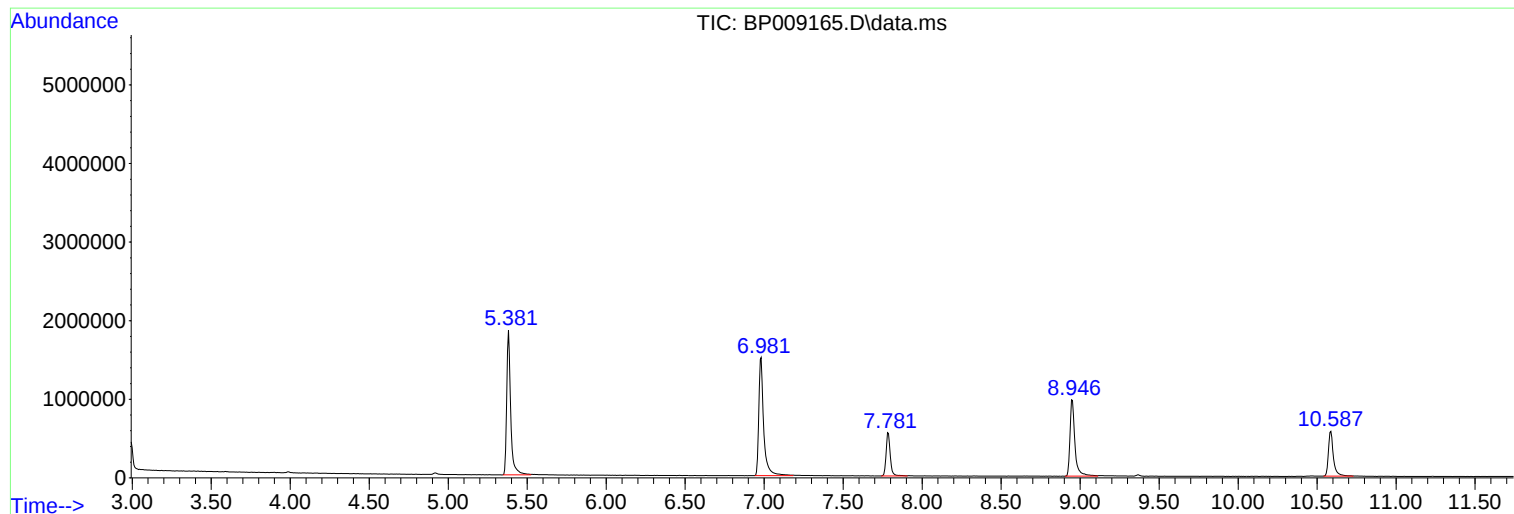

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
Data File : BP009165.D
Acq On : 15 Feb 2022 21:17
Operator : CG/JU
Sample : N1521-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP3-A










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Heneicosanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.992	2.31 ng	263881	Chrysene-d12	21.286

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Heneicosanol	312	C21H44O	015594-90-8	95
2			E-15-Heptadecenal	252	C17H32O	1000130-97-9	94
3			Pentacos-1-ene	350	C25H50	016980-85-1	94
4			n-Nonadecanol-1	284	C19H40O	001454-84-8	94
5			Nonacos-1-ene	406	C29H58	018835-35-3	94

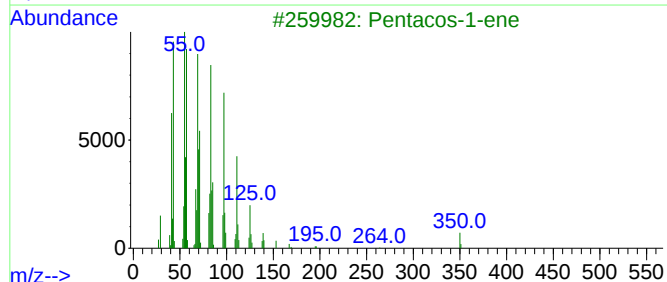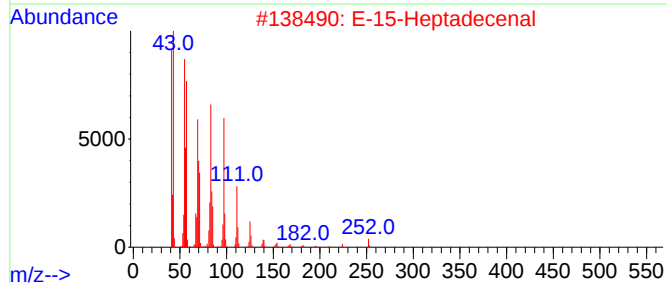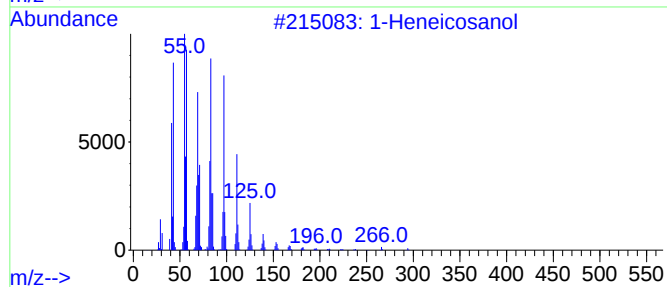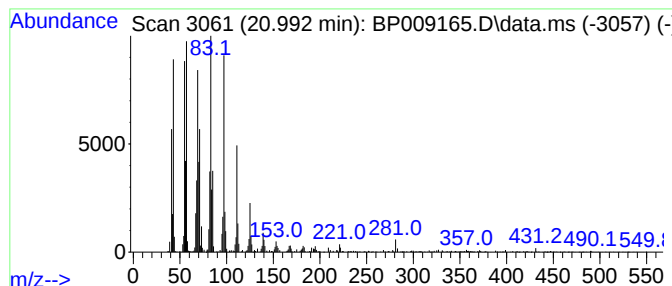

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
Data File : BP009165.D
Acq On : 15 Feb 2022 21:17
Operator : CG/JU
Sample : N1521-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP3-A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Heneicosanol	20.992	2.3	ng	263881	5	21.286	2287830	20.0