
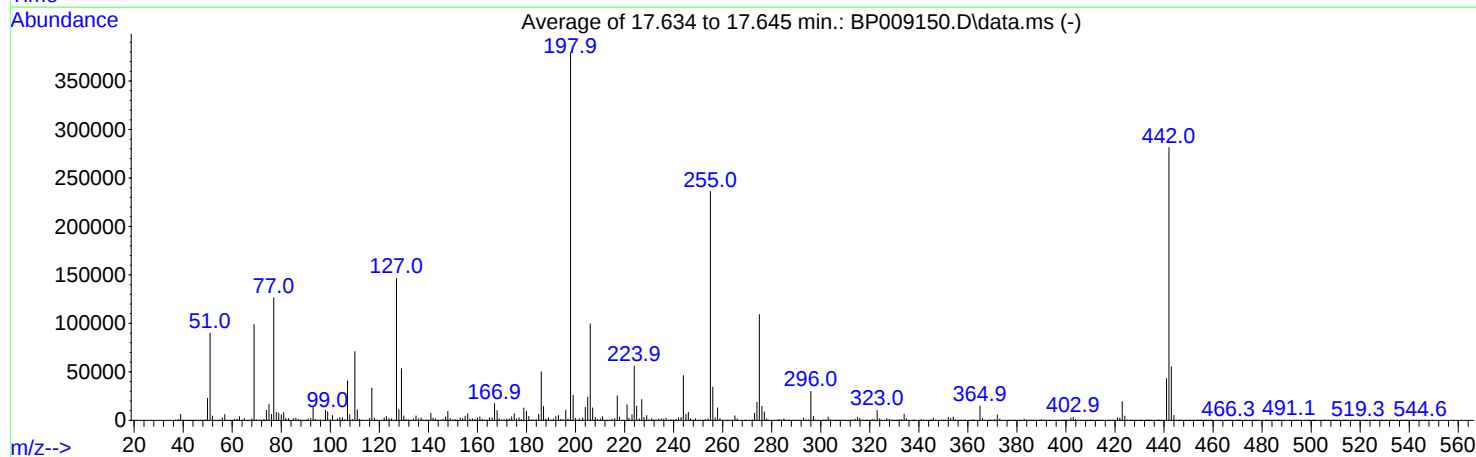


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
 Data File : BP009150.D
 Acq On : 15 Feb 2022 12:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 16 01:29:44 2022

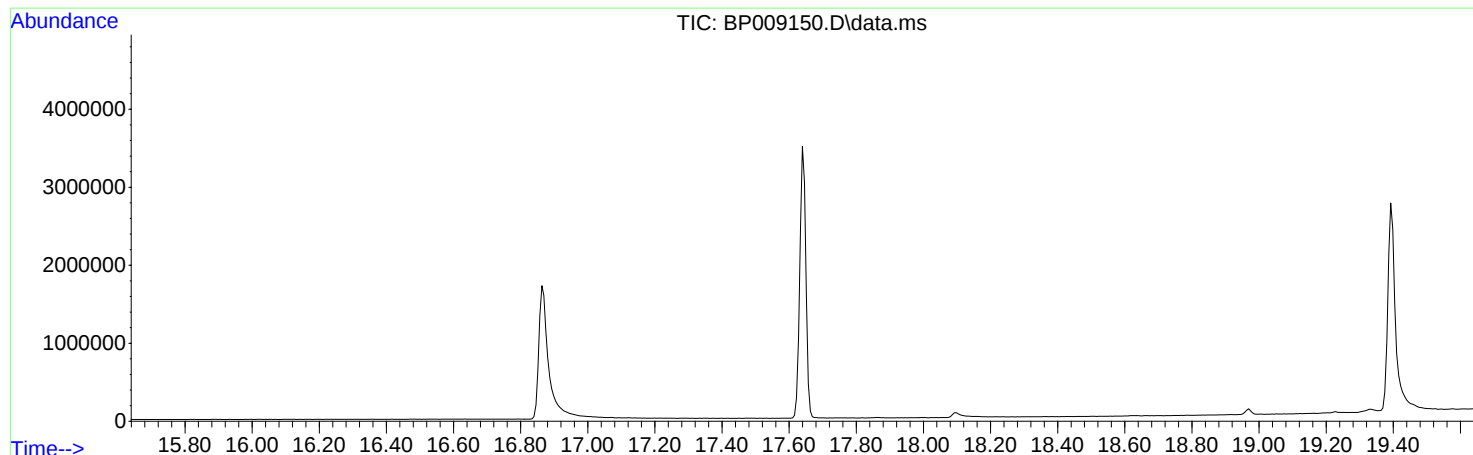




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.8	90156	PASS
68	69	0.00	2	1.6	1619	PASS
69	198	0.00	100	26.1	98872	PASS
70	69	0.00	2	0.5	493	PASS
127	198	10	80	38.6	146591	PASS
197	198	0.00	2	0.4	1575	PASS
198	198	100	100	100.0	379409	PASS
199	198	5	9	6.8	25868	PASS
275	198	10	60	28.8	109095	PASS
365	198	1	100	3.9	14655	PASS
441	198	0.01	100	11.3	43027	PASS
442	442	100	100	100.0	281323	PASS
443	442	15	24	19.7	55283	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
Data File : BP009150.D
Acq On : 15 Feb 2022 12:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 16 02:32:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 01:29:44 2022
Response via : Initial Calibration

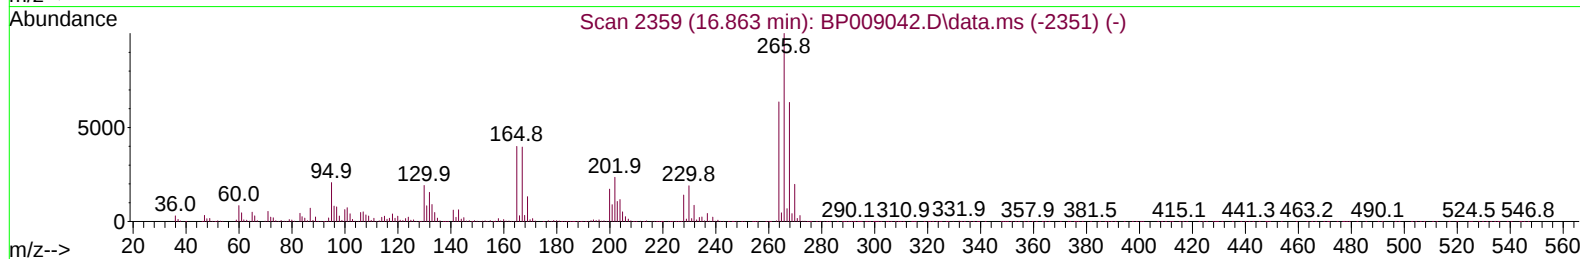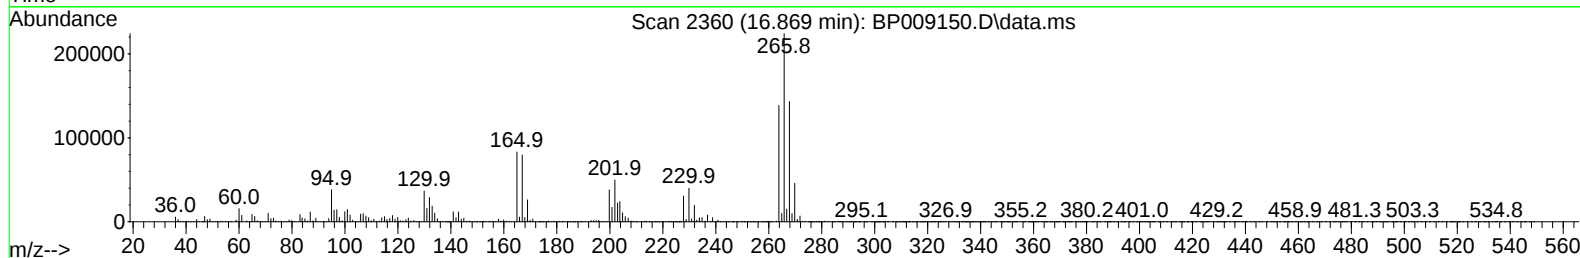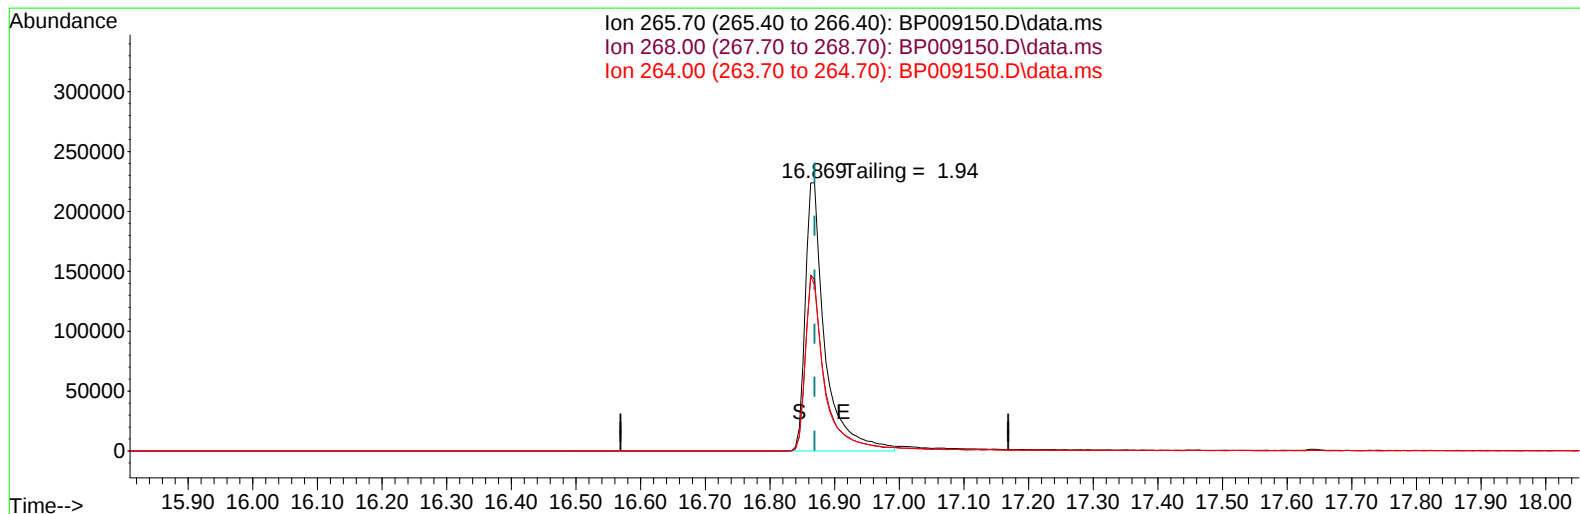

TIC: BP009150.D\data.ms

(70) Pentachlorophenol (C)

16.869min (+ 0.000) 669658.57 ng




response 485167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.90
264.00	62.90	61.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021522\
Data File : BP009150.D
Acq On : 15 Feb 2022 12:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 16 02:32:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 01:29:44 2022
Response via : Initial Calibration

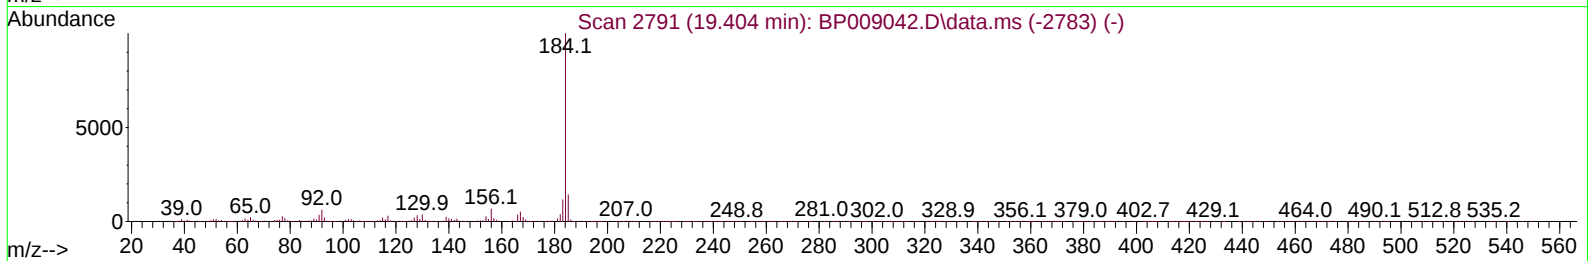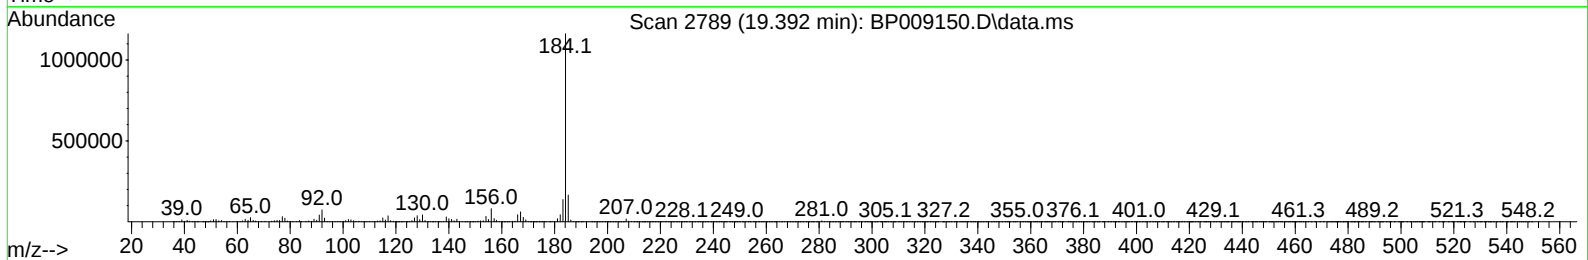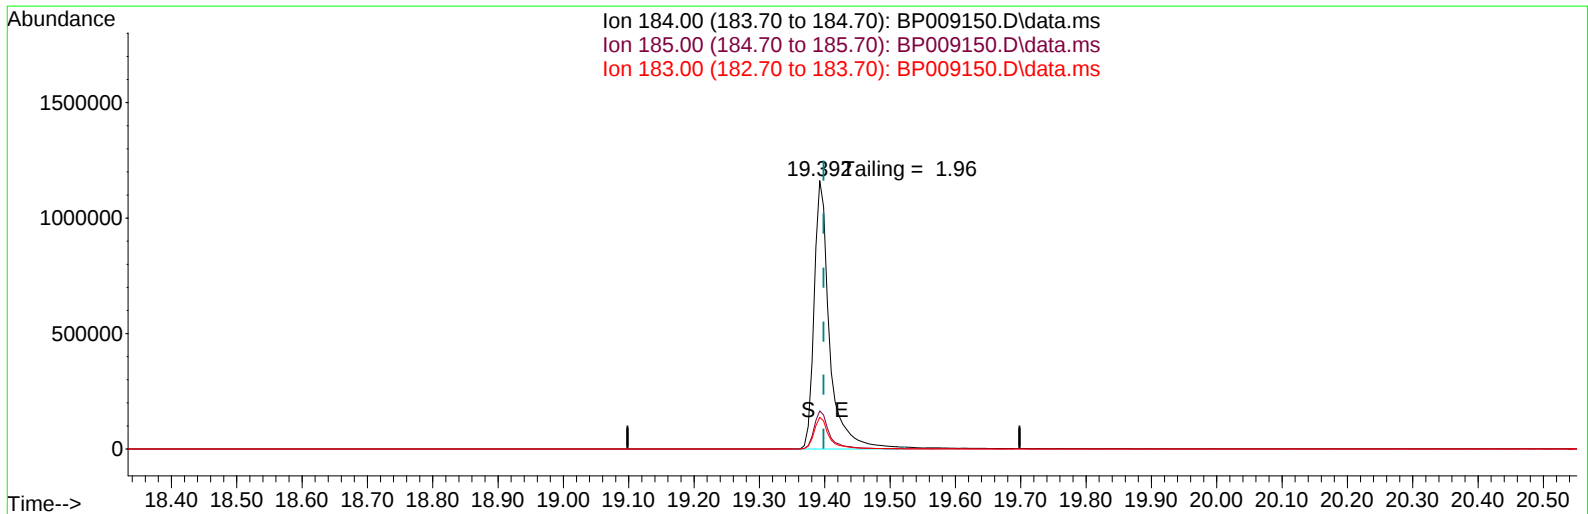

TIC: BP009150.D\data.ms

(77) Benzidine

19.392min (-0.006) 920768.28 ng

response 1924039

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.20
183.00	11.90	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/15/2022	BNA_P	<u>BP009150.D</u>
Compound Name	Response	Retention Time
DDT	1187103	20.592
DDD	18103	20.169
DDE	1638	19.669
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19741	1206844	1.64

Instrument :
BNA_P
ClientSampleId :
DFTPP