

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021524\
 Data File : BP019727.D
 Acq On : 15 Feb 2024 17:28
 Operator : MA/JU
 Sample : P1483-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RT-2327

Quant Time: Feb 15 17:55:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 00:51:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	72386	20.000	ng	-0.01
21) Naphthalene-d8	10.705	136	253574	20.000	ng	-0.01
39) Acenaphthene-d10	14.534	164	160911	20.000	ng	-0.02
64) Phenanthrene-d10	17.292	188	395375	20.000	ng	-0.01
76) Chrysene-d12	21.386	240	451692	20.000	ng	0.00
86) Perylene-d12	23.804	264	509252	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	161608	35.988	ng	-0.01
7) Phenol-d6	7.069	99	195405	32.271	ng	-0.02
23) Nitrobenzene-d5	9.069	82	137047	23.419	ng	-0.02
42) 2,4,6-Tribromophenol	16.034	330	110099	46.862	ng	0.00
45) 2-Fluorobiphenyl	13.163	172	295087	22.671	ng	-0.02
79) Terphenyl-d14	19.857	244	616938	22.462	ng	-0.01
Target Compounds						Qvalue
71) Phenanthrene	17.334	178	99003	4.758	ng	97
72) Anthracene	17.334	178	99003	4.770	ng	98
75) Fluoranthene	19.304	202	174581	6.868	ng	100
78) Pyrene	19.657	202	137008	4.298	ng	100
81) Benzo(a)anthracene	21.422	228	68567	2.156	ng	94
83) Chrysene	21.422	228	68567	2.271	ng	96
88) Benzo(b)fluoranthene	23.069	252	77232	2.406	ng #	94
89) Benzo(k)fluoranthene	23.069	252	77232	2.519	ng #	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021524\
Data File : BP019727.D
Acq On : 15 Feb 2024 17:28
Operator : MA/JU
Sample : P1483-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RT-2327

Quant Time: Feb 15 17:55:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration




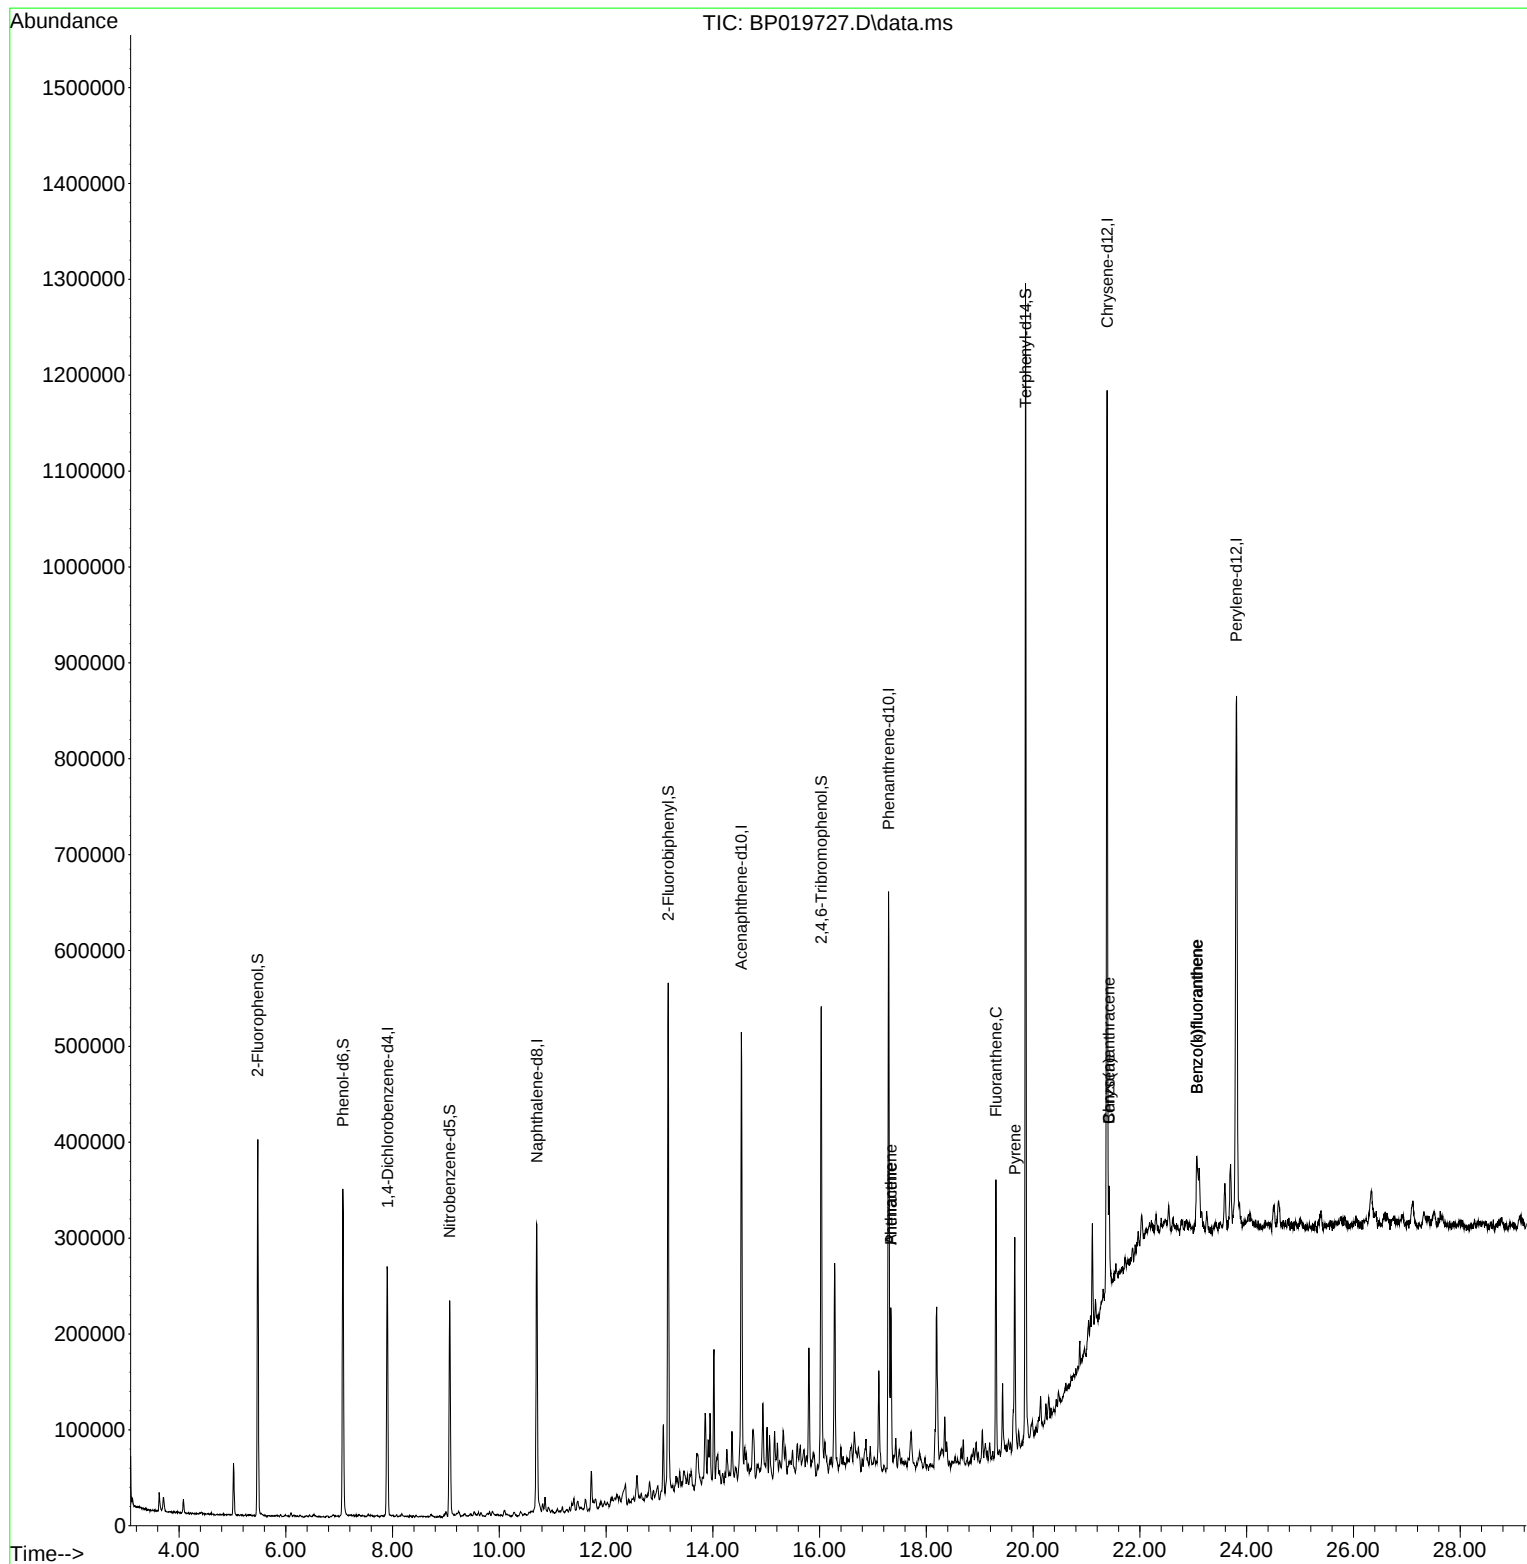




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.905 min Scan# 81
Delta R.T. -0.011 min
Lab File: BP019727.D
Acq: 15 Feb 2024 17:28




Instrument :
BNA_P
ClientSampleId :
RT-2327

Tgt Ion:152 Resp: 72386
Ion Ratio Lower Upper
152 100
150 153.2 121.8 182.8
115 60.5 49.9 74.9

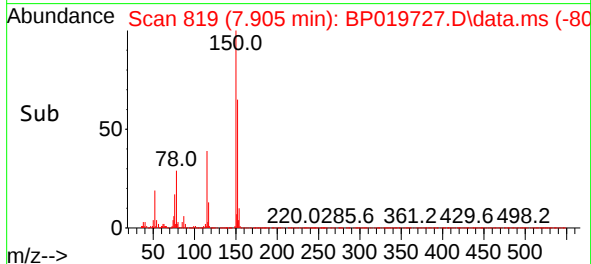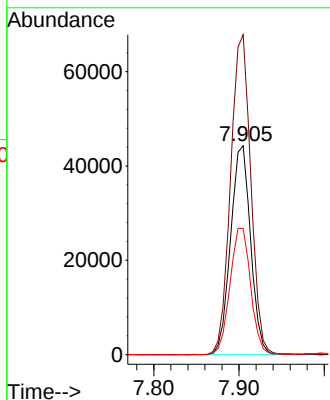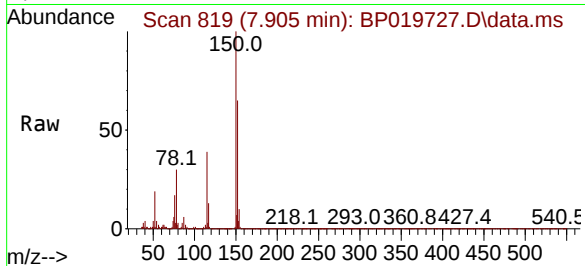

#5
2-Fluorophenol
Concen: 35.988 ng
RT: 5.475 min Scan# 406
Delta R.T. -0.011 min
Lab File: BP019727.D
Acq: 15 Feb 2024 17:28

Tgt Ion:112 Resp: 161608
Ion Ratio Lower Upper
112 100
64 54.2 47.4 71.0
63 30.9 27.0 40.6


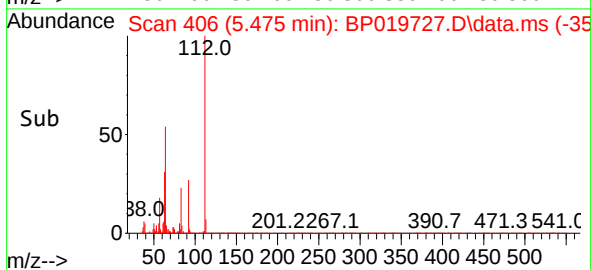
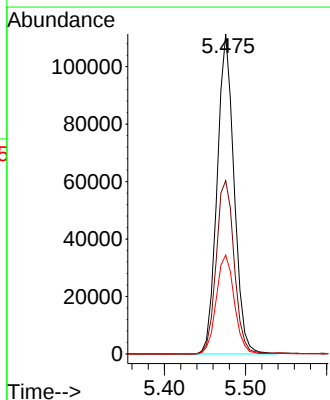
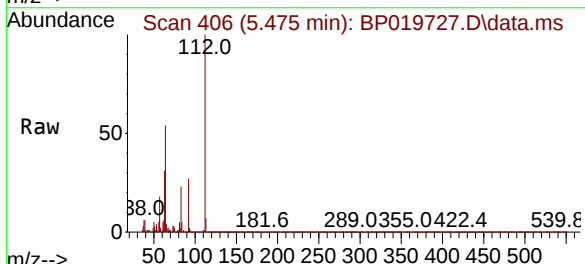




#7
Phenol-d6
Concen: 32.271 ng
RT: 7.069 min Scan# 61
Delta R.T. -0.017 min
Lab File: BP019727.D
Acq: 15 Feb 2024 17:28




Instrument :
BNA_P
ClientSampleId :
RT-2327

Tgt Ion: 99 Resp: 195405
Ion Ratio Lower Upper
99 100
42 18.6 14.7 22.1
71 43.1 34.8 52.2

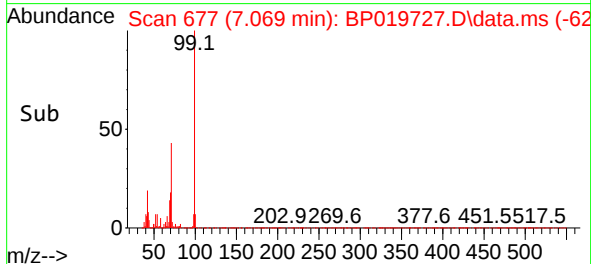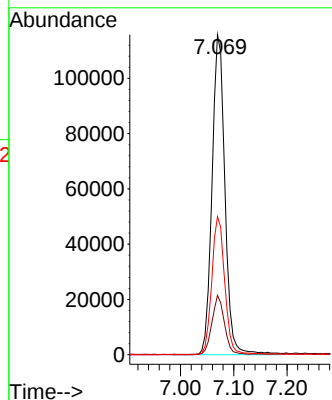

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.705 min Scan# 1295
Delta R.T. -0.011 min
Lab File: BP019727.D
Acq: 15 Feb 2024 17:28

Tgt Ion: 136 Resp: 253574
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 6.6 5.3 7.9
68 4.8 4.1 6.1


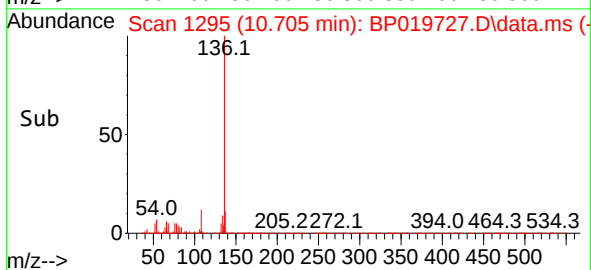
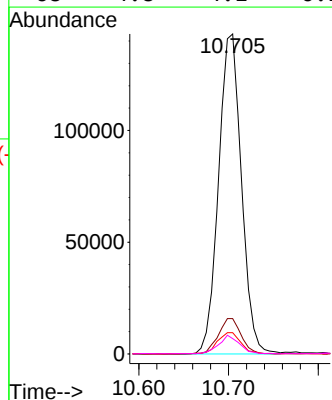
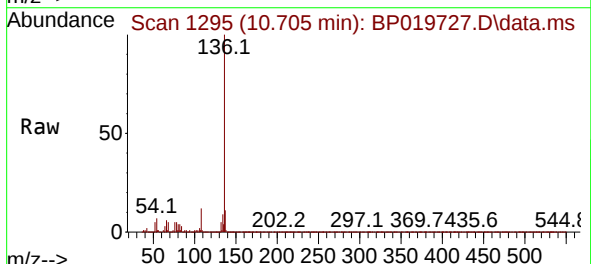




#23
Nitrobenzene-d5
Concen: 23.419 ng
RT: 9.069 min Scan# 1020
Delta R.T. -0.017 min
Lab File: BP019727.D
Acq: 15 Feb 2024 17:28




Instrument :
BNA_P
ClientSampleId :
RT-2327


Tgt Ion: 82 Resp: 137047
Ion Ratio Lower Upper
82 100
128 39.8 29.7 44.5
54 46.9 36.8 55.2

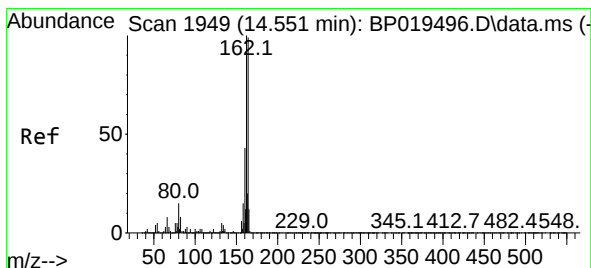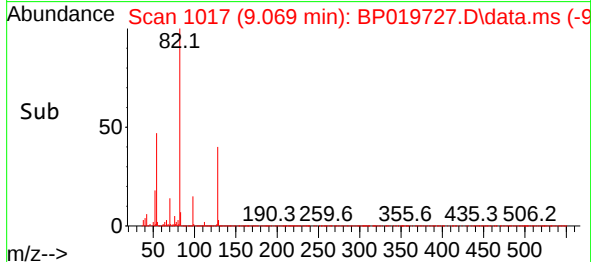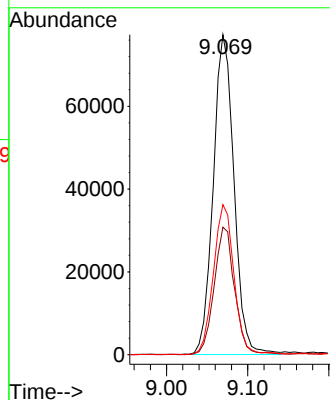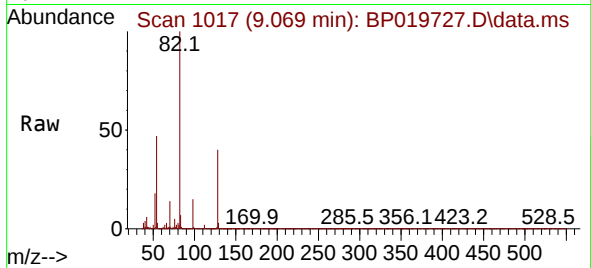

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.534 min Scan# 1946
Delta R.T. -0.017 min
Lab File: BP019727.D
Acq: 15 Feb 2024 17:28

Tgt Ion:164 Resp: 160911
Ion Ratio Lower Upper
164 100
162 104.1 81.2 121.8
160 45.1 35.1 52.7


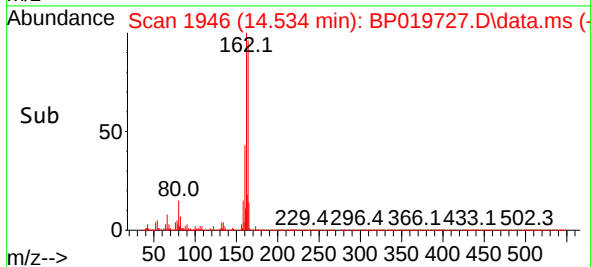
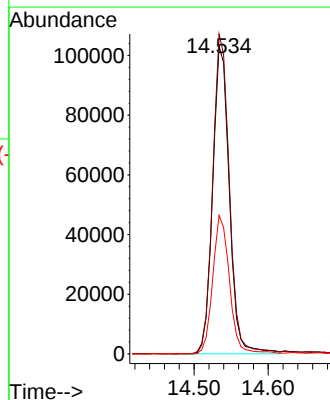
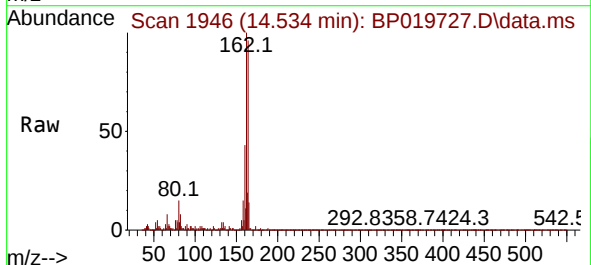




#42
2,4,6-Tribromophenol
Concen: 46.862 ng
RT: 16.034 min Scan# 21
Delta R.T. -0.005 min
Lab File: BP019727.D
Acq: 15 Feb 2024 17:28




Instrument :
BNA_P
ClientSampleId :
RT-2327


Tgt Ion:330 Resp: 110099
Ion Ratio Lower Upper
330 100
332 95.5 77.2 115.8
141 29.8 27.0 40.4

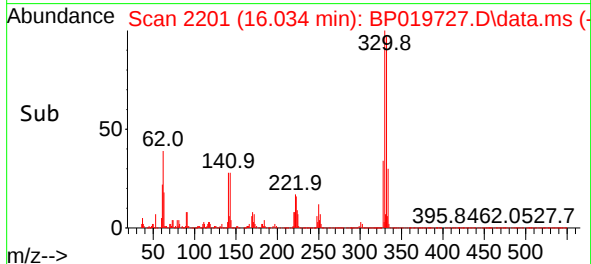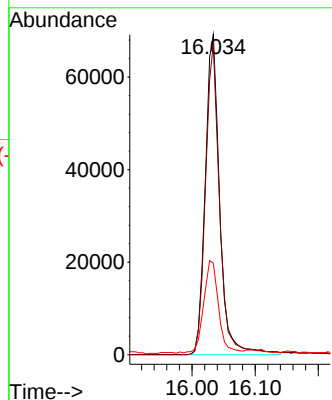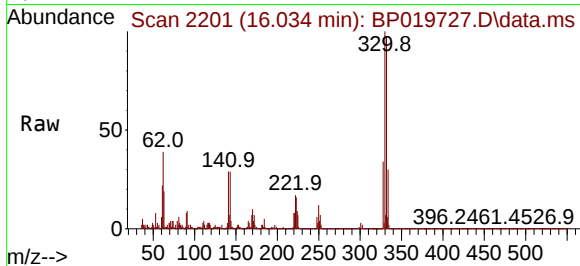

#45
2-Fluorobiphenyl
Concen: 22.671 ng
RT: 13.163 min Scan# 1713
Delta R.T. -0.017 min
Lab File: BP019727.D
Acq: 15 Feb 2024 17:28

Tgt Ion:172 Resp: 295087
Ion Ratio Lower Upper
172 100
171 34.3 28.2 42.4
170 22.8 18.9 28.3

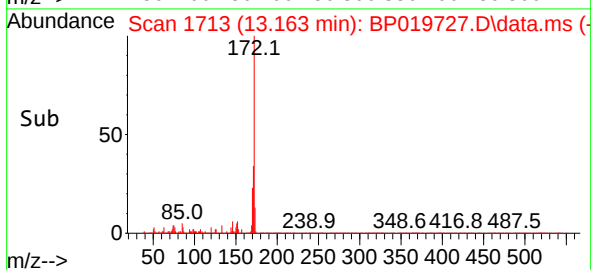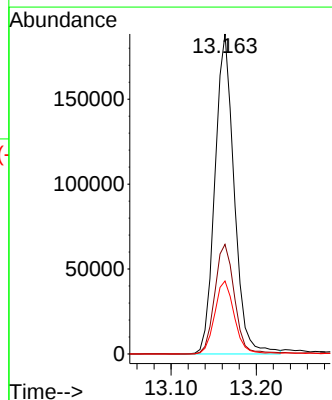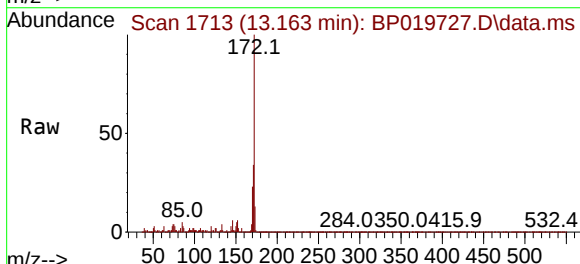

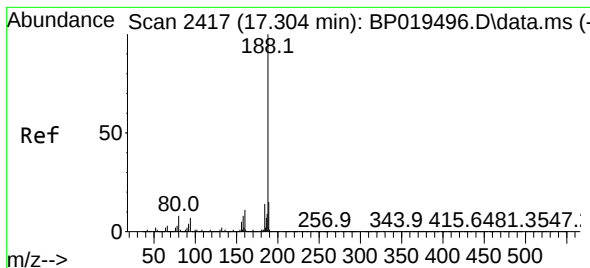

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.292 min Scan# 2415

Delta R.T. -0.012 min

Lab File: BP019727.D

Acq: 15 Feb 2024 17:28

Instrument :

BNA_P

ClientSampleId :

RT-2327





Tgt Ion:188 Resp: 395375

Ion Ratio Lower Upper

188 100

94 6.6 5.4 8.2

80 7.1 6.3 9.5

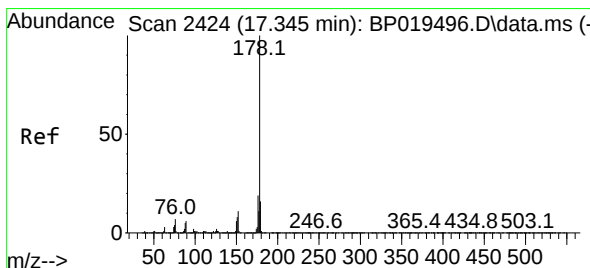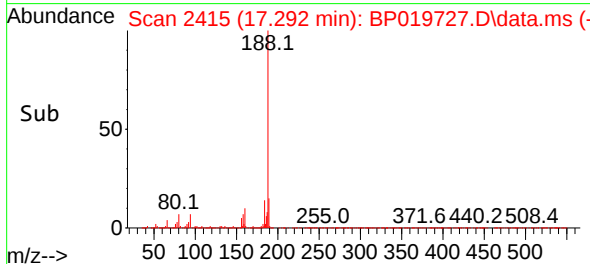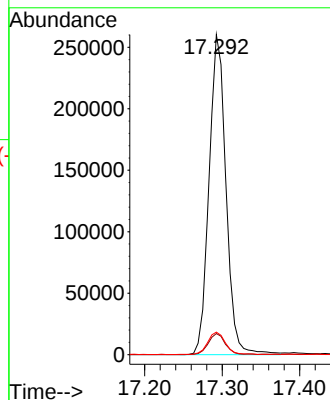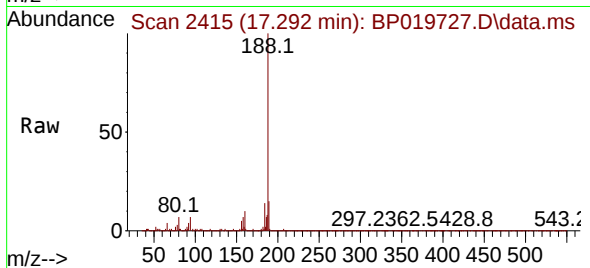

#71

Phenanthrene

Concen: 4.758 ng

RT: 17.334 min Scan# 2422

Delta R.T. -0.011 min

Lab File: BP019727.D

Acq: 15 Feb 2024 17:28




Tgt Ion:178 Resp: 99003


Ion Ratio Lower Upper

178 100

176 18.6 15.5 23.3

179 17.3 12.6 19.0

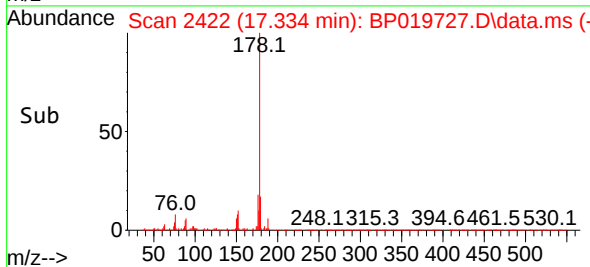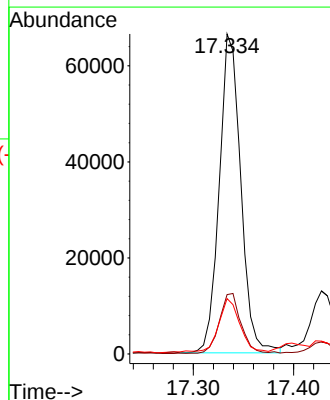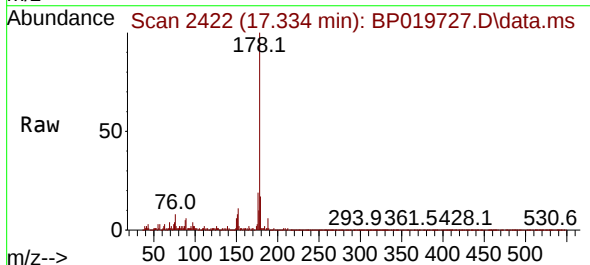

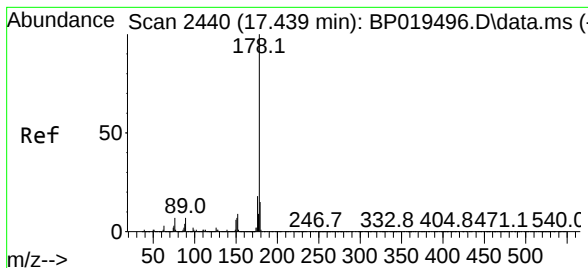

#72

Anthracene

Concen: 4.770 ng

RT: 17.334 min Scan# 2440

Delta R.T. -0.105 min

Lab File: BP019727.D

Acq: 15 Feb 2024 17:28

Instrument :

BNA_P

ClientSampleId :

RT-2327





Tgt Ion:178 Resp: 99003

Ion Ratio Lower Upper

178 100

176 18.6 14.7 22.1

179 17.3 12.2 18.2

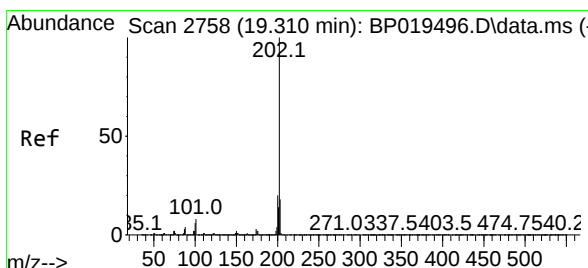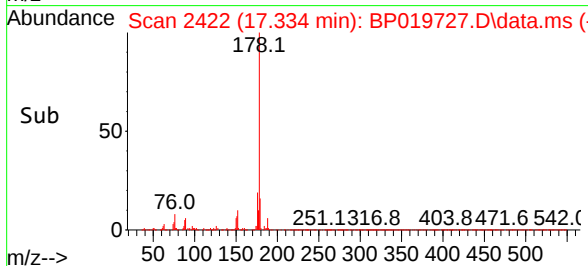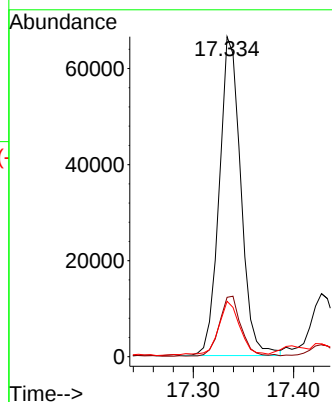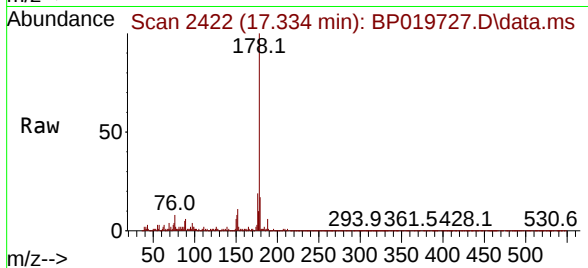

#75

Fluoranthene

Concen: 6.868 ng

RT: 19.304 min Scan# 2757

Delta R.T. -0.005 min

Lab File: BP019727.D

Acq: 15 Feb 2024 17:28




Tgt Ion:202 Resp: 174581


Ion Ratio Lower Upper

202 100

101 7.7 0.0 27.7

203 17.5 0.0 37.5

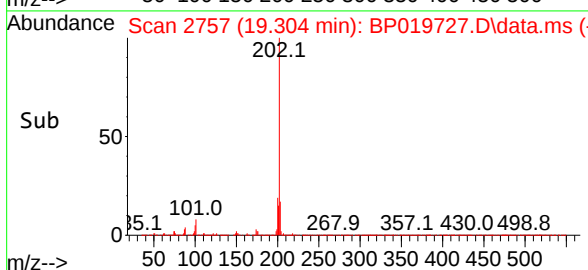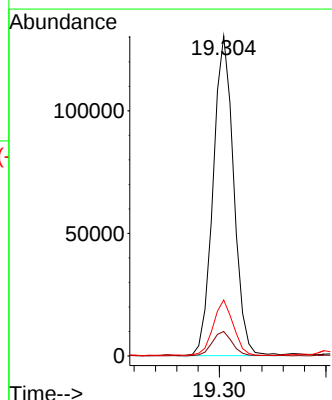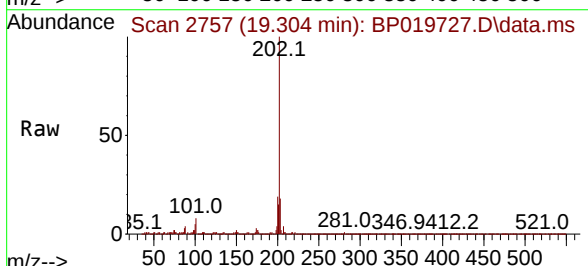

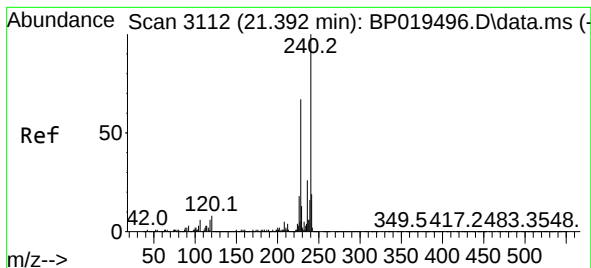

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.386 min Scan# 3111

Delta R.T. -0.005 min

Lab File: BP019727.D

Acq: 15 Feb 2024 17:28

Instrument :

BNA_P

ClientSampleId :

RT-2327





Tgt Ion:240 Resp: 451692

Ion Ratio Lower Upper

240 100

120 6.1 6.1 9.1

236 25.9 20.7 31.1

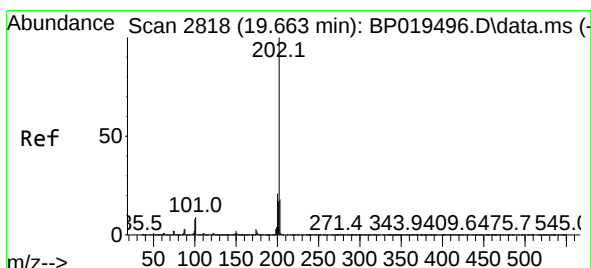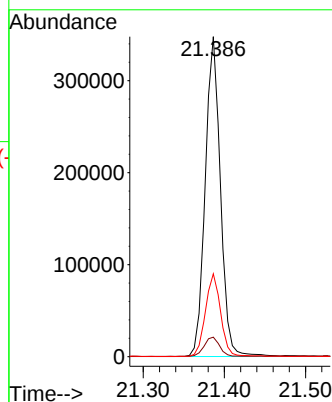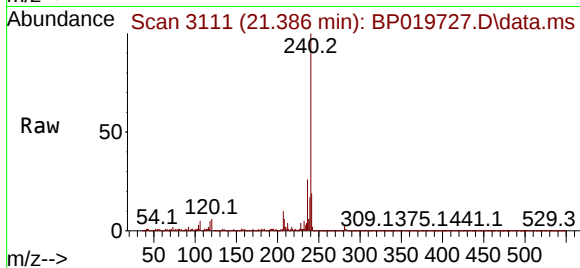

#78

Pyrene

Concen: 4.298 ng

RT: 19.657 min Scan# 2817

Delta R.T. -0.005 min

Lab File: BP019727.D

Acq: 15 Feb 2024 17:28




Tgt Ion:202 Resp: 137008


Ion Ratio Lower Upper

202 100

200 21.1 16.9 25.3

203 17.3 14.2 21.2


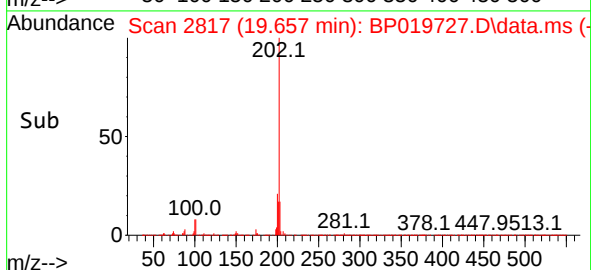
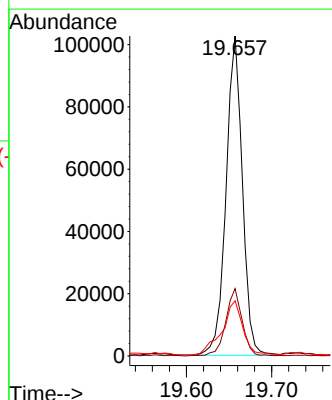
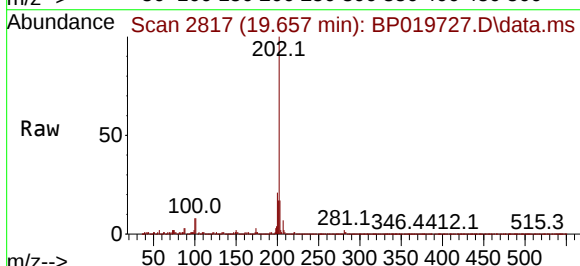




#79
 Terphenyl-d14
 Concen: 22.462 ng
 RT: 19.857 min Scan# 21
 Delta R.T. -0.011 min
 Lab File: BP019727.D
 Acq: 15 Feb 2024 17:28




Instrument :
 BNA_P
 ClientSampleId :
 RT-2327


Tgt Ion:244 Resp: 616938
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.1 9.1
 122 7.1 5.9 8.9

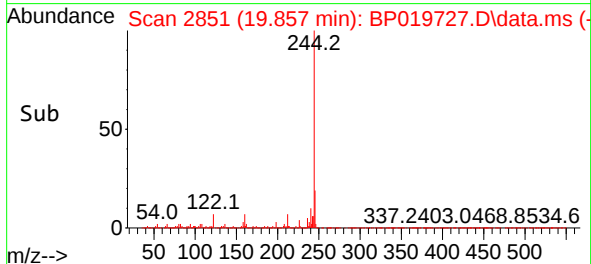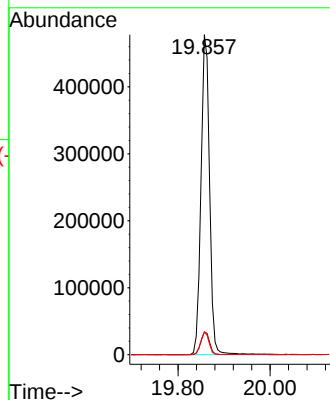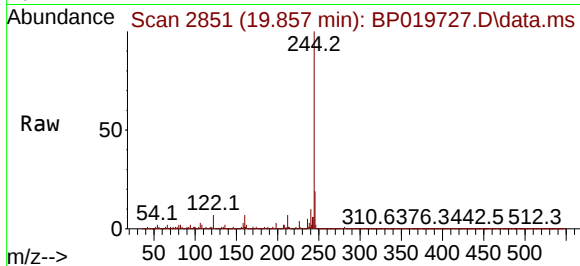

#81
 Benzo(a)anthracene
 Concen: 2.156 ng
 RT: 21.422 min Scan# 3117
 Delta R.T. 0.042 min
 Lab File: BP019727.D
 Acq: 15 Feb 2024 17:28

Tgt Ion:228 Resp: 68567
 Ion Ratio Lower Upper
 228 100
 226 29.9 21.7 32.5
 229 23.0 15.6 23.4

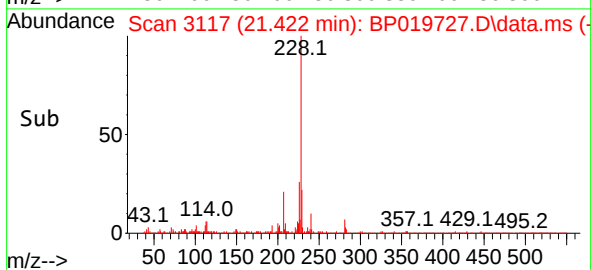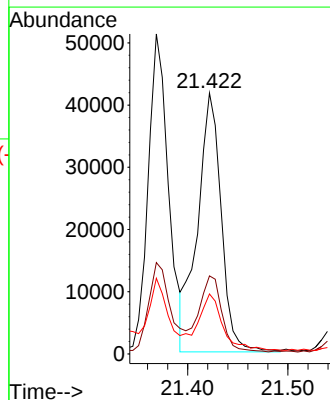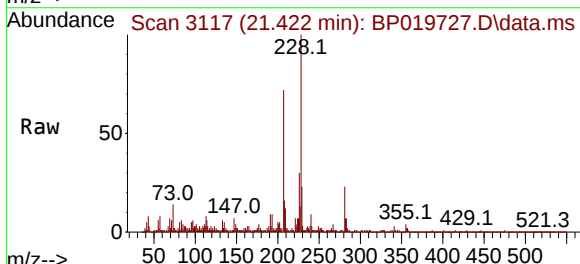

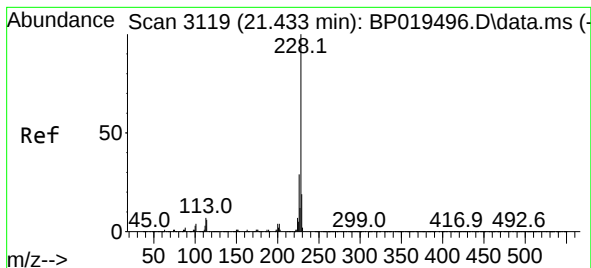

#83

Chrysene

Concen: 2.271 ng

RT: 21.422 min Scan# 3119

Delta R.T. -0.011 min

Lab File: BP019727.D

Acq: 15 Feb 2024 17:28

Instrument :

BNA_P

ClientSampleId :

RT-2327





Tgt Ion:228 Resp: 68567

Ion Ratio Lower Upper

228 100

226 29.9 23.4 35.2

229 23.0 15.6 23.4

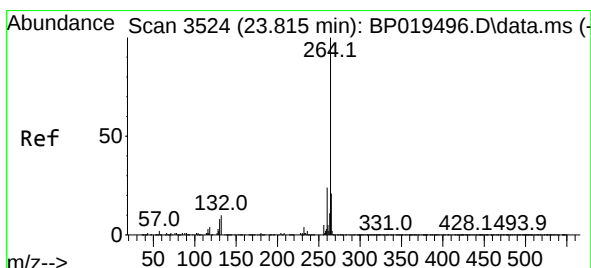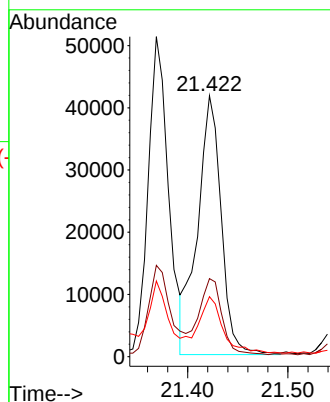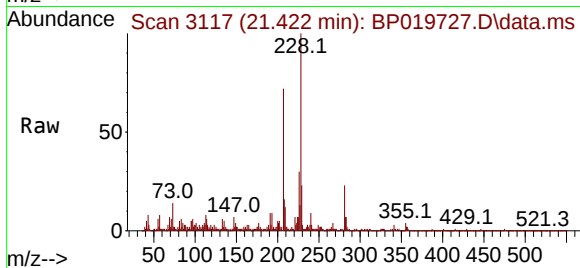

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.804 min Scan# 3522

Delta R.T. -0.011 min

Lab File: BP019727.D

Acq: 15 Feb 2024 17:28




Tgt Ion:264 Resp: 509252


Ion Ratio Lower Upper

264 100

260 23.3 19.2 28.8

265 21.8 17.0 25.4


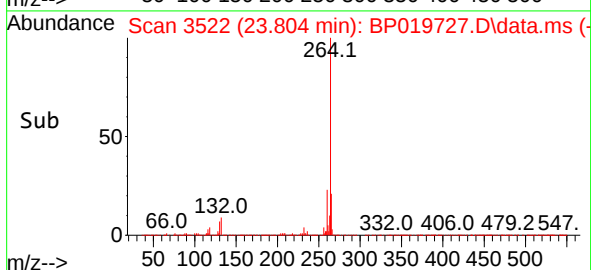
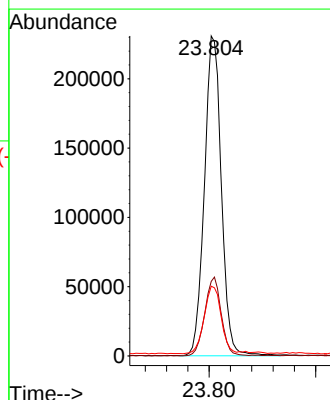
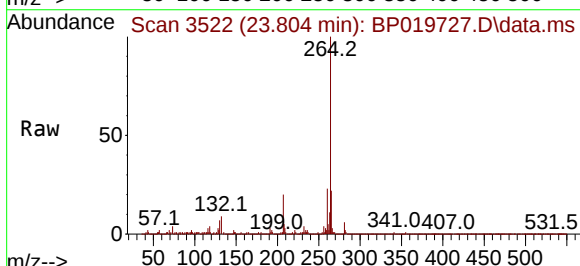




#88
Benzo(b)fluoranthene
Concen: 2.406 ng
RT: 23.069 min Scan# 3397
Delta R.T. -0.011 min
Lab File: BP019727.D
Acq: 15 Feb 2024 17:28

Instrument :
BNA_P
ClientSampleId :
RT-2327

Tgt Ion:252 Resp: 77232
Ion Ratio Lower Upper
252 100
253 23.7 17.3 25.9
125 9.5 4.9 7.3#

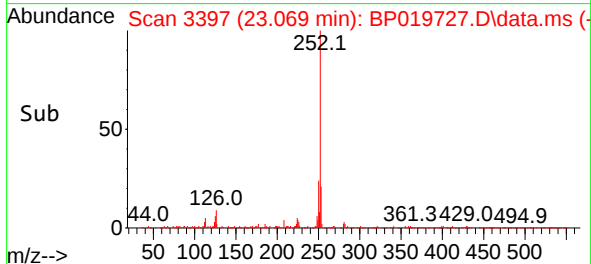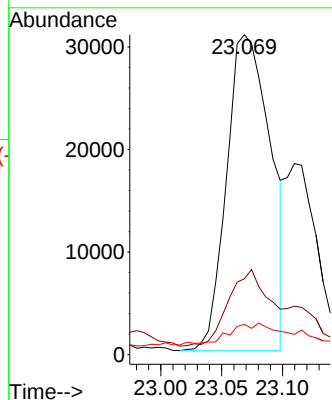

#89
Benzo(k)fluoranthene
Concen: 2.519 ng
RT: 23.069 min Scan# 3397
Delta R.T. -0.058 min
Lab File: BP019727.D
Acq: 15 Feb 2024 17:28

Tgt Ion:252 Resp: 77232
Ion Ratio Lower Upper
252 100
253 23.7 17.1 25.7
125 9.5 5.0 7.6#

