
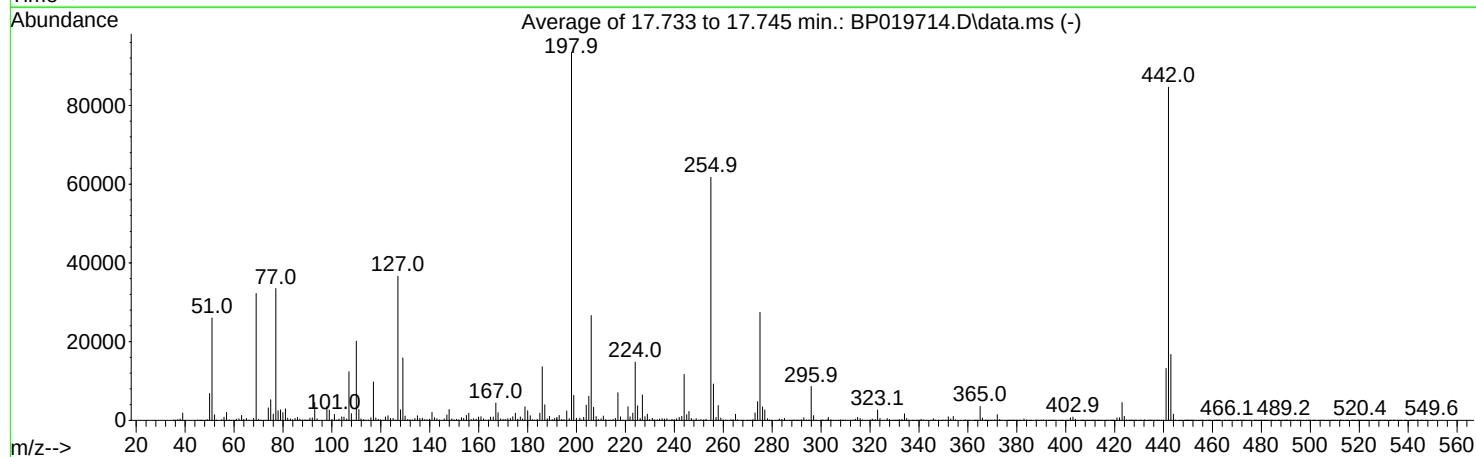


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021524\
Data File : BP019714.D
Acq On : 15 Feb 2024 10:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

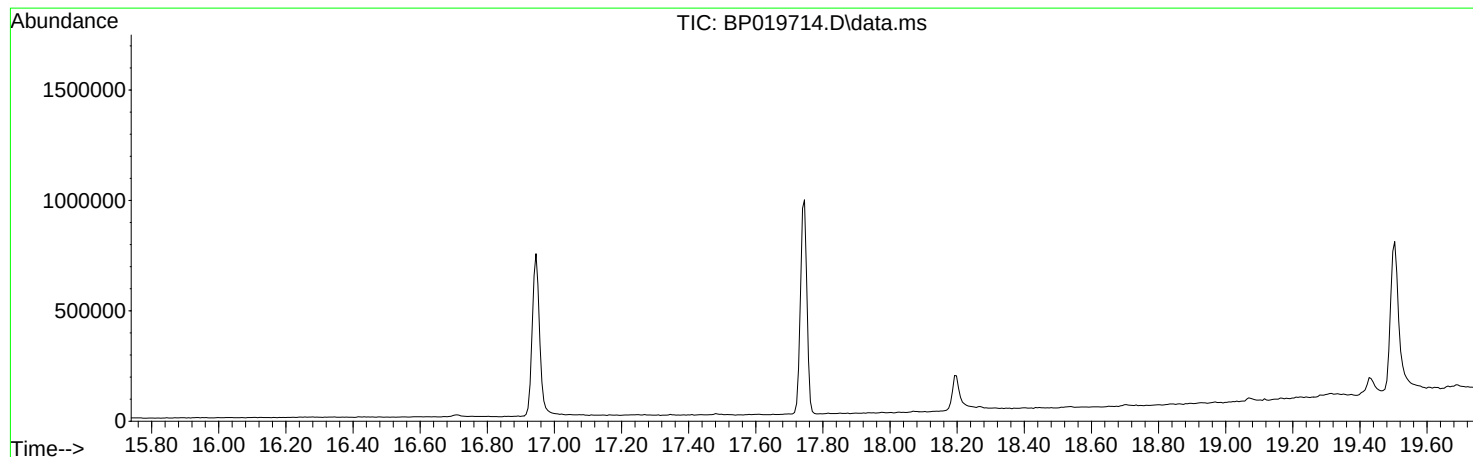




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	26012	PASS
68	69	0.00	2	1.6	506	PASS
69	198	0.00	100	34.5	32232	PASS
70	69	0.00	2	0.9	282	PASS
127	198	10	80	39.2	36637	PASS
197	198	0.00	2	0.5	441	PASS
198	198	100	100	100.0	93432	PASS
199	198	5	9	6.8	6330	PASS
275	198	10	60	29.4	27455	PASS
365	198	1	100	3.8	3544	PASS
441	198	0.01	100	14.1	13217	PASS
442	442	100	100	100.0	84600	PASS
443	442	15	24	19.8	16753	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021524\
Data File : BP019714.D
Acq On : 15 Feb 2024 10:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 16 02:45:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

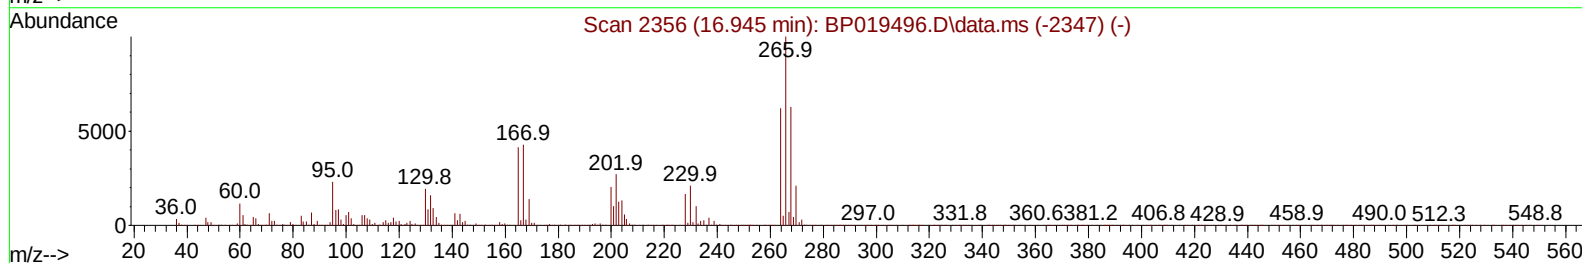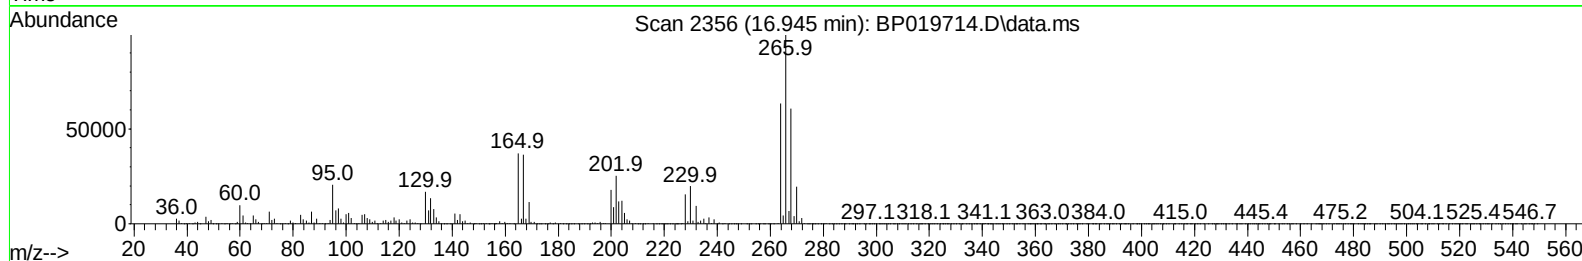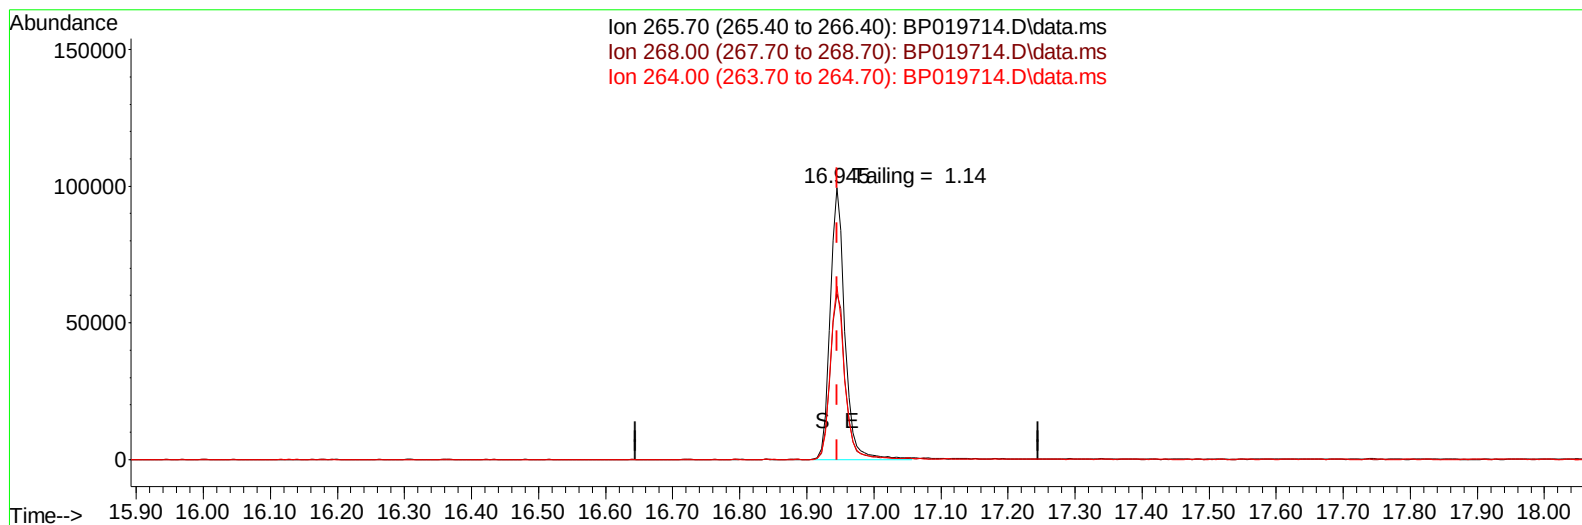

TIC: BP019714.D\data.ms

(70) Pentachlorophenol (C)

16.945min (+ 0.000) 210221.37 ng m




response 152893

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	61.06
264.00	62.10	63.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021524\
Data File : BP019714.D
Acq On : 15 Feb 2024 10:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 16 02:45:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

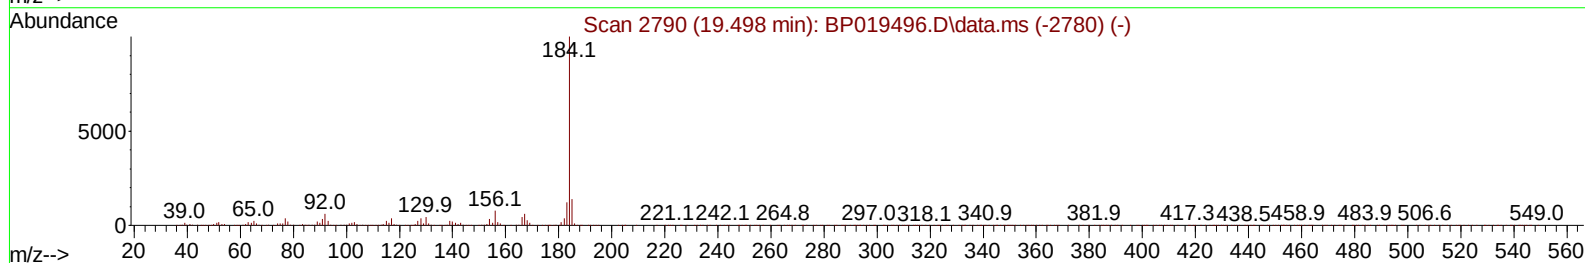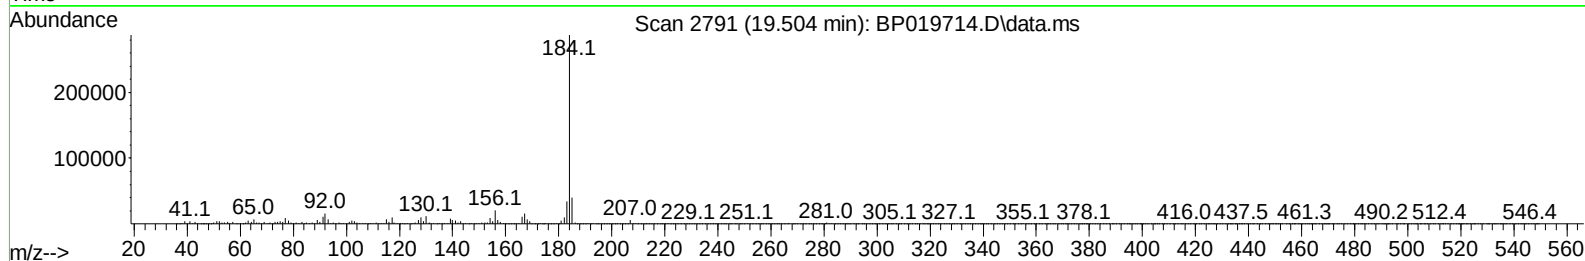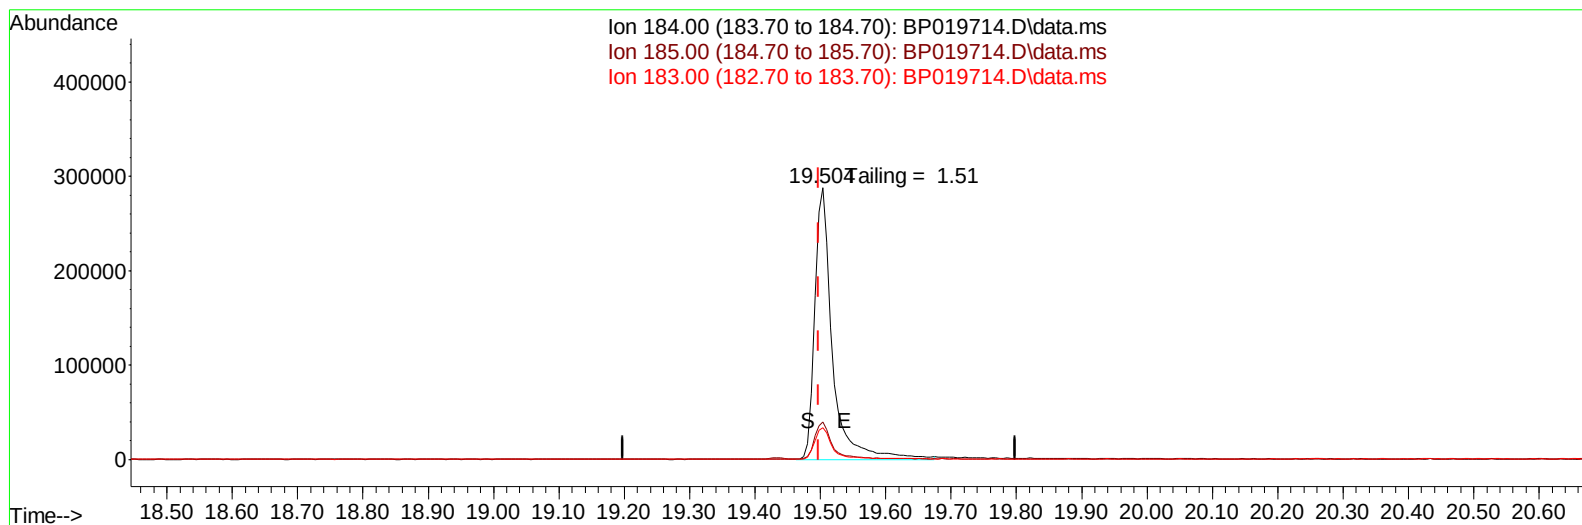

TIC: BP019714.D\data.ms

(77) Benzidine

19.504min (+ 0.006) 63359.26 ng

response 539125

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.86
183.00	12.10	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/15/2024	BNA_P	<u>BP019714.D</u>
Compound Name	Response	Retention Time
DDT	349931	20.698
DDD	15301	20.268
DDE	1117	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16418	366349	4.48

Instrument :
BNA_P
ClientSampleId :
DFTPP