
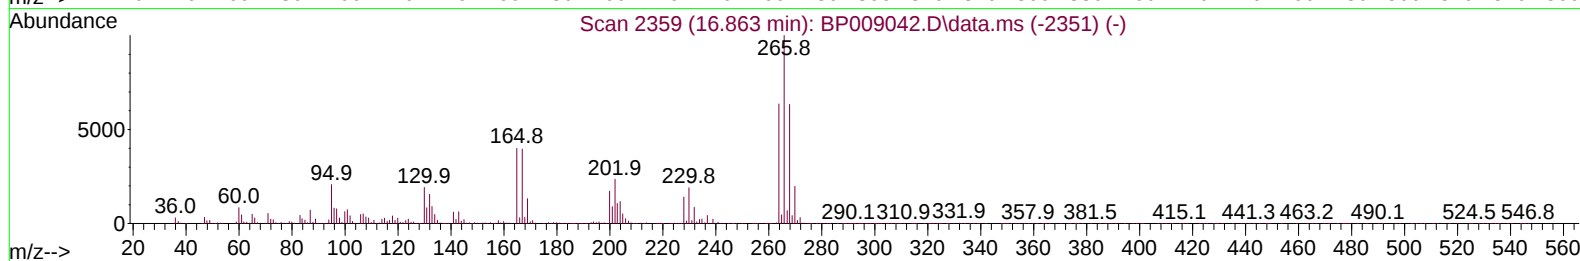
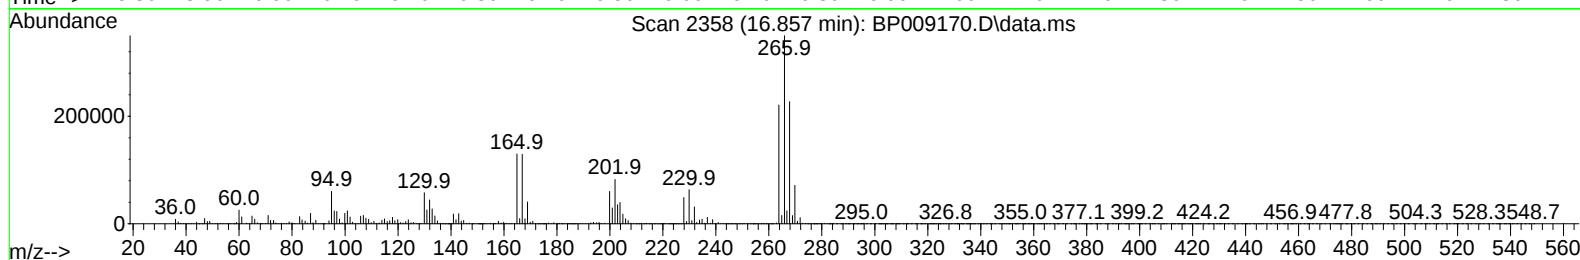


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
Data File : BP009170.D
Acq On : 16 Feb 2022 09:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 14:26:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 01:29:44 2022
Response via : Initial Calibration

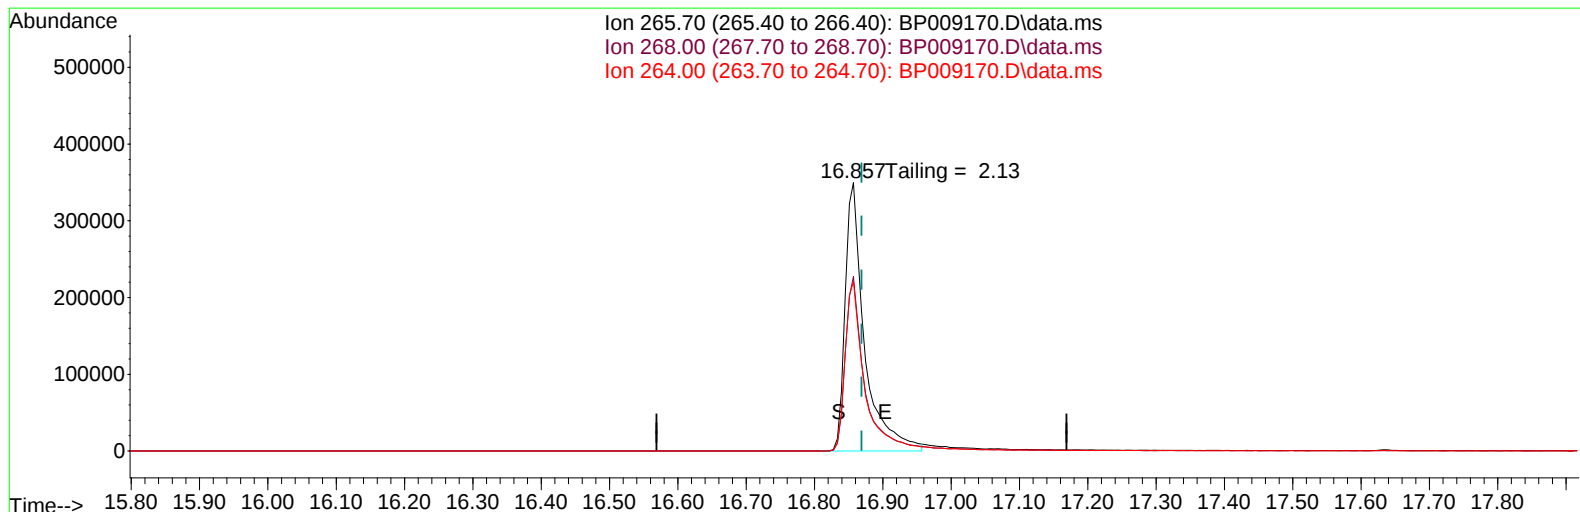

TIC: BP009170.D\data.ms

(70) Pentachlorophenol (C)




16.857min (-0.012) 2709870.60 ng

response 648259

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.98
264.00	62.90	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
 Data File : BP009170.D
 Acq On : 16 Feb 2022 09:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 14:26:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 16 01:29:44 2022
 Response via : Initial Calibration

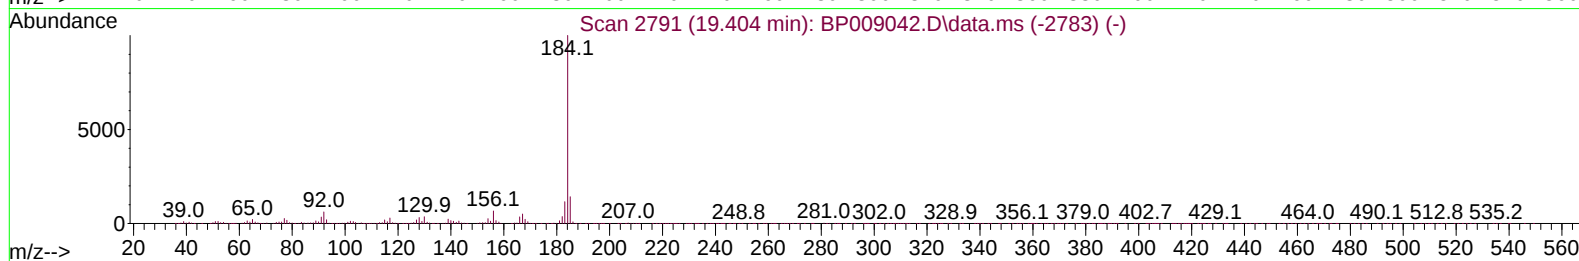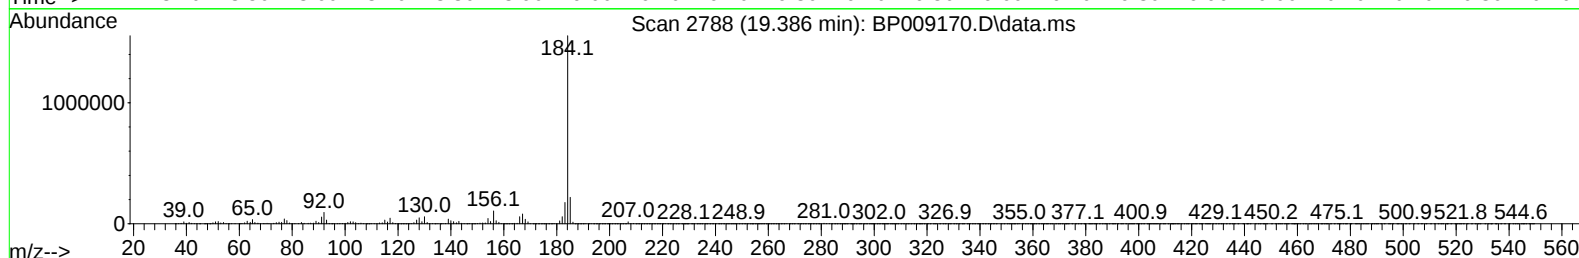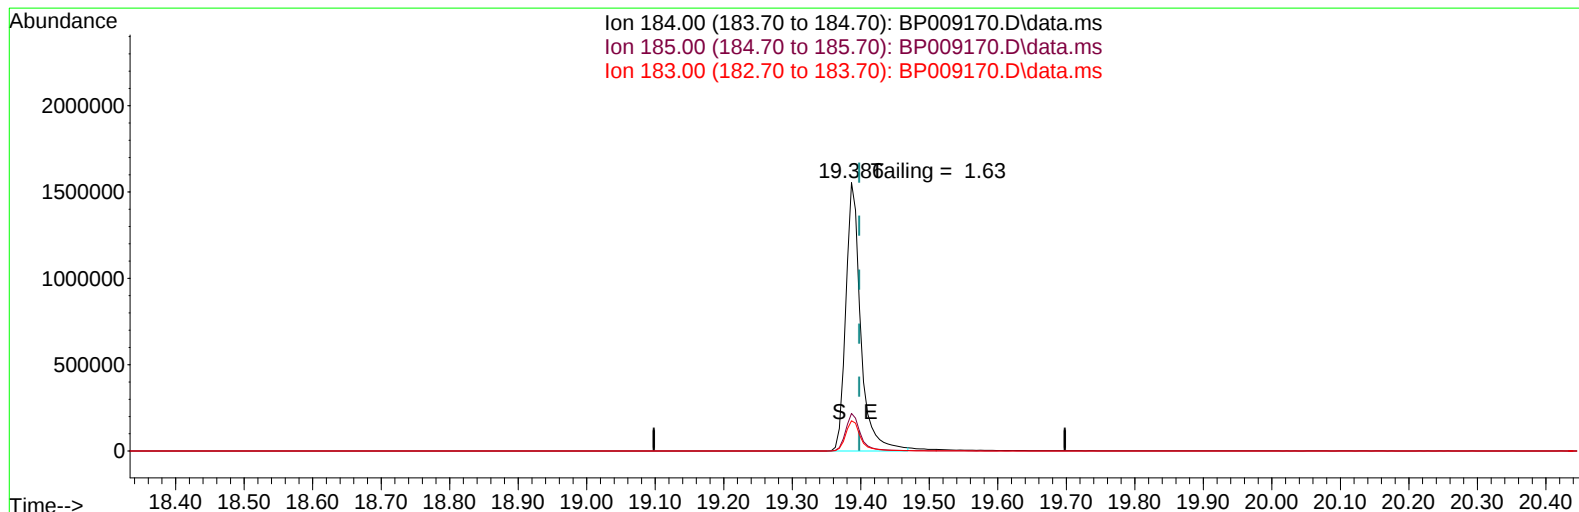

TIC: BP009170.D\data.ms

(77) Benzidine**19.386min (-0.012) 878172.77 ng****response 2165337**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.05
183.00	11.90	11.30
0.00	0.00	0.00