

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
 Data File : BP009172.D
 Acq On : 16 Feb 2022 11:11
 Operator : CG/JU
 Sample : PB142581BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142581BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	400	407	430	rBV	2719162	4719231	27.31%	7.524%
2	6.975	671	678	707	rBV	2544276	4940734	28.59%	7.877%
3	7.781	807	815	830	rBV	612210	1068454	6.18%	1.704%
4	8.946	1005	1013	1040	rBV	1664124	3260702	18.87%	5.199%
5	10.581	1283	1291	1313	rBV	697490	1476827	8.54%	2.355%
6	13.046	1703	1710	1741	rBV	5527647	9048854	52.36%	14.427%
7	14.428	1937	1945	1966	rBV	1356302	2274632	13.16%	3.627%
8	15.928	2192	2200	2235	rBV	4394604	7799771	45.13%	12.436%
9	17.186	2408	2414	2432	rBV	1820890	3032817	17.55%	4.835%
10	19.751	2844	2850	2862	rBV	13161515	17283046	100.00%	27.555%
11	21.286	3105	3111	3123	rBV	2610846	3882718	22.47%	6.190%
12	23.674	3510	3517	3528	rVB2	1781611	3933099	22.76%	6.271%




Sum of corrected areas: 62720885

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
Data File : BP009172.D
Acq On : 16 Feb 2022 11:11
Operator : CG/JU
Sample : PB142581BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142581BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

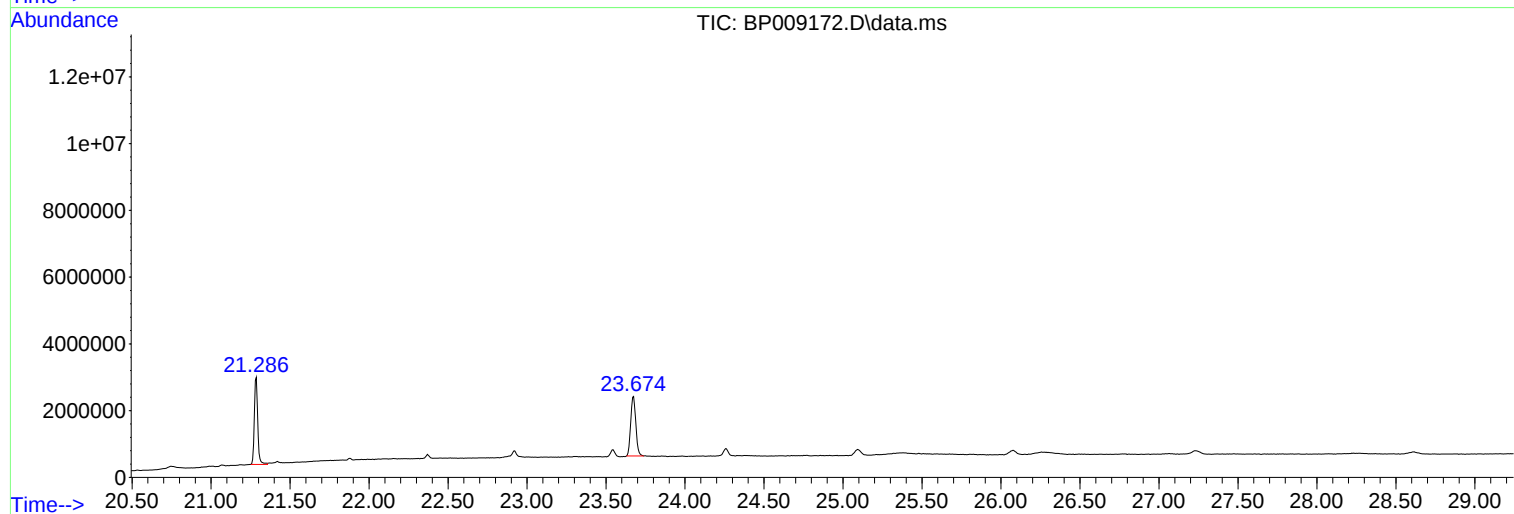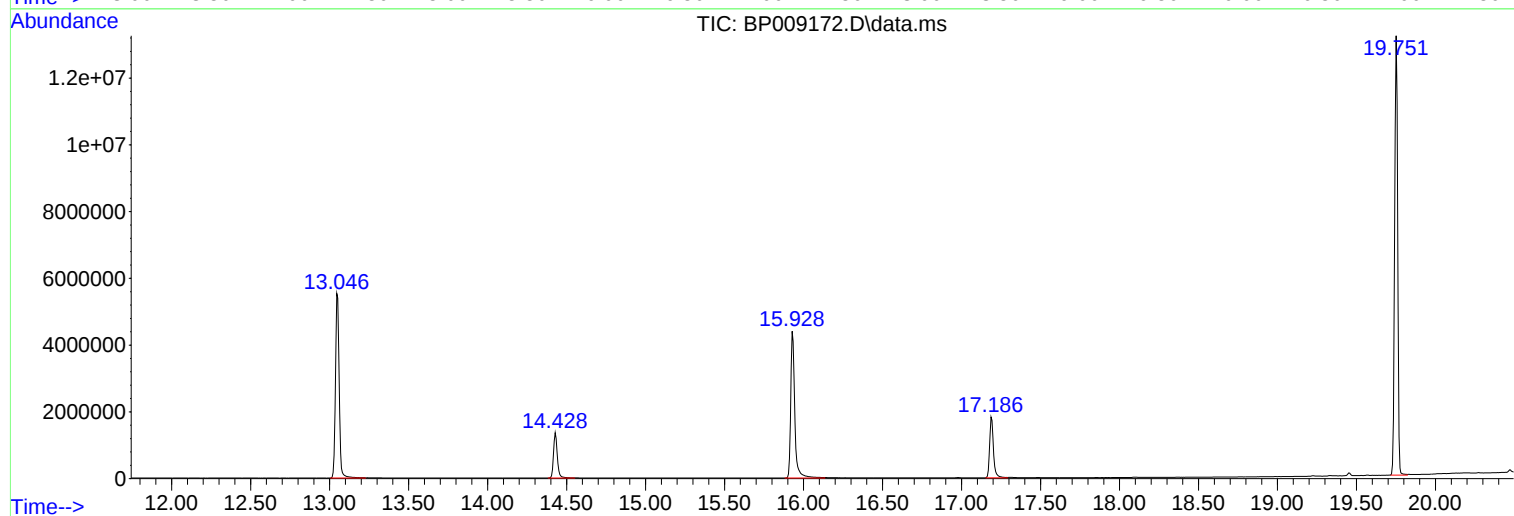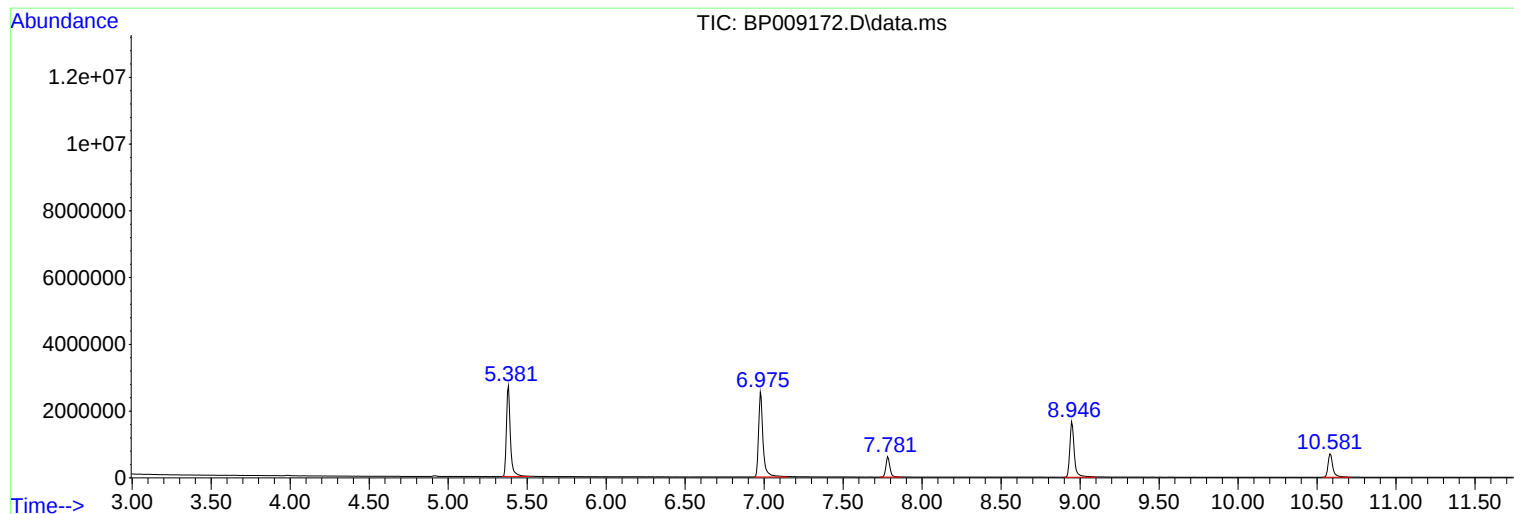

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
Data File : BP009172.D
Acq On : 16 Feb 2022 11:11
Operator : CG/JU
Sample : PB142581BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142581BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
Data File : BP009172.D
Acq On : 16 Feb 2022 11:11
Operator : CG/JU
Sample : PB142581BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142581BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------