

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
 Data File : BP009173.D
 Acq On : 16 Feb 2022 11:46
 Operator : CG/JU
 Sample : PB142605BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142605BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	401	407	434	rBV	3043510	5263771	28.74%	7.850%
2	6.975	671	678	712	rBV	2805823	5472608	29.88%	8.162%
3	7.781	808	815	833	rBV	626784	1146802	6.26%	1.710%
4	8.951	1006	1014	1042	rBV	1761280	3529694	19.27%	5.264%
5	10.581	1284	1291	1314	rBV	735655	1593185	8.70%	2.376%
6	13.051	1703	1711	1739	rBV	6051824	9809707	53.56%	14.630%
7	14.428	1938	1945	1970	rBV	1372959	2455465	13.41%	3.662%
8	15.933	2193	2201	2230	rBV	4613328	8308962	45.36%	12.391%
9	17.192	2408	2415	2431	rBV	1872974	3230889	17.64%	4.818%
10	19.751	2844	2850	2866	rBV	13304933	18316498	100.00%	27.316%
11	21.286	3106	3111	3121	rBV	2828288	3929549	21.45%	5.860%
12	23.674	3510	3517	3533	rVB2	1830505	3996651	21.82%	5.960%




Sum of corrected areas: 67053781

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
Data File : BP009173.D
Acq On : 16 Feb 2022 11:46
Operator : CG/JU
Sample : PB142605BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142605BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

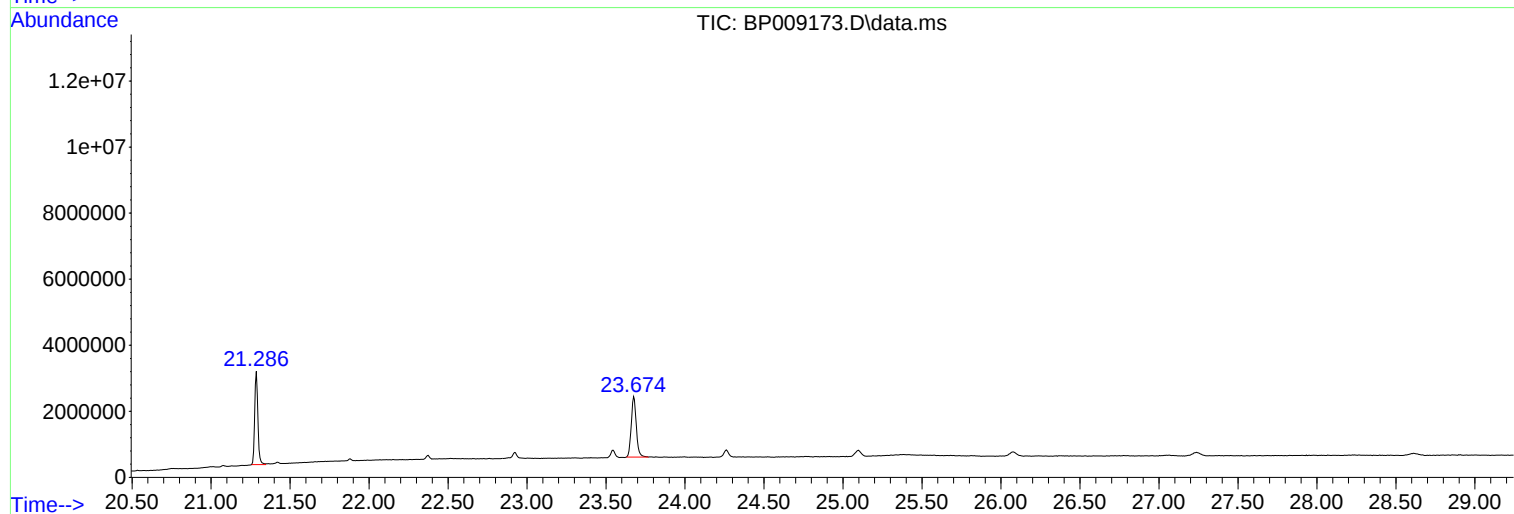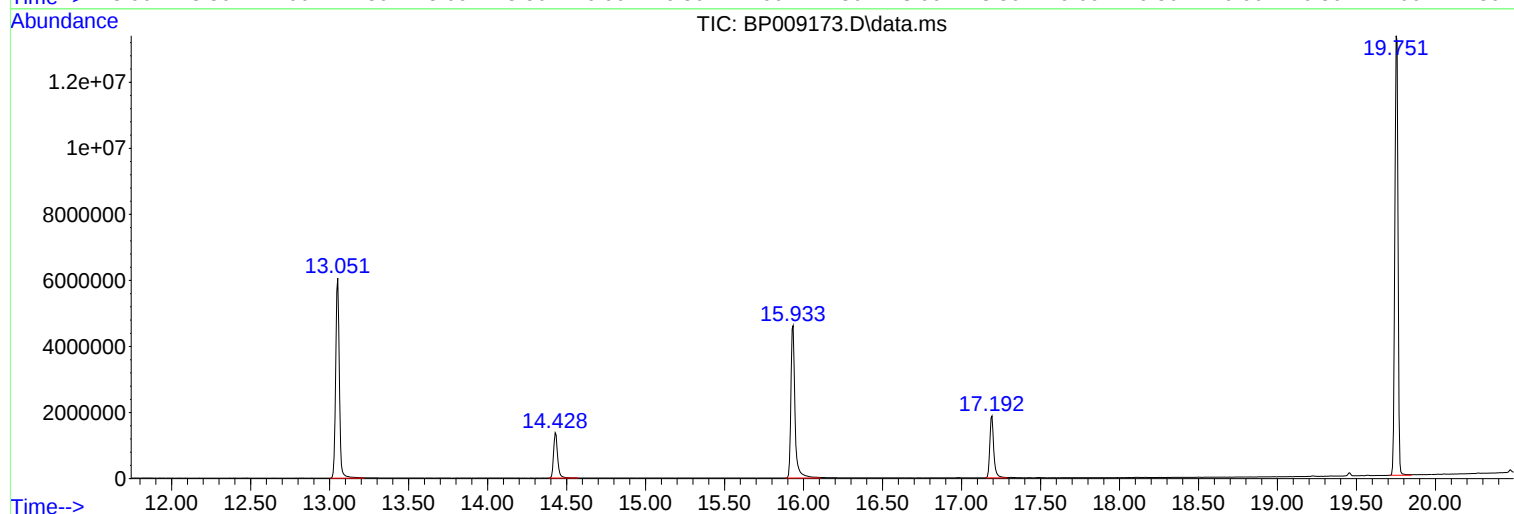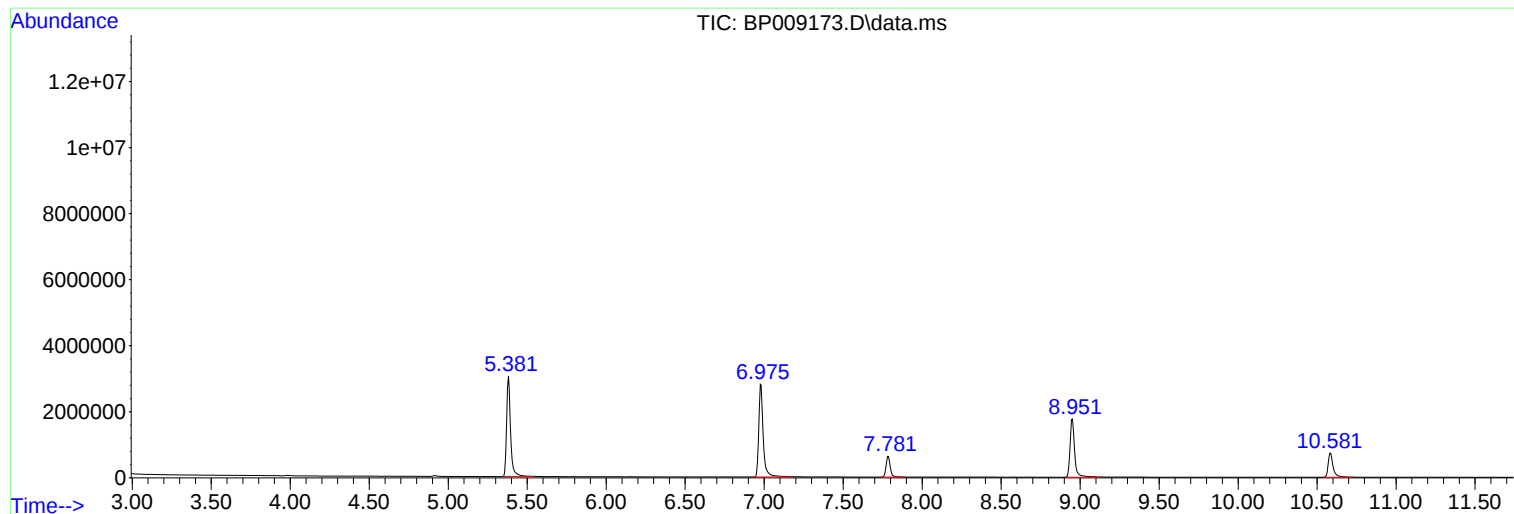

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
Data File : BP009173.D
Acq On : 16 Feb 2022 11:46
Operator : CG/JU
Sample : PB142605BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142605BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
Data File : BP009173.D
Acq On : 16 Feb 2022 11:46
Operator : CG/JU
Sample : PB142605BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142605BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------